


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120817\
 Data File : BF101234.D
 Acq On : 8 Dec 2017 13:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 08 18:17:31 2017

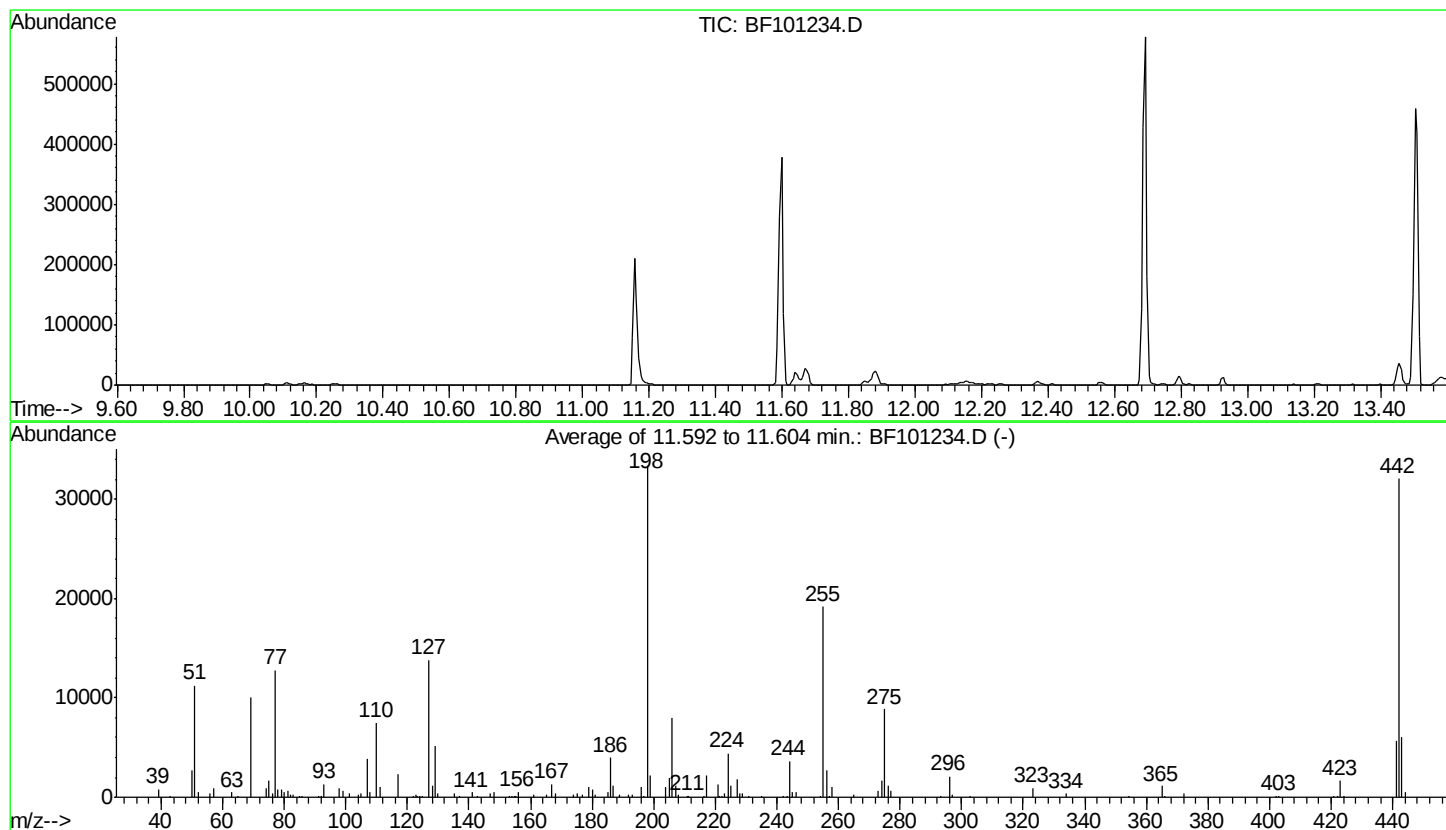

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	11274	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.2	10070	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.5	13855	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33398	PASS
199	198	5	9	6.5	2163	PASS
275	198	10	60	26.5	8846	PASS
365	198	1	100	3.4	1152	PASS
441	443	0.01	100	92.5	5652	PASS
442	198	50	100	96.1	32085	PASS
443	442	15	24	19.0	6109	PASS