


Data Path : Z:\HPCHEM1\BNA F\Data\BF120817\
 Data File : BF101259.D
 Acq On : 9 Dec 2017 2:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 08 18:17:31 2017

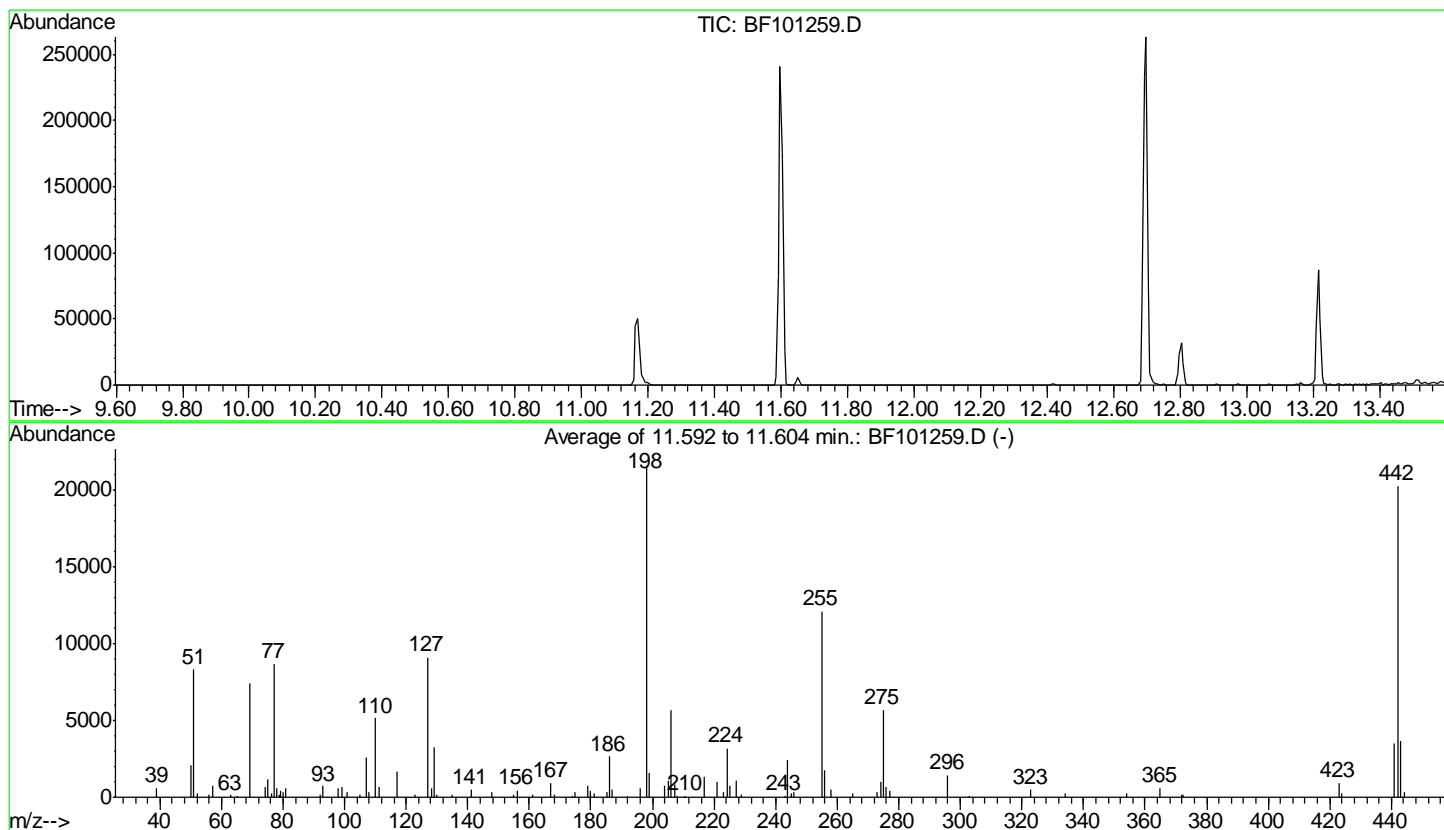

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	8335	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.2	7391	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.2	9122	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21623	PASS
199	198	5	9	7.3	1589	PASS
275	198	10	60	26.3	5681	PASS
365	198	1	100	2.8	600	PASS
441	443	0.01	100	95.1	3485	PASS
442	198	50	100	93.9	20310	PASS
443	442	15	24	18.1	3666	PASS