

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120820\
Data File : BF122586.D
Acq On : 8 Dec 2020 13:38
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	570	576	579	rBV	5492260	7418577	73.77%	13.238%
2	6.481	740	747	750	rBV	5467179	7421284	73.79%	13.243%
3	6.840	804	808	811	rBV	1576221	1253079	12.46%	2.236%
4	7.404	898	904	907	rBV	3881062	5135791	51.07%	9.164%
5	8.122	1021	1026	1035	rBV	1858698	1709640	17.00%	3.051%
6	9.204	1203	1210	1213	rBV	7462222	8867363	88.17%	15.823%
7	9.875	1319	1324	1328	rBV	2131321	2068745	20.57%	3.692%
8	10.675	1452	1460	1463	rBV	5042297	6173559	61.39%	11.016%
9	11.363	1571	1577	1584	rBV	2583916	2160469	21.48%	3.855%
10	12.963	1840	1849	1852	rBV	7645764	10056652	100.00%	17.945%
11	14.004	2021	2026	2037	rBV	2188939	2041946	20.30%	3.644%
12	15.468	2269	2275	2290	rVB	1242530	1733080	17.23%	3.093%




Sum of corrected areas: 56040185

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120820\
Data File : BF122586.D
Acq On : 8 Dec 2020 13:38
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

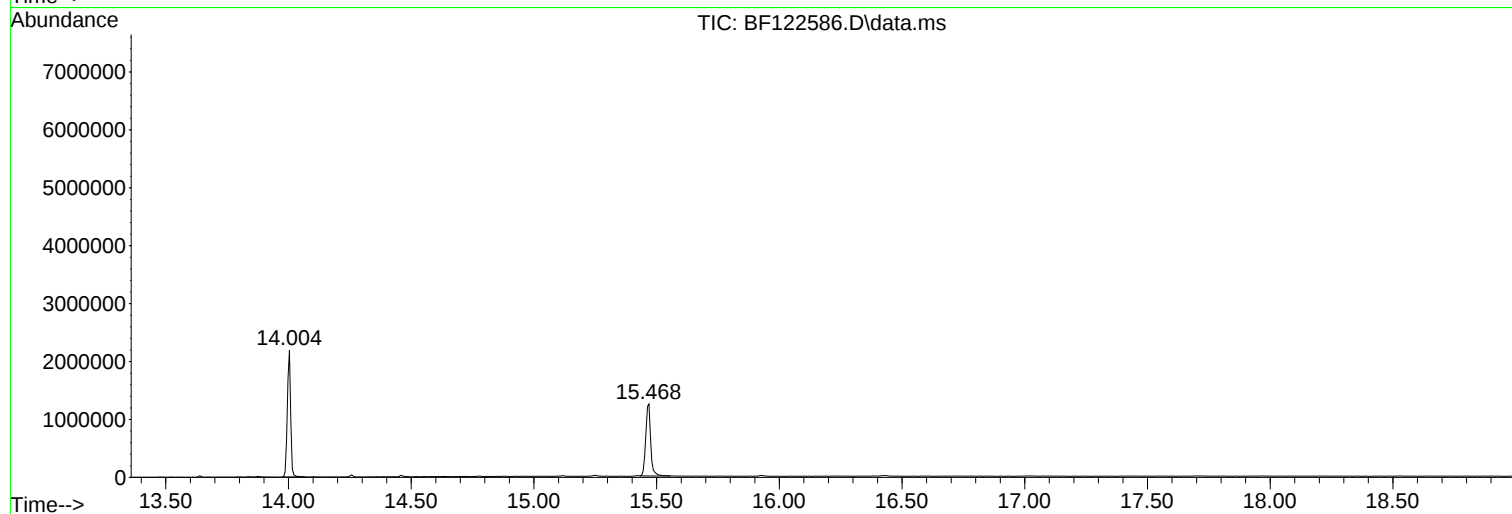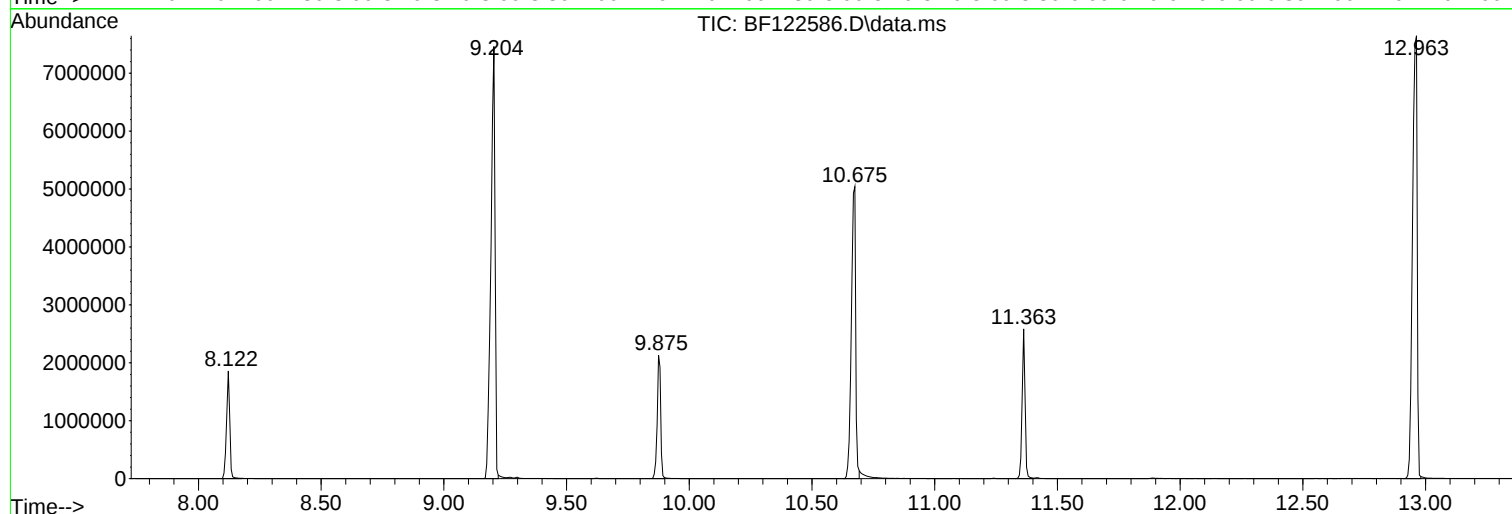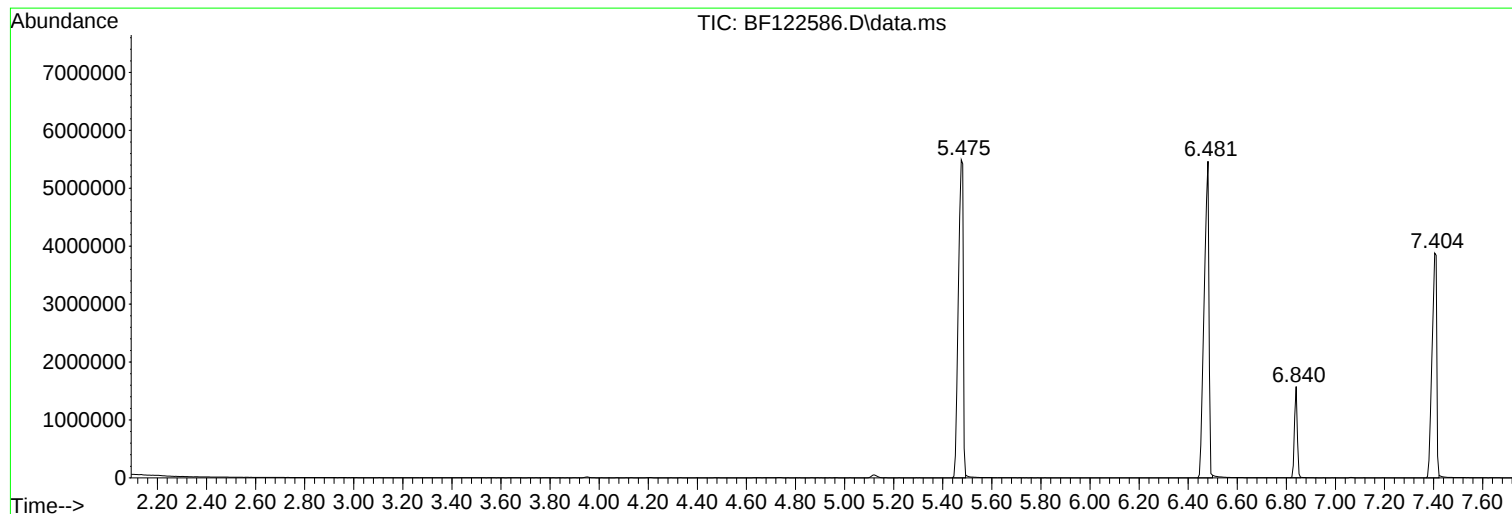

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120820\
Data File : BF122586.D
Acq On : 8 Dec 2020 13:38
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120820\
Data File : BF122586.D
Acq On : 8 Dec 2020 13:38
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------