


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120820\
 Data File : BF122584.D
 Acq On : 8 Dec 2020 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 07 12:08:49 2020

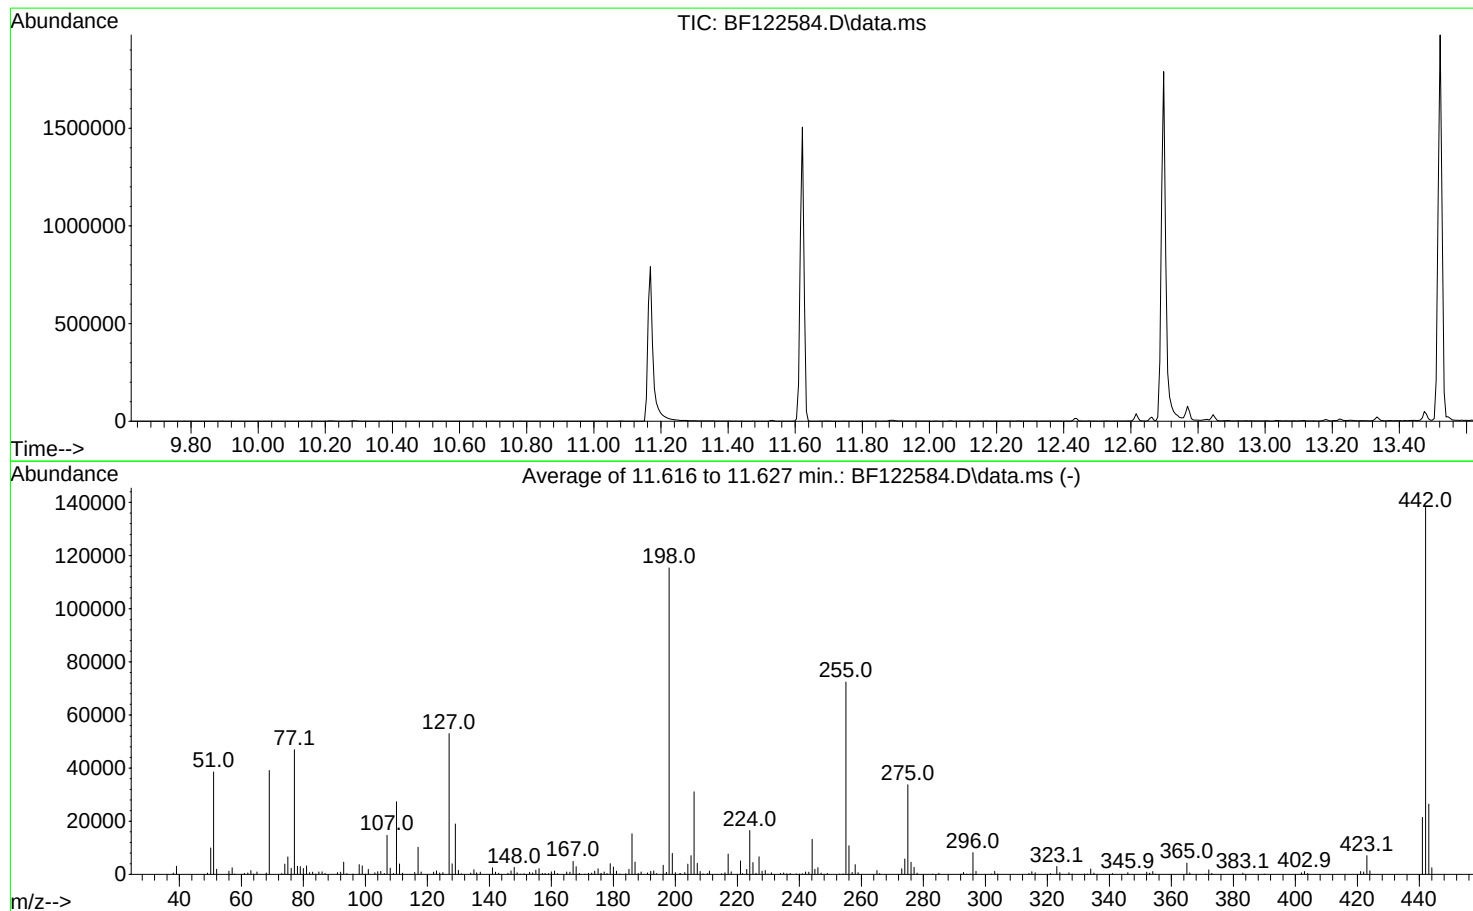

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	38520	PASS
68	69	0.00	2	1.3	524	PASS
69	198	0.00	100	33.9	39087	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	52981	PASS
197	198	0.00	2	0.7	794	PASS
198	198	100	100	100.0	115325	PASS
199	198	5	9	6.8	7896	PASS
275	198	10	60	29.3	33752	PASS
365	198	1	100	3.7	4275	PASS
441	198	0.01	100	18.6	21471	PASS
442	442	100	100	100.0	138464	PASS
443	442	15	24	19.1	26444	PASS