

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
 Data File : BF136465.D
 Acq On : 08 Dec 2023 13:58
 Operator : CG\JU
 Sample : PB157617BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157617BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	10	13	18	rVB	42794	53633	1.04%	0.189%
2	5.069	503	507	516	rVB	44053	63809	1.24%	0.225%
3	5.451	566	572	575	rBV	3641996	3578743	69.39%	12.593%
4	6.445	734	741	743	rBV	3115941	3554414	68.92%	12.507%
5	6.792	797	800	804	rVB	937898	751865	14.58%	2.646%
6	7.357	890	896	899	rBV	2161146	2295999	44.52%	8.079%
7	8.069	1012	1017	1021	rBV	1111205	1047052	20.30%	3.684%
8	9.151	1195	1201	1204	rBV	4916857	4737493	91.86%	16.670%
9	9.827	1310	1316	1319	rBV	1505475	1222419	23.70%	4.301%
10	10.622	1445	1451	1454	rBV	2958770	2896786	56.17%	10.193%
11	11.321	1566	1570	1573	rBV	1464678	1288615	24.99%	4.534%
12	12.921	1837	1842	1845	rBV	5394948	5157442	100.00%	18.148%
13	13.974	2016	2021	2024	rBV	1039427	995293	19.30%	3.502%
14	15.451	2266	2272	2277	rBV	617065	775097	15.03%	2.727%




Sum of corrected areas: 28418660

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136465.D
Acq On : 08 Dec 2023 13:58
Operator : CG\JU
Sample : PB157617BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157617BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

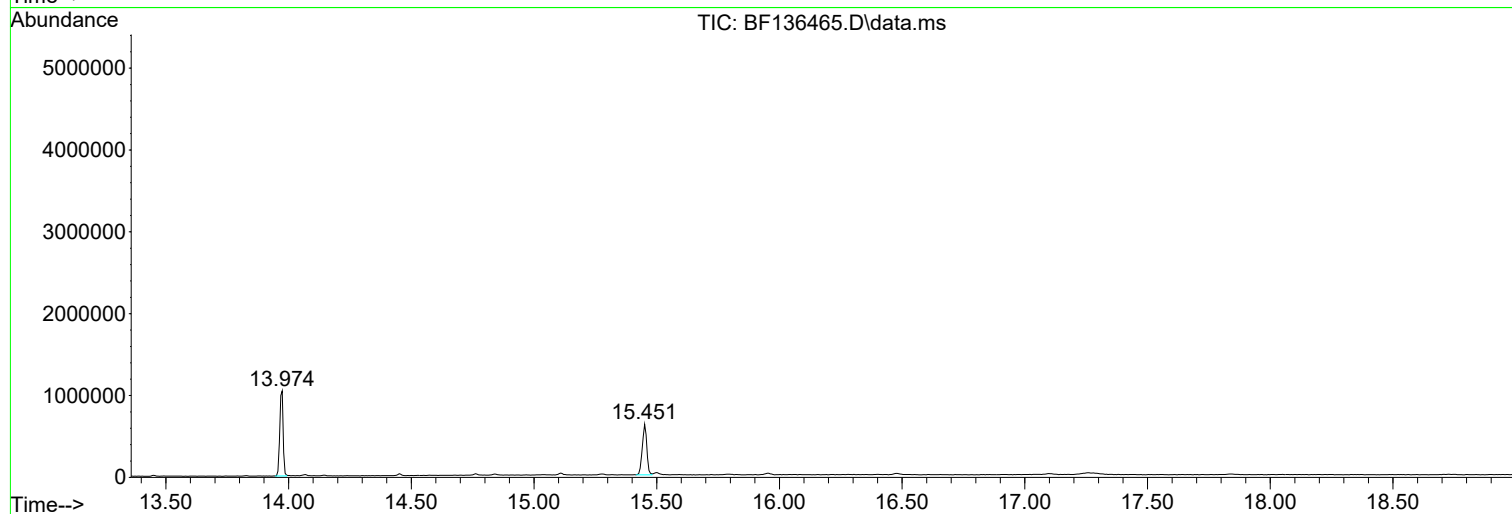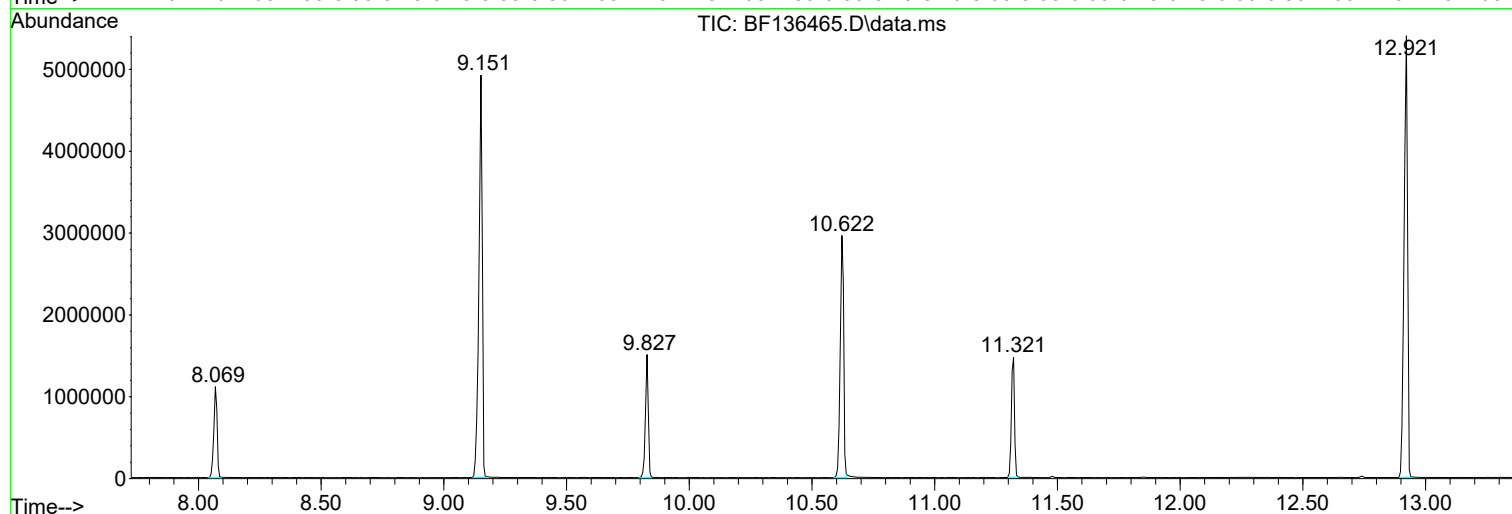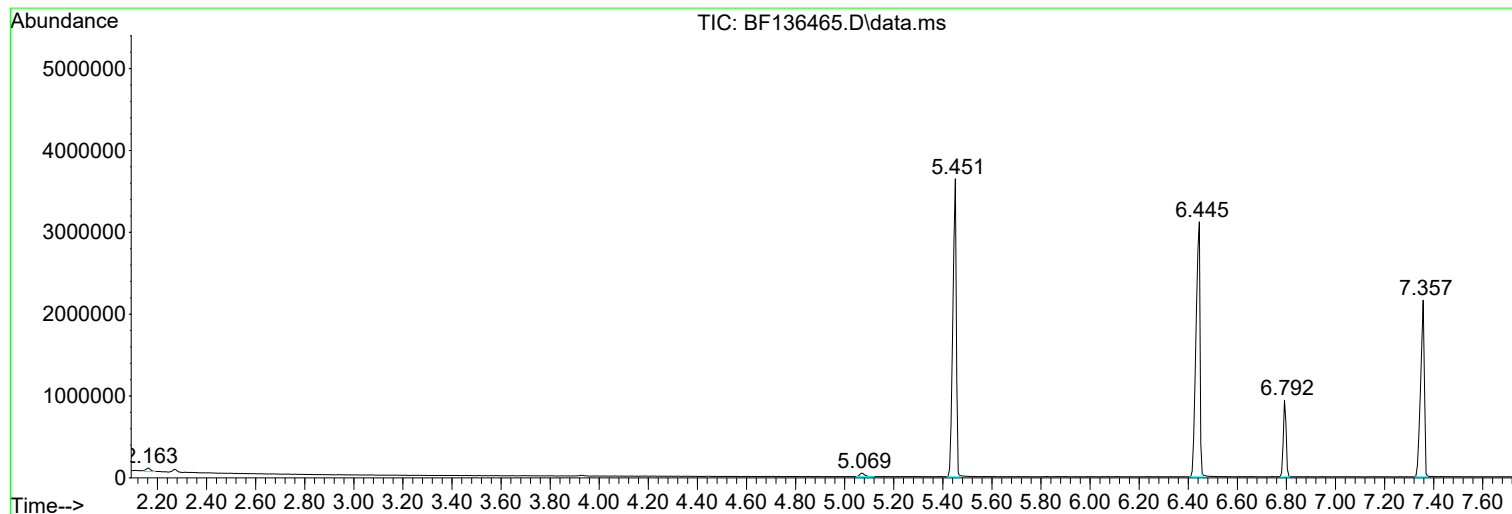

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136465.D
Acq On : 08 Dec 2023 13:58
Operator : CG\JU
Sample : PB157617BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157617BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136465.D
Acq On : 08 Dec 2023 13:58
Operator : CG\JU
Sample : PB157617BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157617BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------