

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
 Data File : BF136477.D
 Acq On : 08 Dec 2023 20:14
 Operator : CG\JU
 Sample : 05599-01RE
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-01RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.222	19	23	30	rVB4	32645	51716	1.83%	0.317%
2	5.034	497	501	510	rVB	222779	266034	9.44%	1.628%
3	5.440	566	570	573	rBV	2272802	2023591	71.80%	12.387%
4	6.440	735	740	743	rBV	2252618	2112310	74.95%	12.930%
5	6.793	797	800	804	rVB	743704	640144	22.71%	3.919%
6	7.357	890	896	899	rBV	1627422	1418487	50.33%	8.683%
7	8.069	1013	1017	1021	rBV	922092	851231	30.20%	5.211%
8	9.151	1195	1201	1204	rBV	3570149	2818423	100.00%	17.253%
9	9.828	1312	1316	1320	rBV	1158946	905399	32.12%	5.542%
10	10.622	1447	1451	1454	rBV	1325595	1189051	42.19%	7.279%
11	11.322	1566	1570	1573	rBV	899038	783343	27.79%	4.795%
12	12.739	1808	1811	1814	rBV	55635	46841	1.66%	0.287%
13	12.916	1837	1841	1844	rBV	2468499	2049242	72.71%	12.544%
14	13.451	1928	1932	1936	rBV	41810	36181	1.28%	0.221%
15	13.904	2003	2009	2010	rBV5	23012	34839	1.24%	0.213%
16	13.969	2017	2020	2024	rVB	586713	550064	19.52%	3.367%
17	14.839	2165	2168	2174	rVB2	39500	41981	1.49%	0.257%
18	15.451	2267	2272	2277	rBV	430318	517281	18.35%	3.166%




Sum of corrected areas: 16336158

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136477.D
Acq On : 08 Dec 2023 20:14
Operator : CG\JU
Sample : 05599-01RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

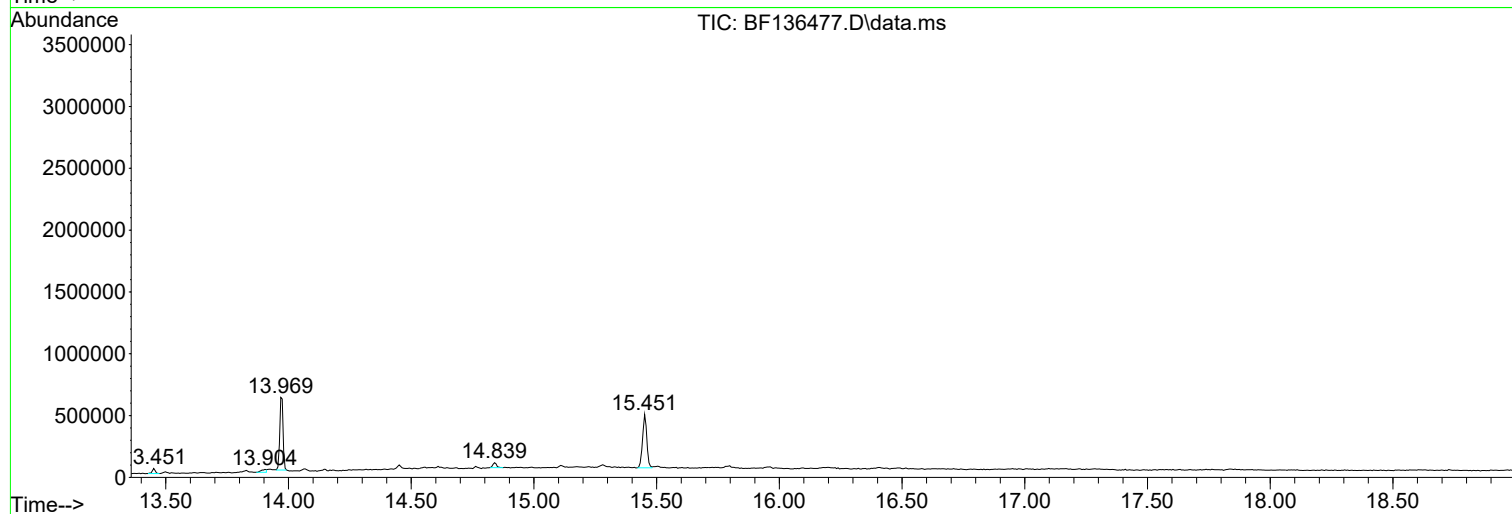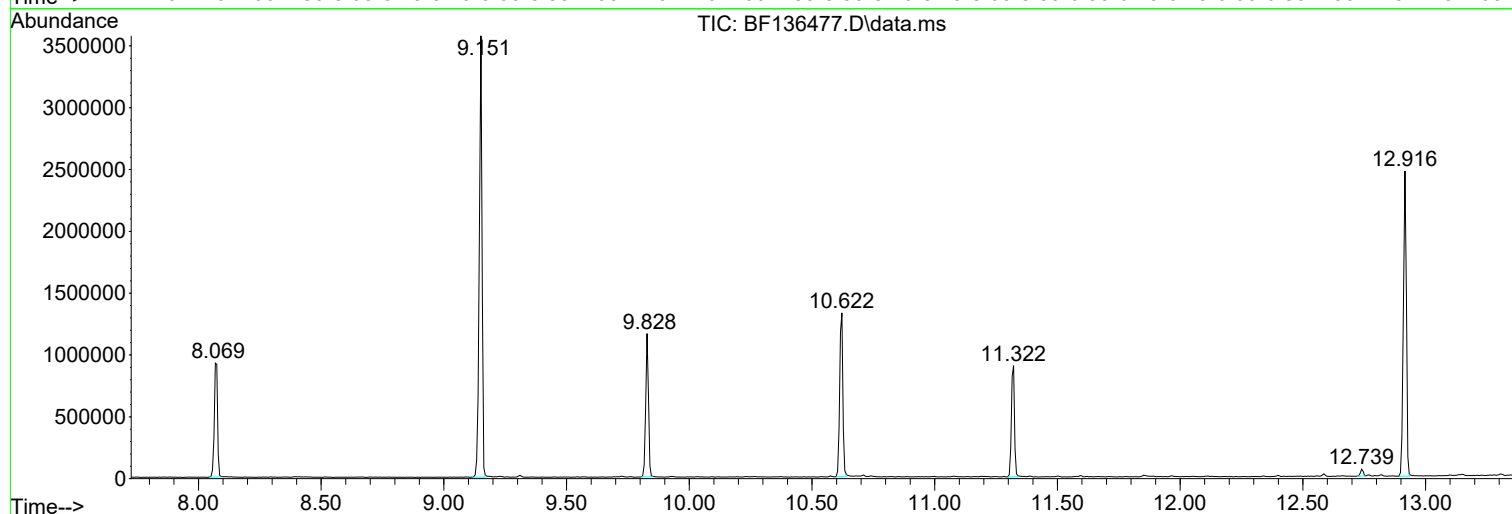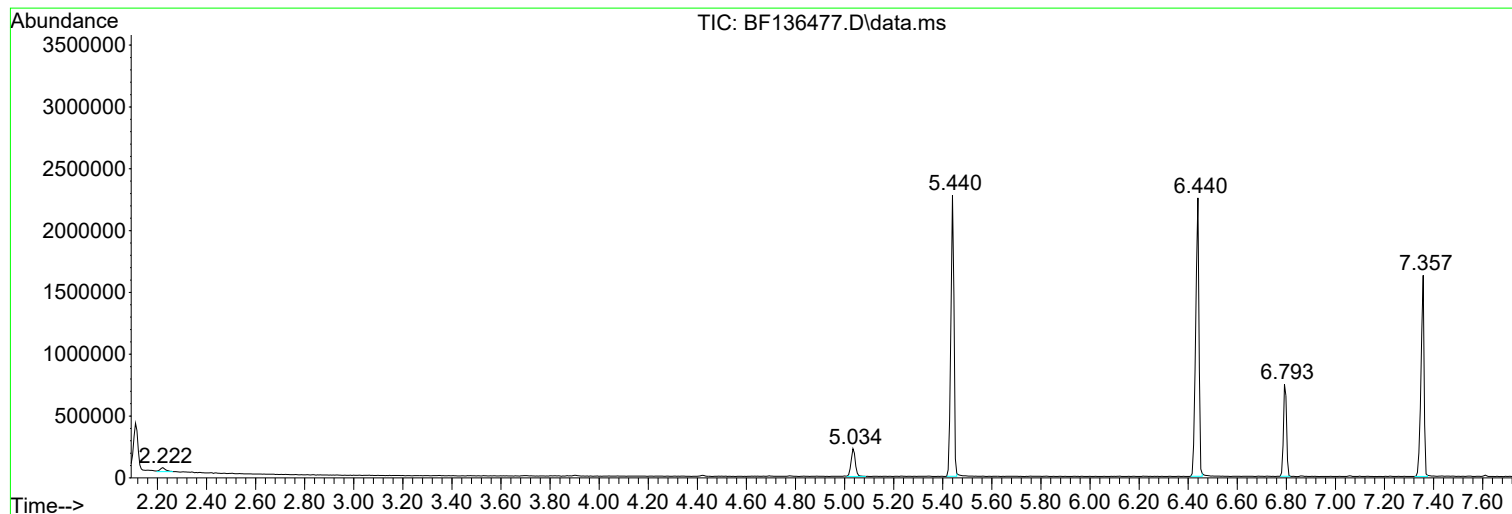

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136477.D
Acq On : 08 Dec 2023 20:14
Operator : CG\JU
Sample : 05599-01RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136477.D
Acq On : 08 Dec 2023 20:14
Operator : CG\JU
Sample : 05599-01RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------