

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
 Data File : BF136478.D
 Acq On : 08 Dec 2023 20:46
 Operator : CG\JU
 Sample : 05599-03RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-02RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	3	7	13	rVB	455895	558129	16.40%	2.930%
2	2.234	22	25	35	rVB2	38536	61304	1.80%	0.322%
3	5.040	497	502	510	rVB	378992	448210	13.17%	2.353%
4	5.445	566	571	574	rBV	2469473	2226131	65.40%	11.685%
5	6.440	735	740	743	rBV	2329633	2471447	72.61%	12.972%
6	6.792	797	800	804	rBV	783657	697740	20.50%	3.662%
7	7.357	890	896	899	rBV	1860049	1742303	51.18%	9.145%
8	8.075	1013	1018	1021	rBV	1036275	915600	26.90%	4.806%
9	9.151	1195	1201	1204	rBV	4029140	3403938	100.00%	17.867%
10	9.828	1312	1316	1319	rBV	1231448	951444	27.95%	4.994%
11	10.622	1447	1451	1454	rBV	1178723	1062050	31.20%	5.575%
12	11.322	1566	1570	1573	rBV	883271	765417	22.49%	4.018%
13	12.916	1837	1841	1844	rBV	2707335	2474603	72.70%	12.989%
14	13.927	2005	2013	2016	rBV8	22229	67105	1.97%	0.352%
15	13.974	2017	2021	2026	rVB	674219	655122	19.25%	3.439%
16	15.451	2267	2272	2278	rBV	454523	551143	16.19%	2.893%




Sum of corrected areas: 19051686

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136478.D
Acq On : 08 Dec 2023 20:46
Operator : CG\JU
Sample : 05599-03RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-02RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

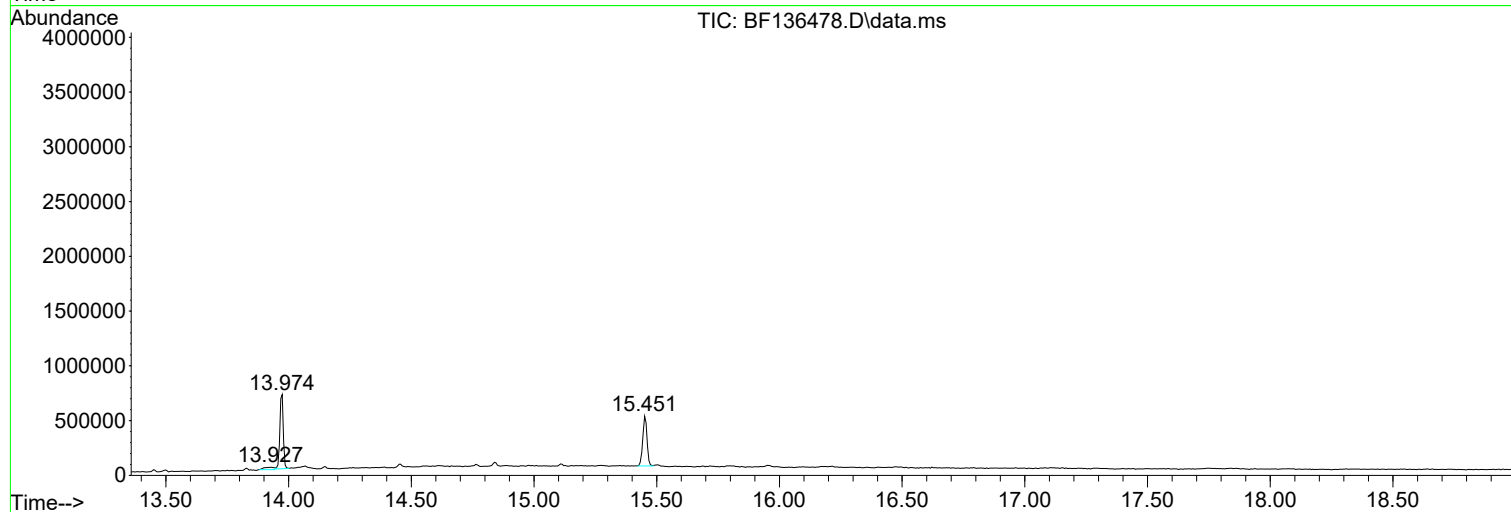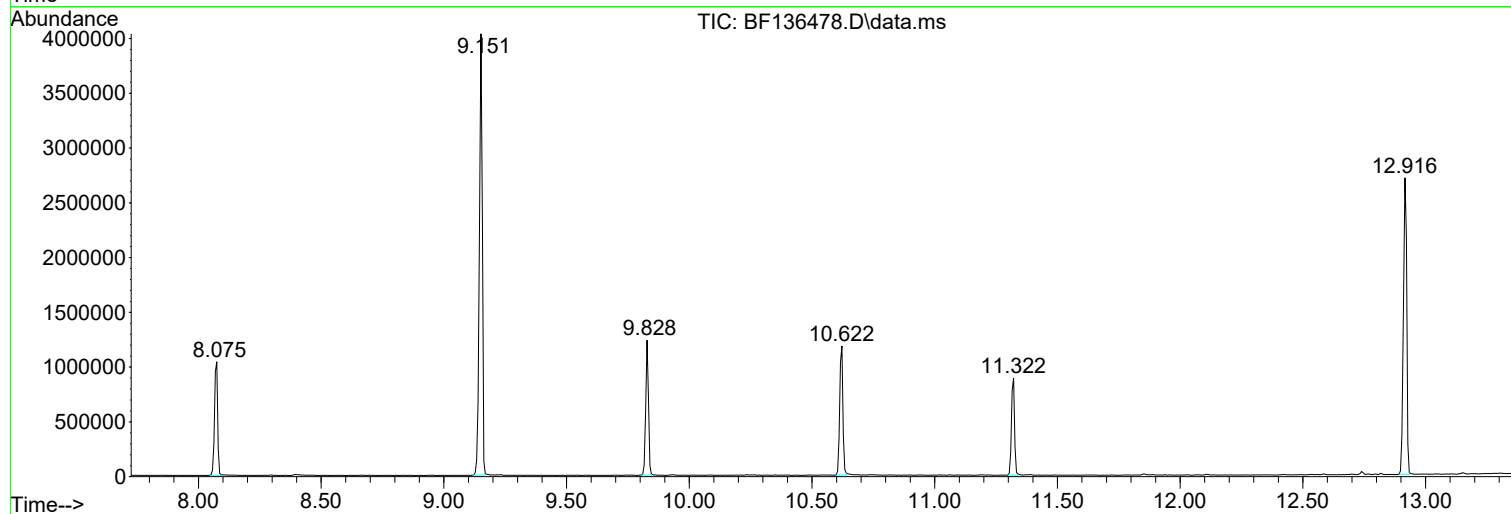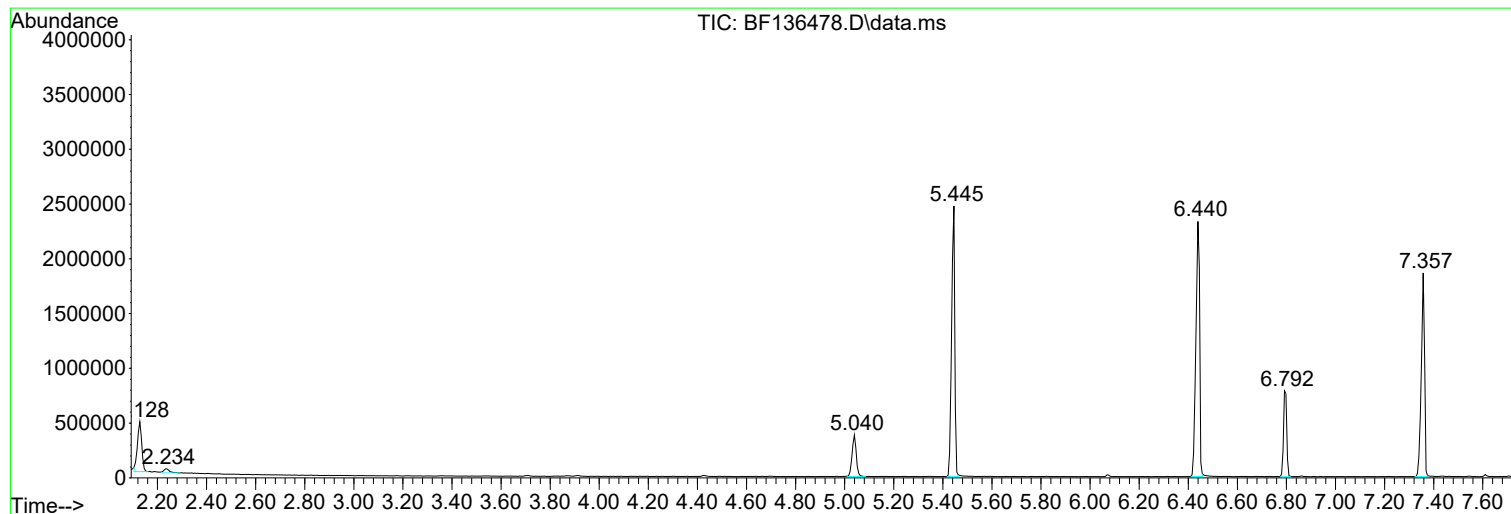

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136478.D
Acq On : 08 Dec 2023 20:46
Operator : CG\JU
Sample : 05599-03RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-02RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136478.D
Acq On : 08 Dec 2023 20:46
Operator : CG\JU
Sample : 05599-03RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-02RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------