

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
 Data File : BF136479.D
 Acq On : 08 Dec 2023 21:18
 Operator : CG\JU
 Sample : 05599-07RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-04RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	18	21	28	rVB	39260	61461	2.01%	0.344%
2	5.040	498	502	508	rVB	56578	70441	2.30%	0.394%
3	5.440	565	570	573	rBV	2534904	2406873	78.68%	13.472%
4	6.439	735	740	743	rBV	2402475	2393430	78.24%	13.396%
5	6.792	797	800	804	rBV	799618	701265	22.92%	3.925%
6	7.357	890	896	899	rBV	1773428	1563723	51.12%	8.752%
7	8.075	1013	1018	1021	rBV	1031821	914768	29.90%	5.120%
8	9.151	1196	1201	1204	rBV	3802828	3059012	100.00%	17.122%
9	9.827	1312	1316	1320	rBV	1182512	943005	30.83%	5.278%
10	10.622	1447	1451	1454	rBV	1524512	1295778	42.36%	7.253%
11	11.321	1566	1570	1573	rBV	872800	746692	24.41%	4.179%
12	11.592	1609	1616	1619	rBV2	36895	37013	1.21%	0.207%
13	11.857	1657	1661	1665	rBV2	86885	96739	3.16%	0.541%
14	12.915	1837	1841	1845	rBV	2332855	2158561	70.56%	12.082%
15	13.815	1989	1994	1999	rBV6	23501	50152	1.64%	0.281%
16	13.921	2003	2012	2013	rBV8	35213	84065	2.75%	0.471%
17	13.974	2017	2021	2027	rVB	727182	668354	21.85%	3.741%
18	14.451	2098	2102	2106	rBV3	41455	52178	1.71%	0.292%
19	15.451	2267	2272	2278	rBV	437002	562769	18.40%	3.150%




Sum of corrected areas: 17866279

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136479.D
Acq On : 08 Dec 2023 21:18
Operator : CG\JU
Sample : 05599-07RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-04RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

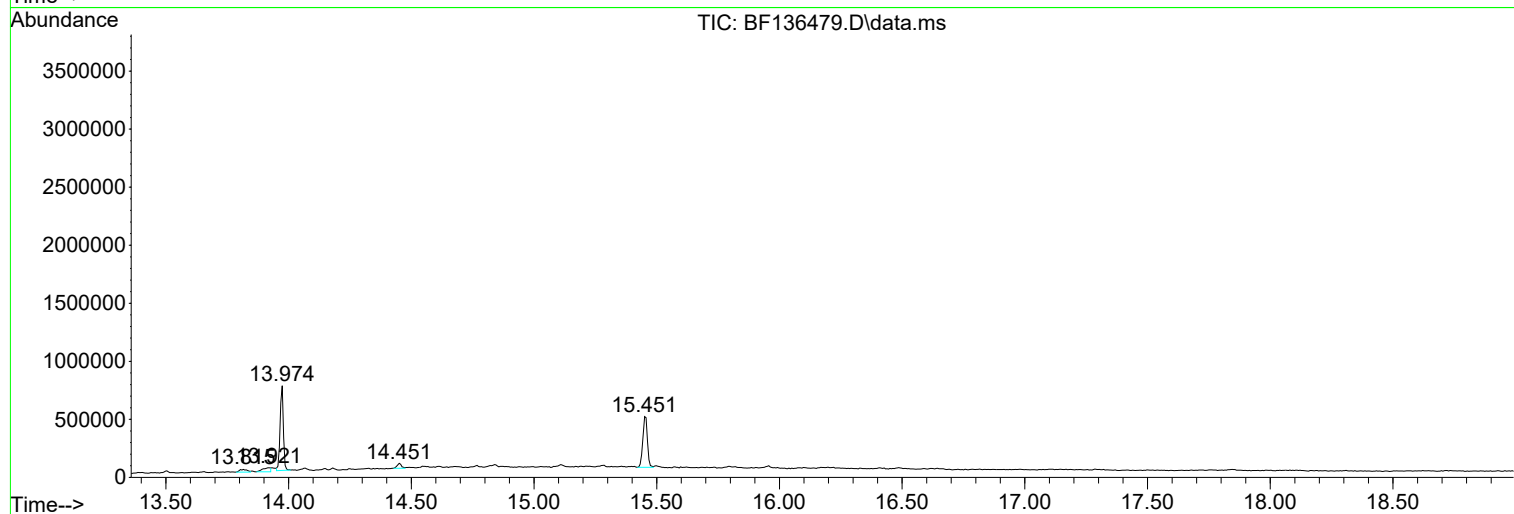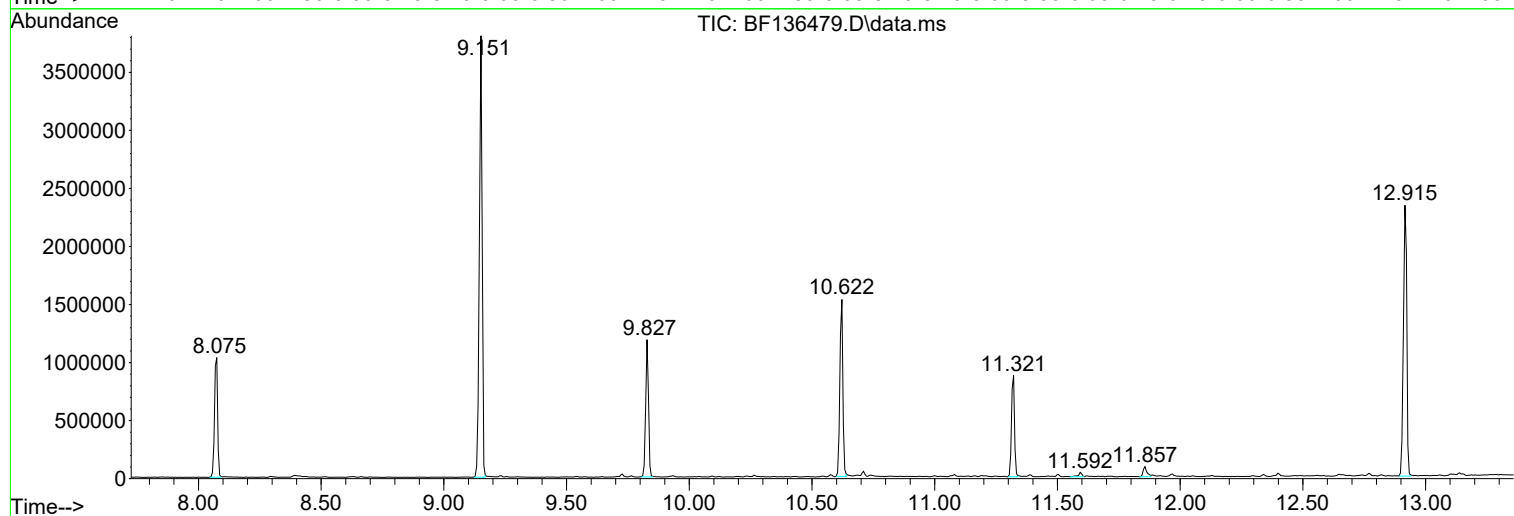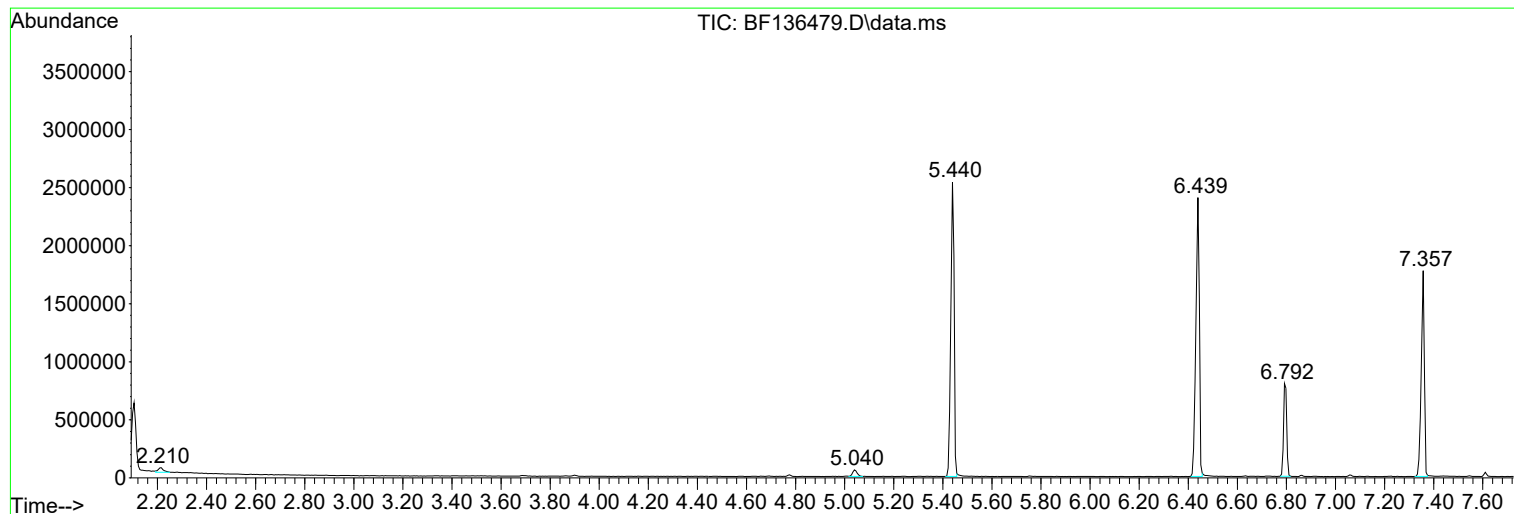

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136479.D
Acq On : 08 Dec 2023 21:18
Operator : CG\JU
Sample : 05599-07RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-04RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136479.D
Acq On : 08 Dec 2023 21:18
Operator : CG\JU
Sample : 05599-07RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-04RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------