

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
 Data File : BF136482.D
 Acq On : 08 Dec 2023 22:57
 Operator : CG\JU
 Sample : 05599-13RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-07RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.216	19	22	33	rVB2	37115	62765	1.92%	0.328%
2	5.045	498	503	512	rVB	54882	74468	2.28%	0.389%
3	5.440	565	570	573	rBV	2654499	2591934	79.31%	13.551%
4	6.439	735	740	743	rBV	2452769	2578474	78.89%	13.481%
5	6.792	797	800	804	rVB	815035	692628	21.19%	3.621%
6	7.357	890	896	899	rBV	1756800	1675566	51.27%	8.760%
7	7.610	935	939	942	rBV	49222	37646	1.15%	0.197%
8	8.075	1012	1018	1021	rBV	1015268	918884	28.12%	4.804%
9	8.386	1067	1071	1084	rBV	29886	66828	2.04%	0.349%
10	9.151	1195	1201	1204	rBV	3931992	3268286	100.00%	17.087%
11	9.828	1312	1316	1319	rBV	1236927	964867	29.52%	5.044%
12	10.622	1446	1451	1454	rBV	1804526	1509978	46.20%	7.894%
13	11.322	1566	1570	1573	rBV	934393	810674	24.80%	4.238%
14	11.857	1657	1661	1666	rBV	77535	96263	2.95%	0.503%
15	12.916	1837	1841	1844	rBV	2773496	2370653	72.54%	12.394%
16	13.827	1989	1996	2002	rBV5	26478	61781	1.89%	0.323%
17	13.927	2003	2013	2016	rBV8	32114	110394	3.38%	0.577%
18	13.968	2017	2020	2024	rVB	658867	606993	18.57%	3.173%
19	14.063	2032	2036	2043	rVB5	21619	40432	1.24%	0.211%
20	14.451	2098	2102	2107	rBV3	41946	55167	1.69%	0.288%
21	15.451	2267	2272	2277	rBV	424937	532523	16.29%	2.784%




Sum of corrected areas: 19127204

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136482.D
Acq On : 08 Dec 2023 22:57
Operator : CG\JU
Sample : 05599-13RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-07RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

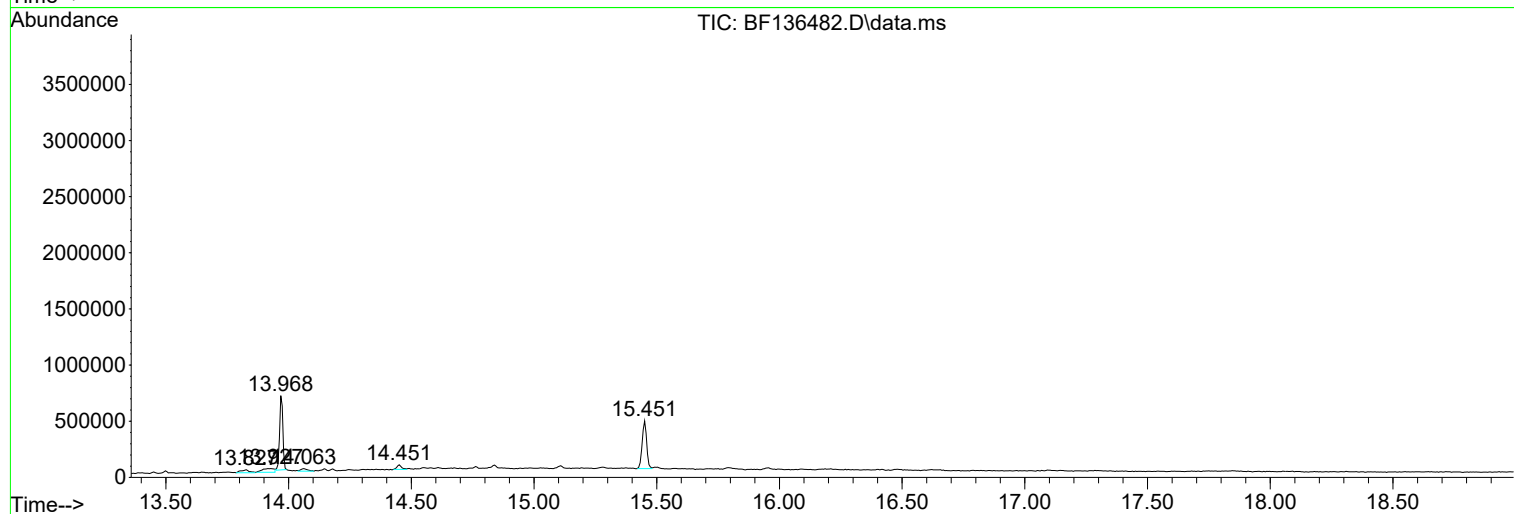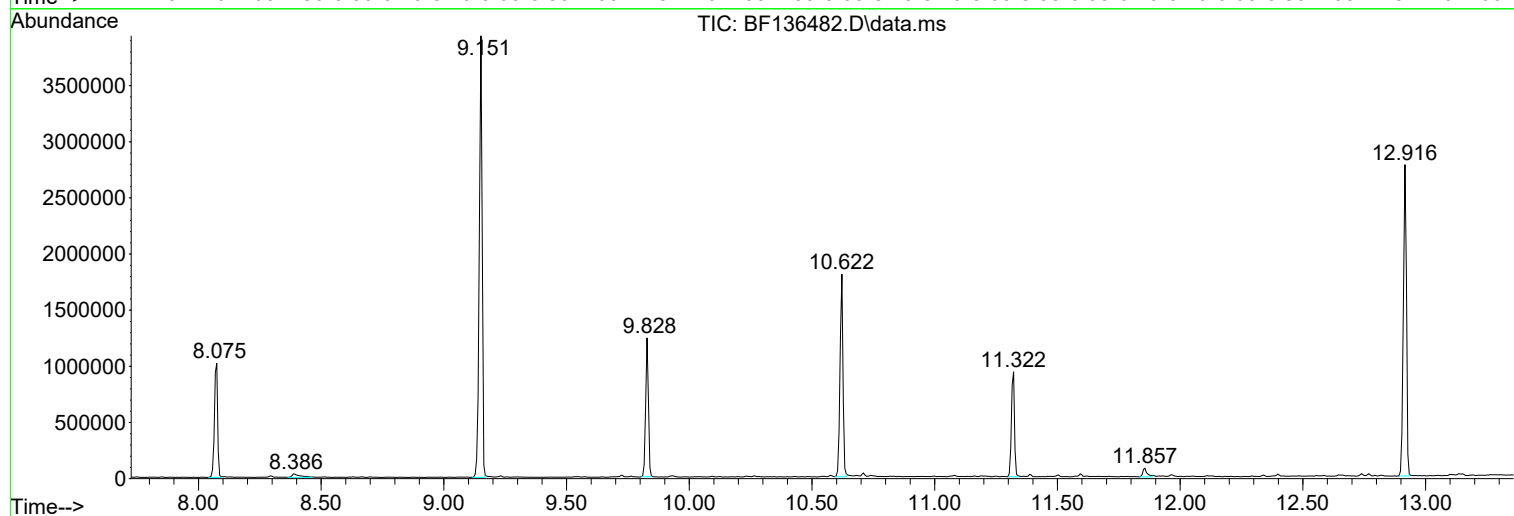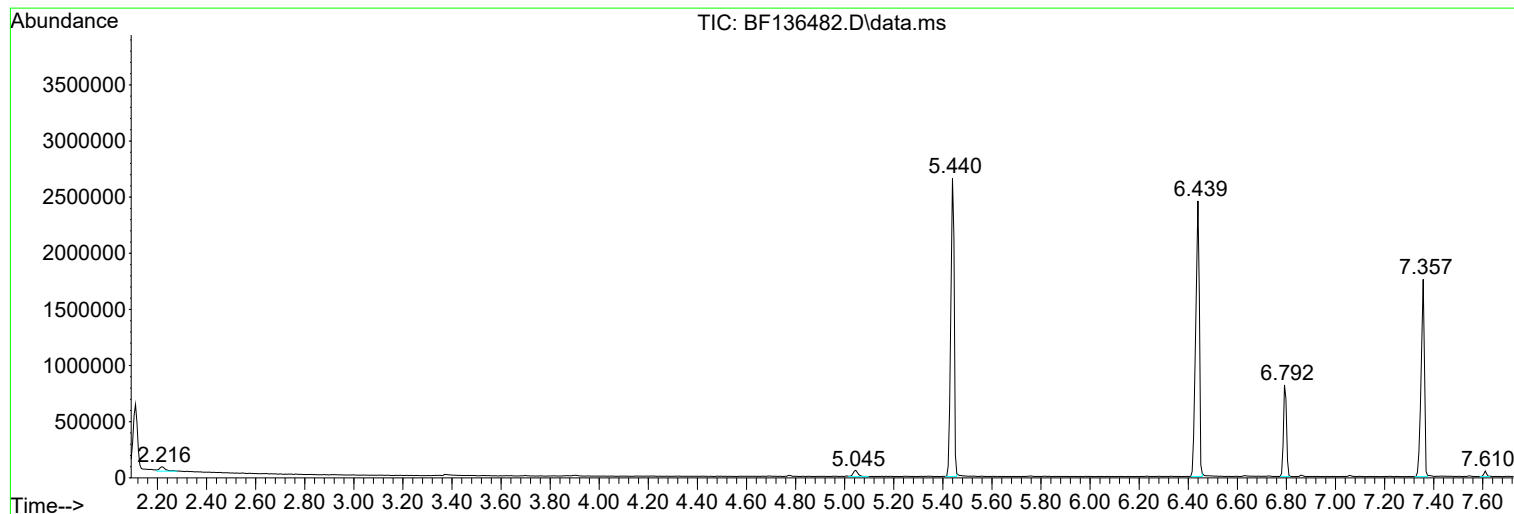

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136482.D
Acq On : 08 Dec 2023 22:57
Operator : CG\JU
Sample : 05599-13RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-07RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136482.D
Acq On : 08 Dec 2023 22:57
Operator : CG\JU
Sample : 05599-13RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-07RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------