

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
 Data File : BF136483.D
 Acq On : 08 Dec 2023 23:30
 Operator : CG\JU
 Sample : 05599-15RE
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LKWD-BACKFILL-08RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	17	21	32	rVB3	36923	71175	2.33%	0.398%
2	5.040	498	502	508	rVB	59607	71180	2.33%	0.398%
3	5.440	565	570	573	rBV	2566251	2345383	76.82%	13.120%
4	6.440	735	740	743	rBV	2354172	2346047	76.84%	13.123%
5	6.792	797	800	804	rVB	819006	696552	22.81%	3.896%
6	7.357	891	896	899	rBV	1719226	1535226	50.28%	8.588%
7	7.610	936	939	942	rBV	50615	39190	1.28%	0.219%
8	8.069	1013	1017	1021	rBV	1035342	917353	30.05%	5.132%
9	8.386	1068	1071	1082	rBV	48208	84634	2.77%	0.473%
10	9.151	1196	1201	1204	rBV	3874065	3053172	100.00%	17.079%
11	9.828	1312	1316	1320	rBV	1219779	964236	31.58%	5.394%
12	9.933	1327	1334	1338	rBV	63101	87149	2.85%	0.488%
13	10.622	1446	1451	1454	rBV	1553911	1358836	44.51%	7.601%
14	11.322	1566	1570	1573	rBV	895213	794298	26.02%	4.443%
15	11.857	1657	1661	1665	rBV	50817	62104	2.03%	0.347%
16	12.916	1837	1841	1844	rBV	2659462	2191997	71.79%	12.262%
17	13.910	2004	2010	2011	rBV6	22021	38642	1.27%	0.216%
18	13.968	2016	2020	2024	rVV	658059	636672	20.85%	3.561%
19	14.451	2099	2102	2106	rBV3	48275	51252	1.68%	0.287%
20	15.451	2267	2272	2277	rBV	428534	531596	17.41%	2.974%




Sum of corrected areas: 17876694

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136483.D
Acq On : 08 Dec 2023 23:30
Operator : CG\JU
Sample : 05599-15RE
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-08RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

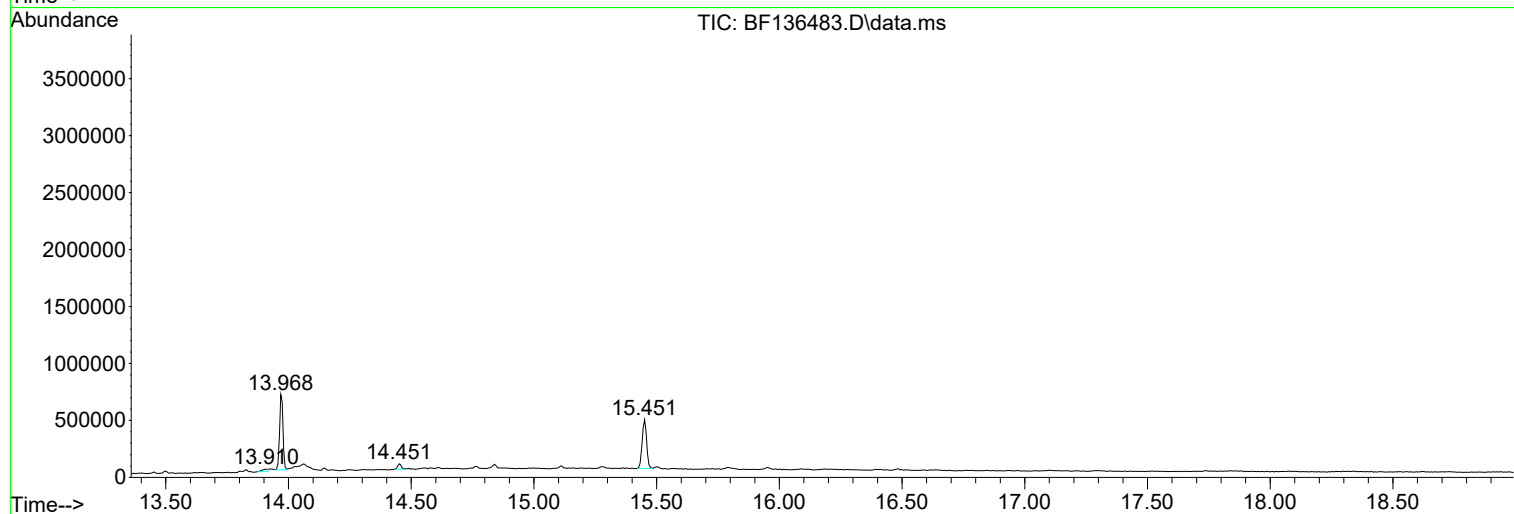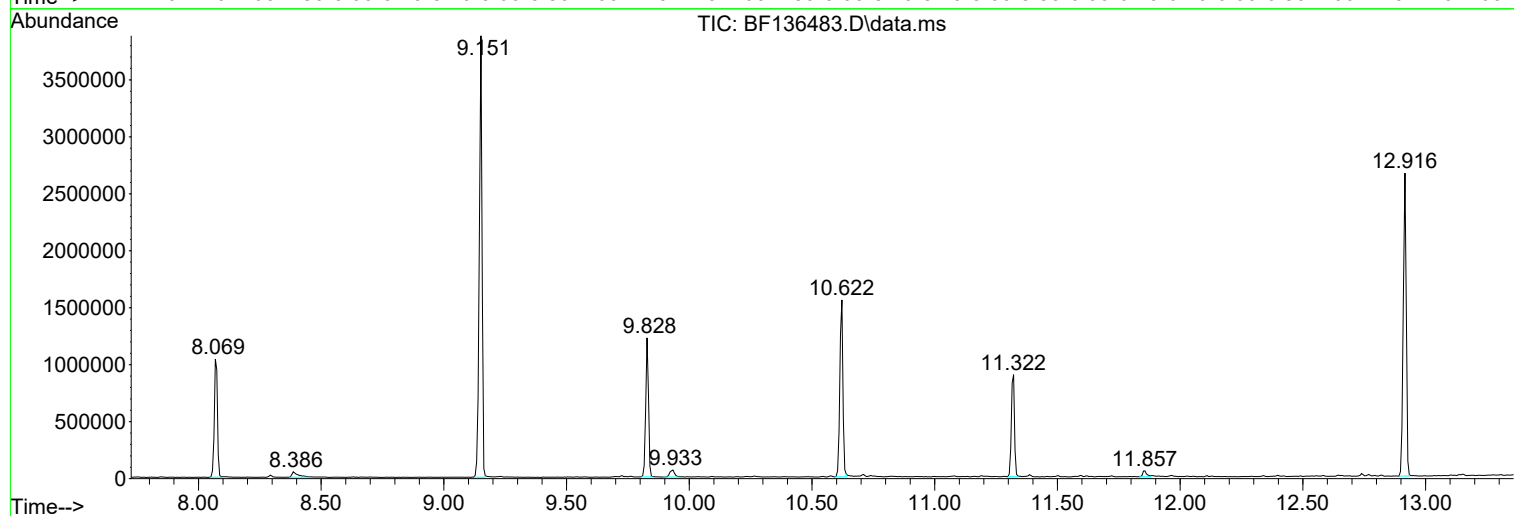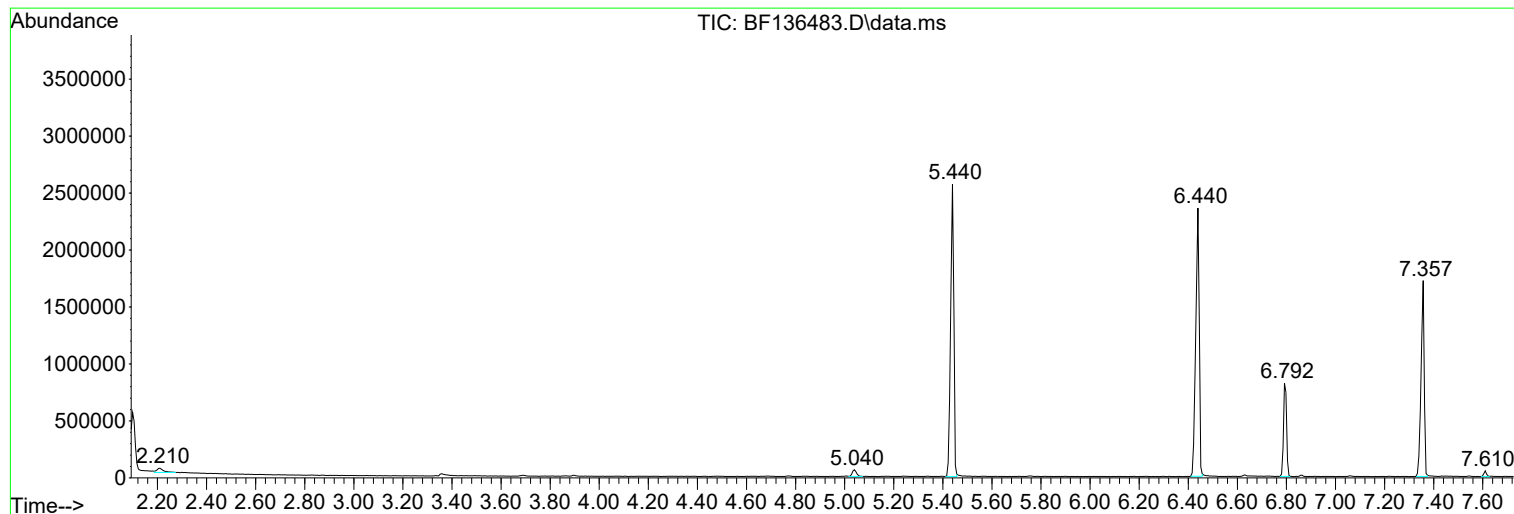

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136483.D
Acq On : 08 Dec 2023 23:30
Operator : CG\JU
Sample : 05599-15RE
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-08RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136483.D
Acq On : 08 Dec 2023 23:30
Operator : CG\JU
Sample : 05599-15RE
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LKWD-BACKFILL-08RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------