


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136463.D
Acq On : 08 Dec 2023 12:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 09:40:27 2023

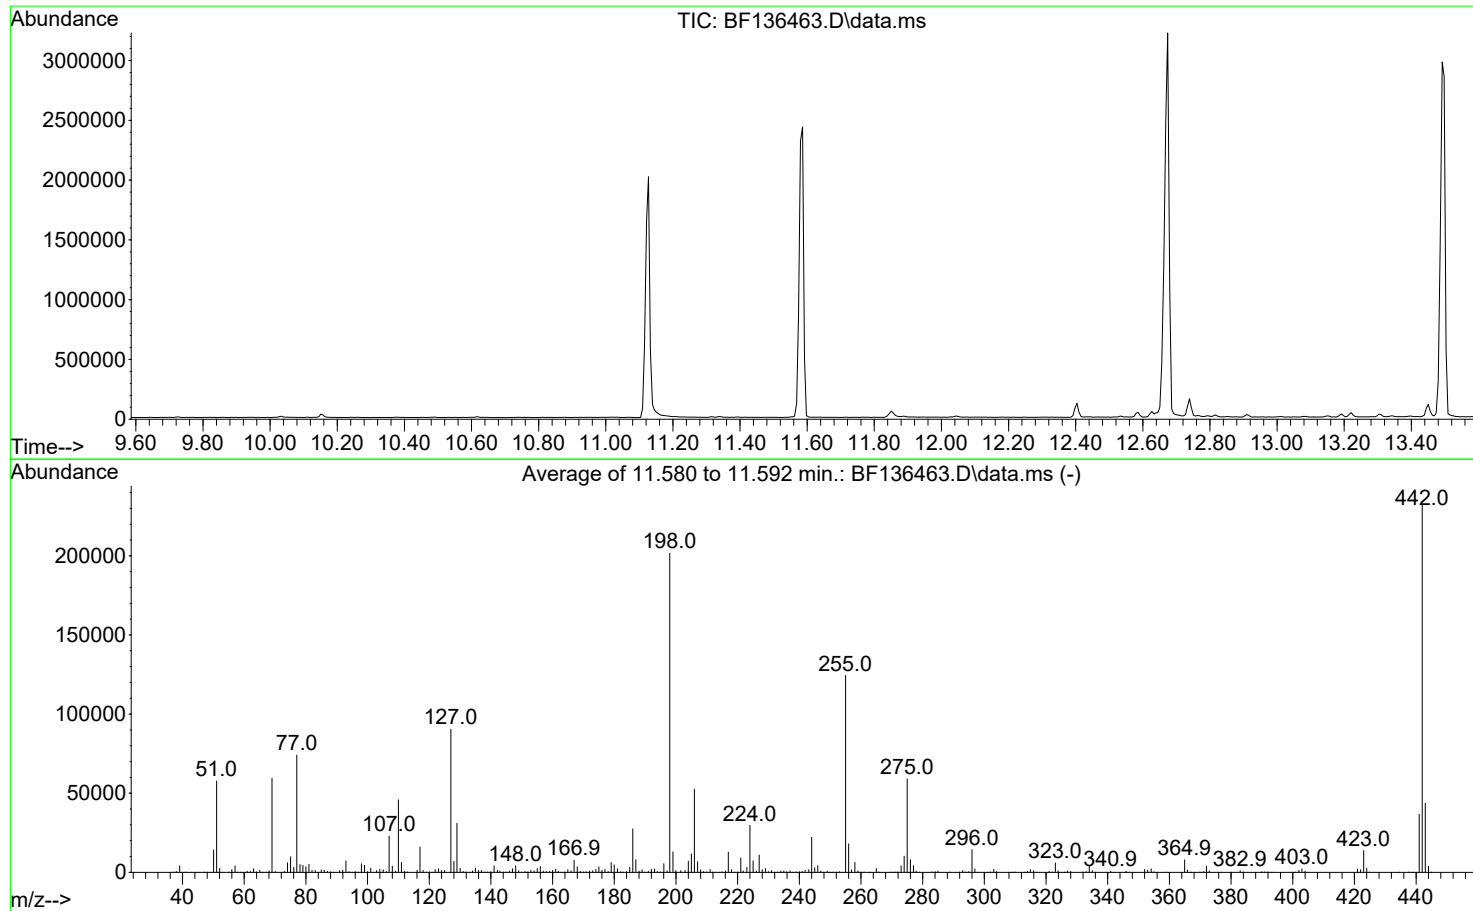

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	57690	PASS
68	69	0.00	2	1.8	1059	PASS
69	198	0.00	100	29.5	59511	PASS
70	69	0.00	2	0.8	470	PASS
127	198	10	80	44.8	90417	PASS
197	198	0.00	2	0.5	984	PASS
198	198	100	100	100.0	201688	PASS
199	198	5	9	6.4	12962	PASS
275	198	10	60	29.3	59085	PASS
365	198	1	100	3.9	7893	PASS
441	198	0.01	100	18.2	36701	PASS
442	442	50	100	100.0	232448	PASS
443	442	15	24	18.8	43704	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/8/2023	BNA_F	<u>BF136463.D</u>
Compound Name	Response	Retention Time
DDT	606383	13.498
DDD	10360	13.221
DDE	603	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10963	617346	1.78

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136463.D
Acq On : 08 Dec 2023 12:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 08 17:21:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

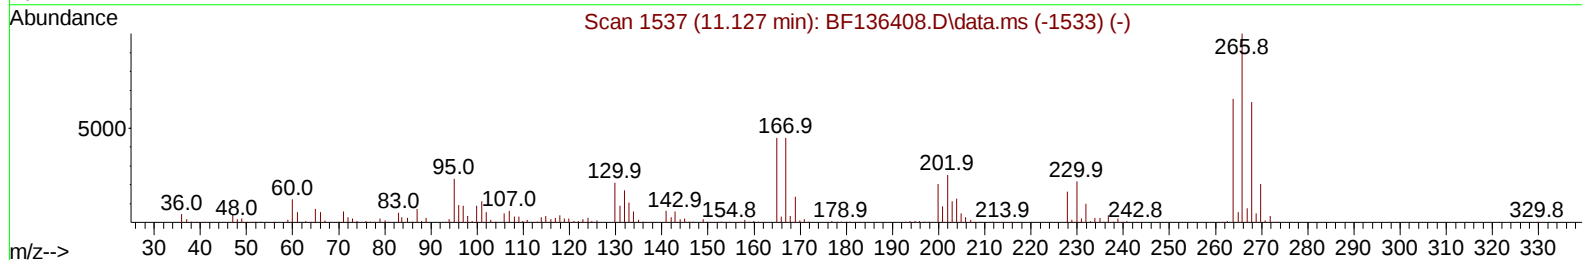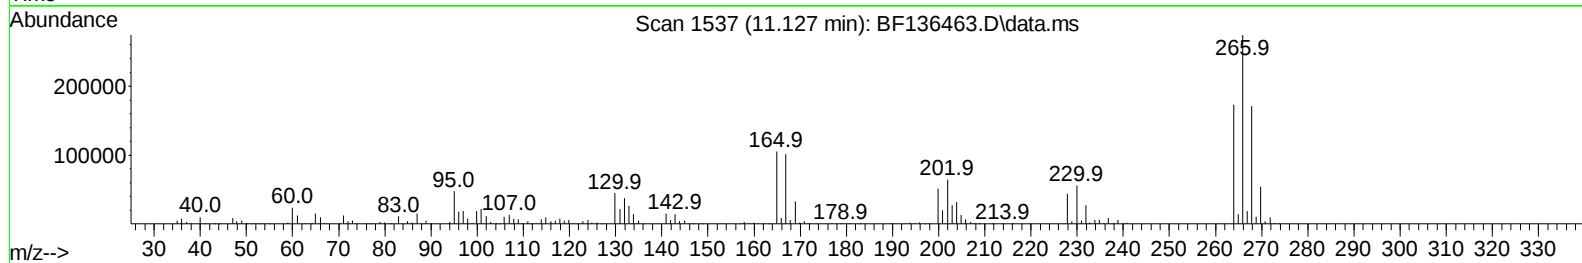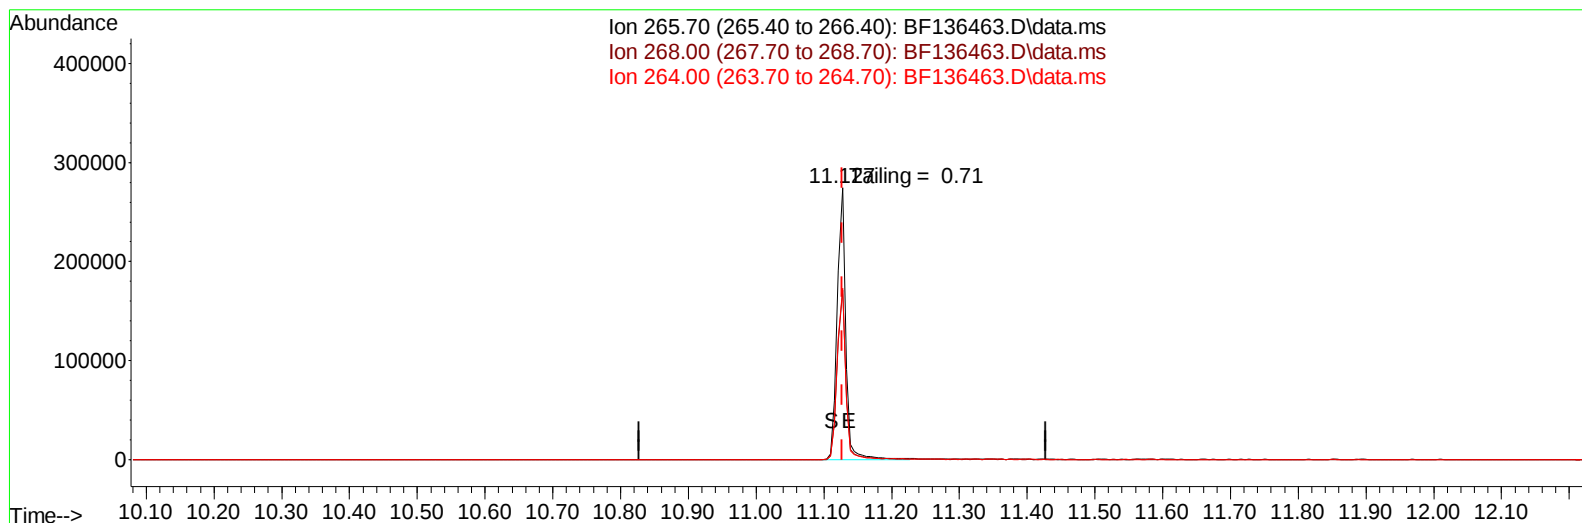

TIC: BF136463.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 19124.33 ng




response 236994

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.30
264.00	65.30	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120823\
Data File : BF136463.D
Acq On : 08 Dec 2023 12:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 08 17:21:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

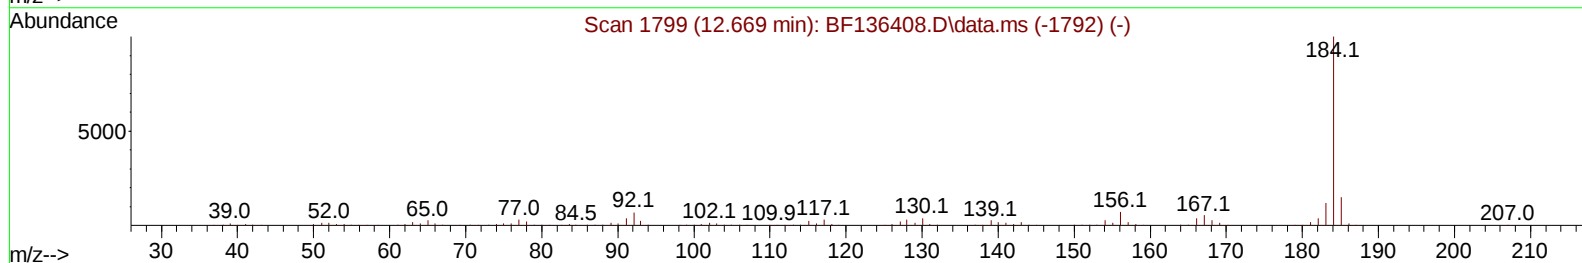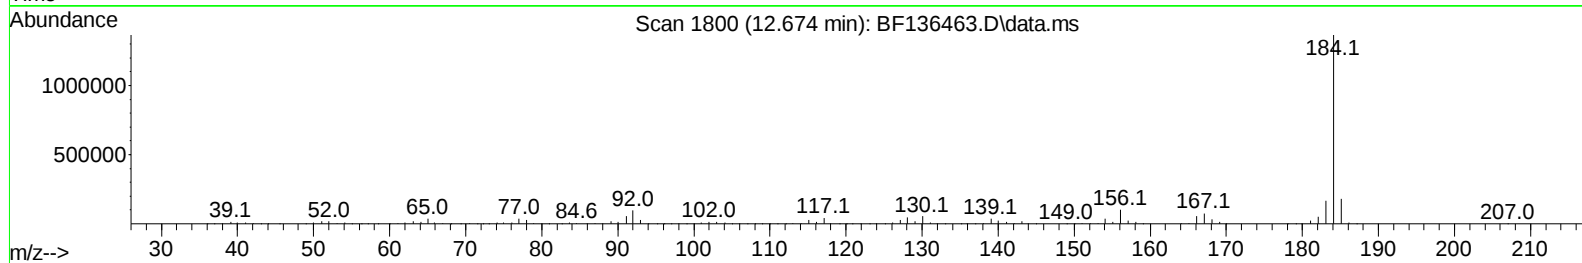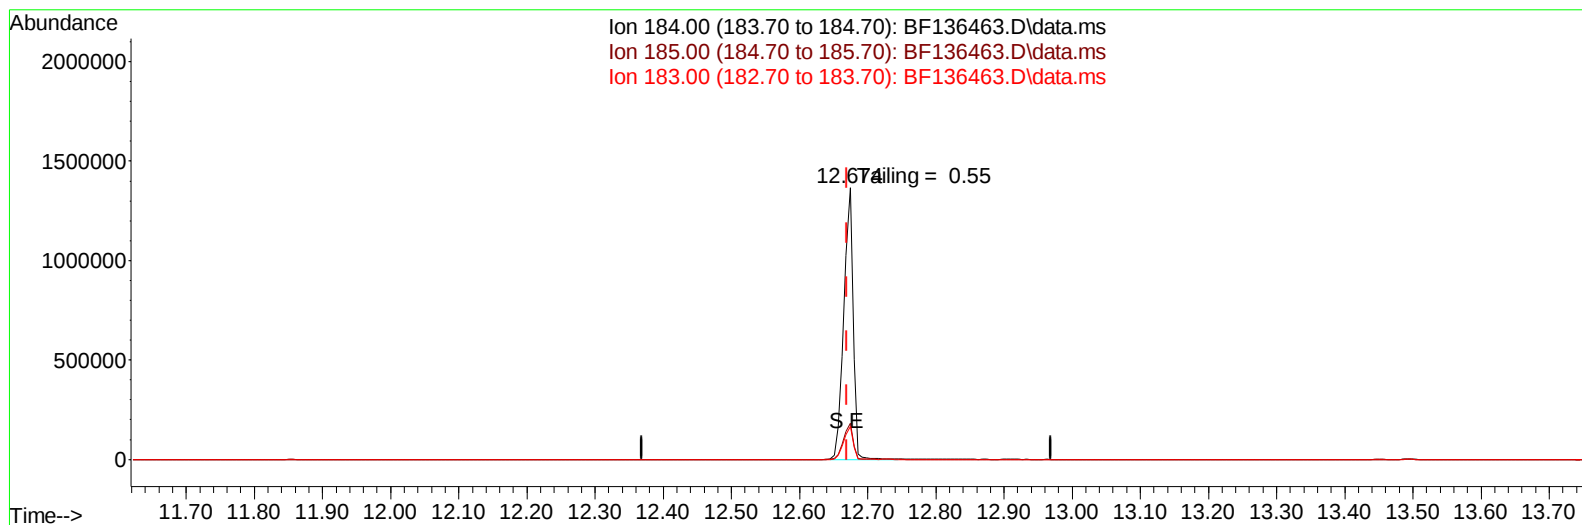

TIC: BF136463.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 1259.87 ng

response 1297201

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.40
183.00	11.70	12.16
0.00	0.00	0.00