
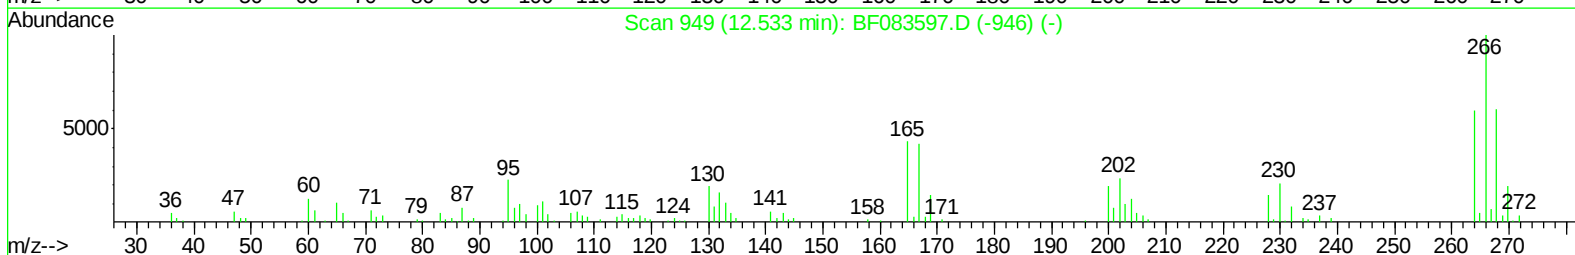
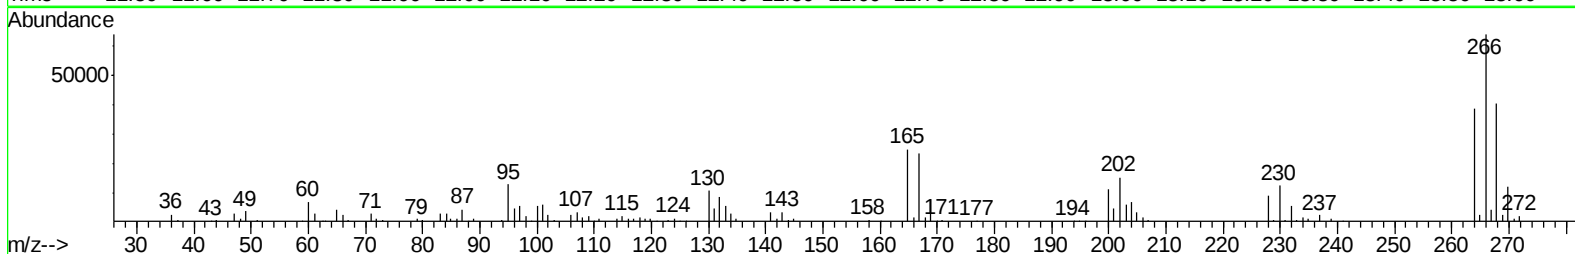


Data Path : Z:\HPCHEM1\BNA F\Data\BF120915\
Data File : BF083635.D
Acq On : 9 Dec 2015 12:42
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 07:03:06 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

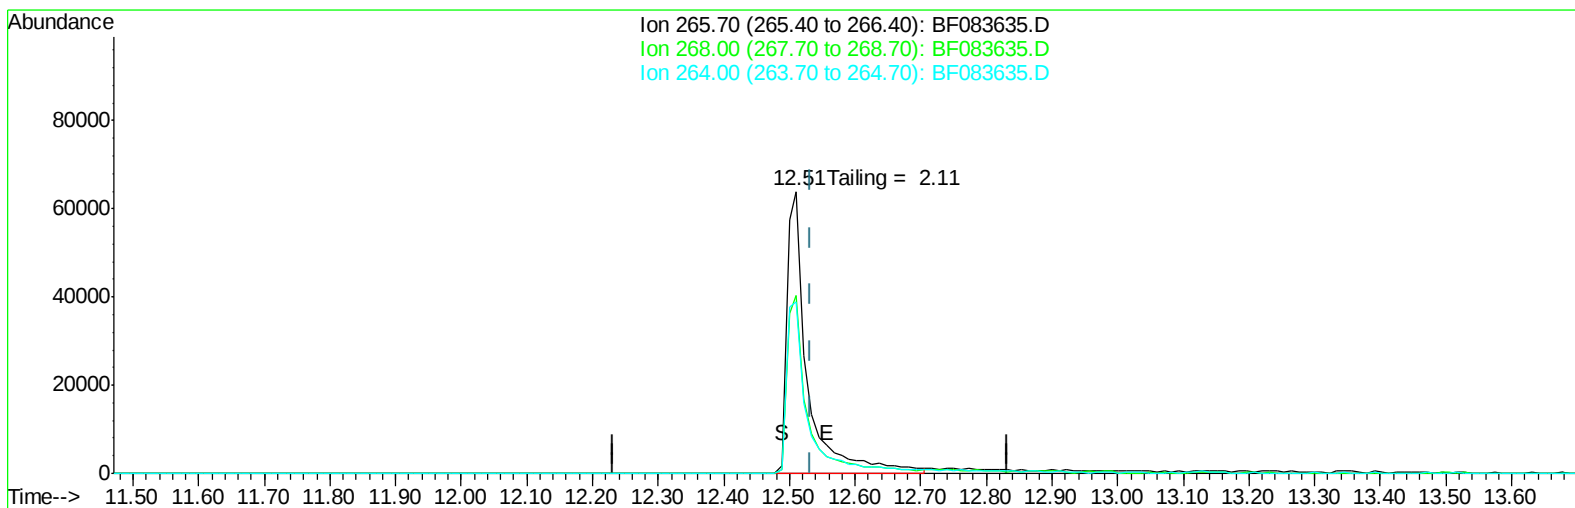

TIC: BF083635.D

(69) Pentachlorophenol (C)




12.511min (-0.022) 0.00ng

response 143227

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	63.05
264.00	64.30	60.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF120915\
Data File : BF083635.D
Acq On : 9 Dec 2015 12:42
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 07:03:06 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

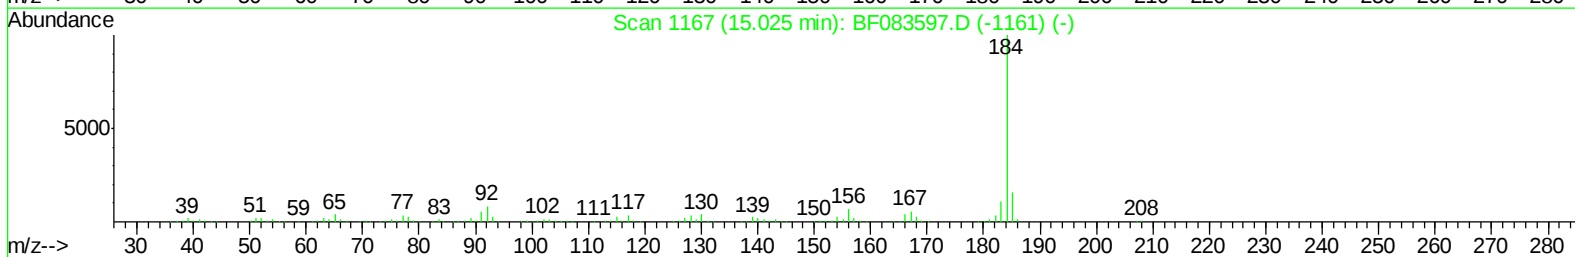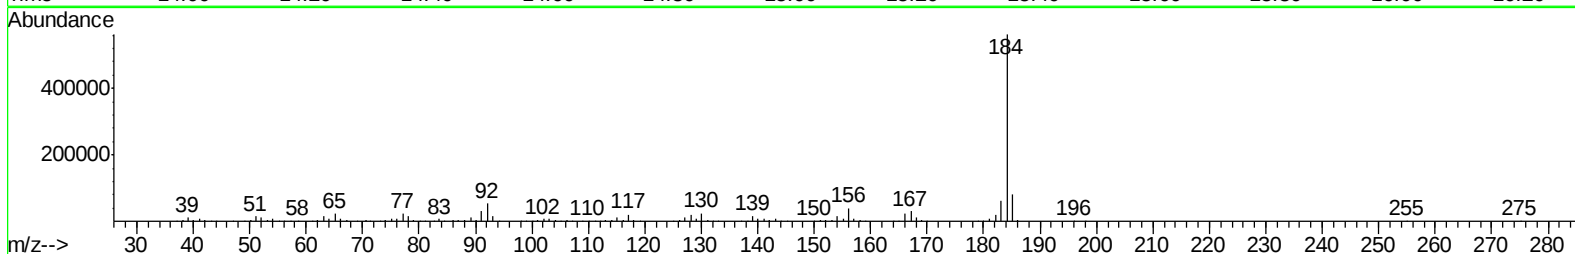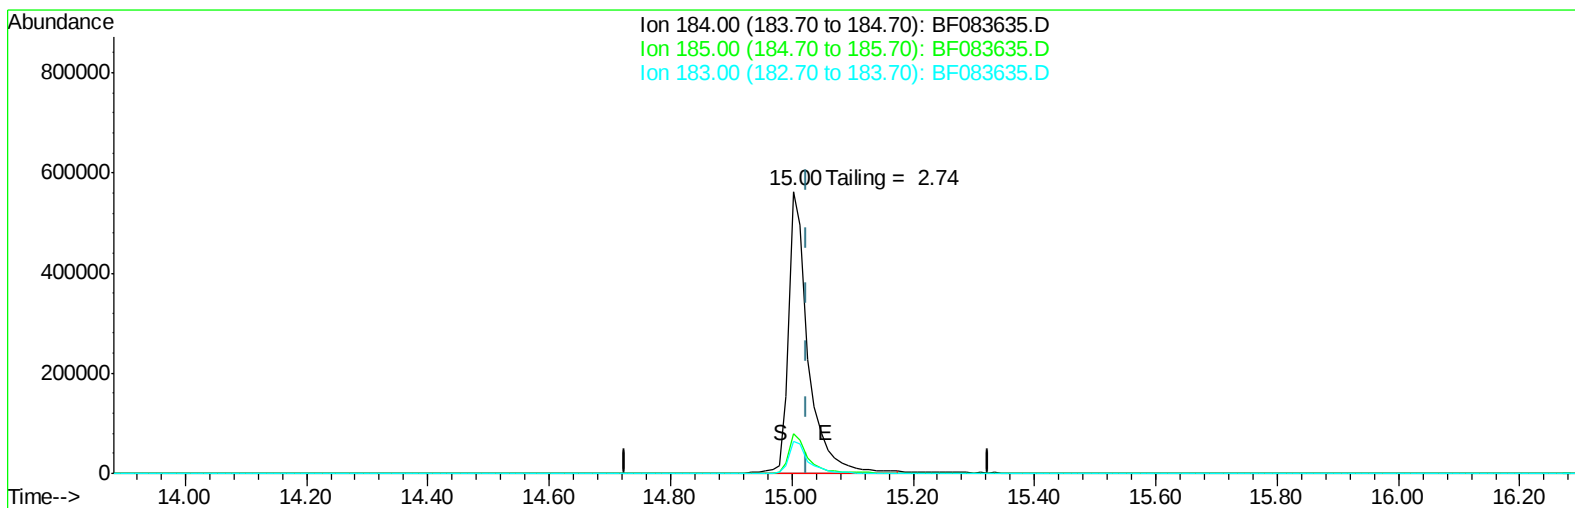

TIC: BF083635.D

(76) Benzidine

15.002min (-0.023) 16722.09ng

response 1280572

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.32
183.00	11.20	11.25
0.00	0.00	0.00