
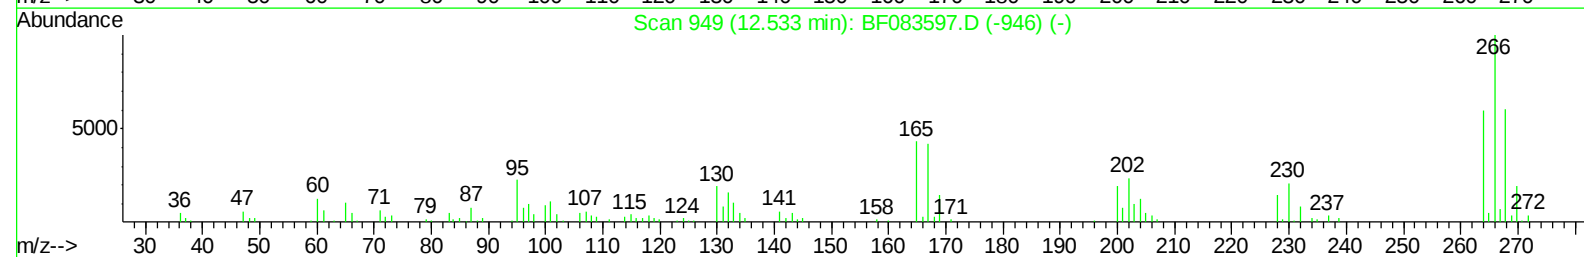
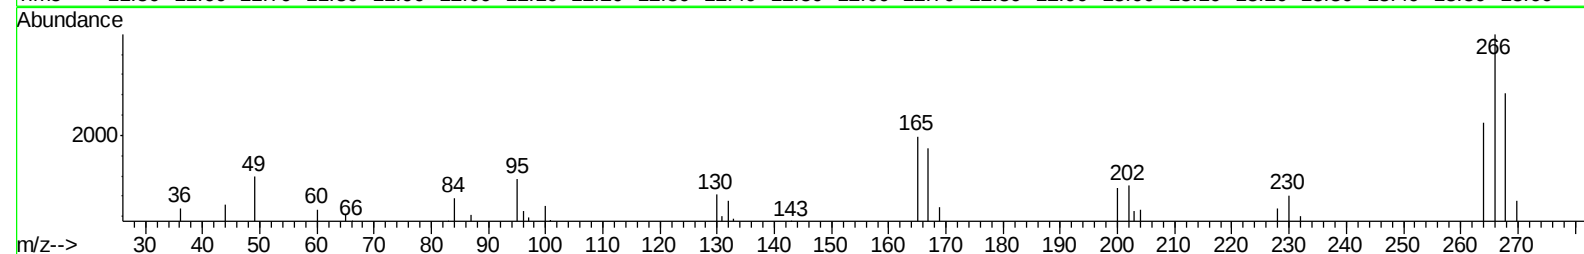


Data Path : Z:\HPCHEM1\BNA F\Data\BF120915\
Data File : BF083658.D
Acq On : 10 Dec 2015 1:16
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 07:00:35 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

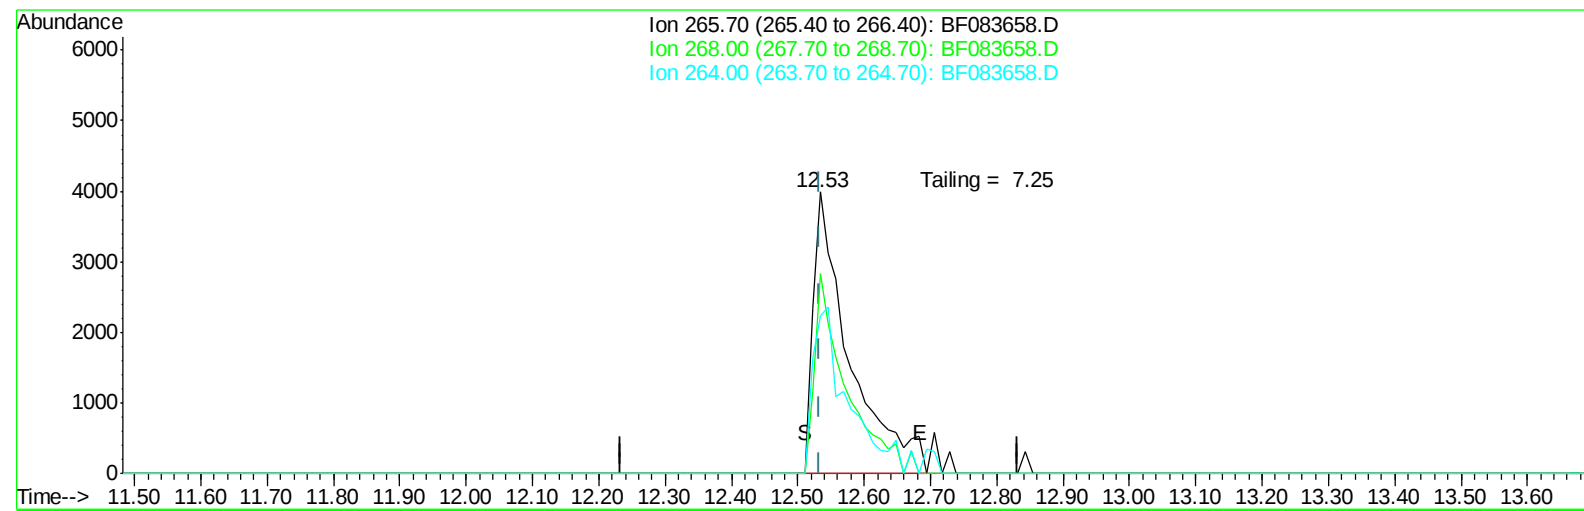

TIC: BF083658.D

(69) Pentachlorophenol (C)




12.534min (+0.001) 0.00ng

response 15036

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	70.89
264.00	64.30	56.06
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF120915\
Data File : BF083658.D
Acq On : 10 Dec 2015 1:16
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 07:00:35 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

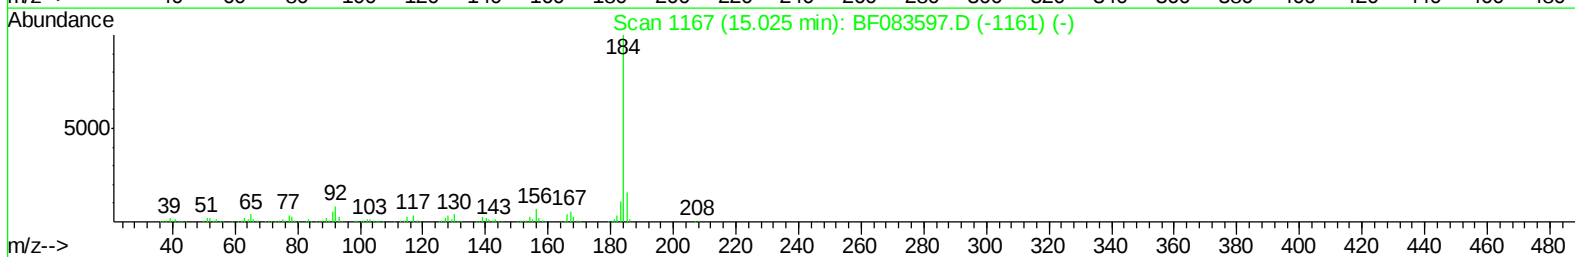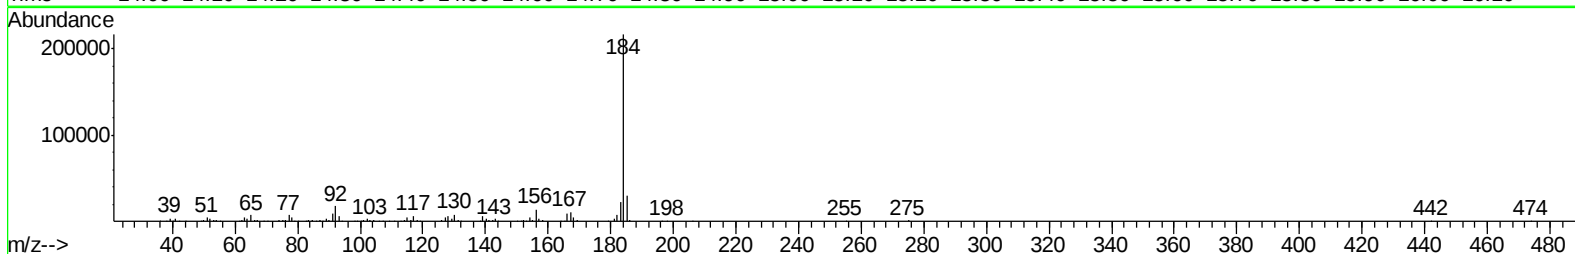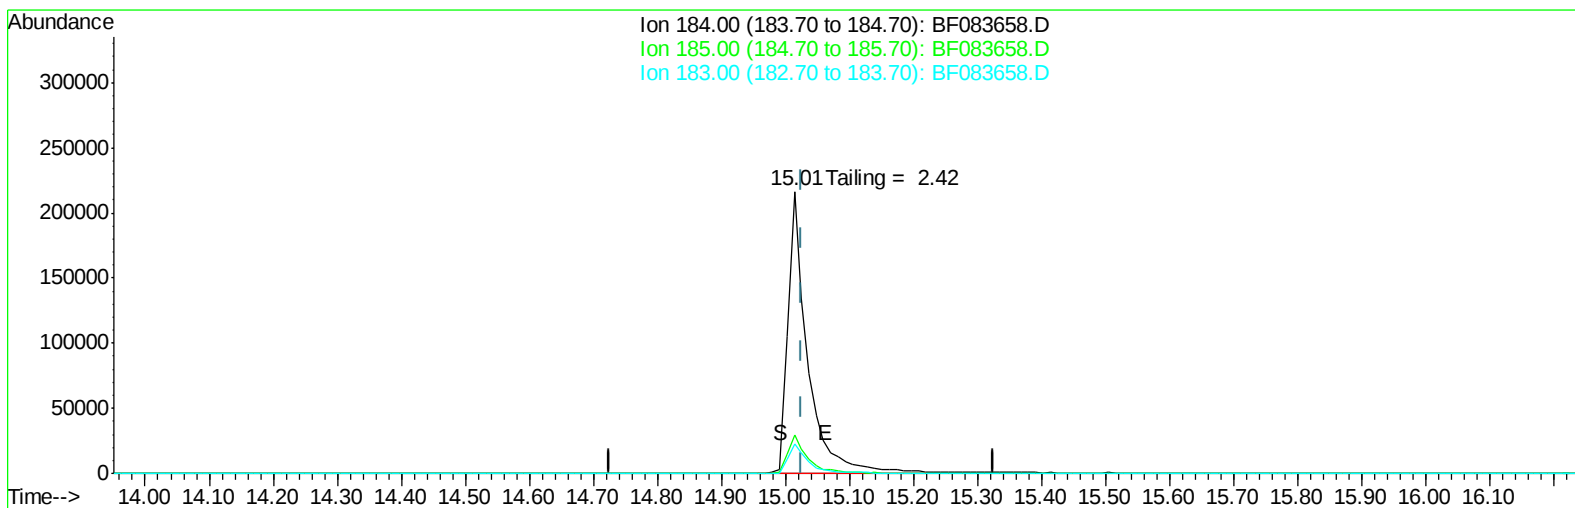

TIC: BF083658.D

(76) Benzidine

15.014min (-0.011) 0.00ng

response 469314

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.62
183.00	11.20	10.56
0.00	0.00	0.00