

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120915\
 Data File : BF083650.D
 Acq On : 9 Dec 2015 20:31
 Operator : UM/IZ
 Sample : G4691-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NC-HC-006

Quant Time: Dec 10 03:18:07 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 00:23:35 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.68	152	149557	20.00	ng	-0.02
21) Naphthalene-d8	7.57	136	582692	20.00	ng	-0.03
38) Acenaphthene-d10	10.36	164	267704	20.00	ng	-0.02
63) Phenanthrene-d10	12.76	188	421503	20.00	ng	-0.02
75) Chrysene-d12	16.98	240	340031	20.00	ng	-0.01
86) Perylene-d12	18.61	264	280743	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	3.96	112	1421338	144.14	ng	-0.01
7) Phenol-d6	5.25	99	2066771	156.87	ng	-0.02
23) Nitrobenzene-d5	6.51	82	1221636	97.83	ng	-0.02
41) 2,4,6-Tribromophenol	11.66	330	300313	125.92	ng	-0.02
44) 2-Fluorobiphenyl	9.32	172	1850413	97.28	ng	-0.02
78) Terphenyl-d14	15.39	244	1275222	88.24	ng	-0.02
Target Compounds						
49) Dimethylphthalate	10.01	163	261039	12.25	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120915\
Data File : BF083650.D
Acq On : 9 Dec 2015 20:31
Operator : UM/IZ
Sample : G4691-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NC-HC-006

Quant Time: Dec 10 03:18:07 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

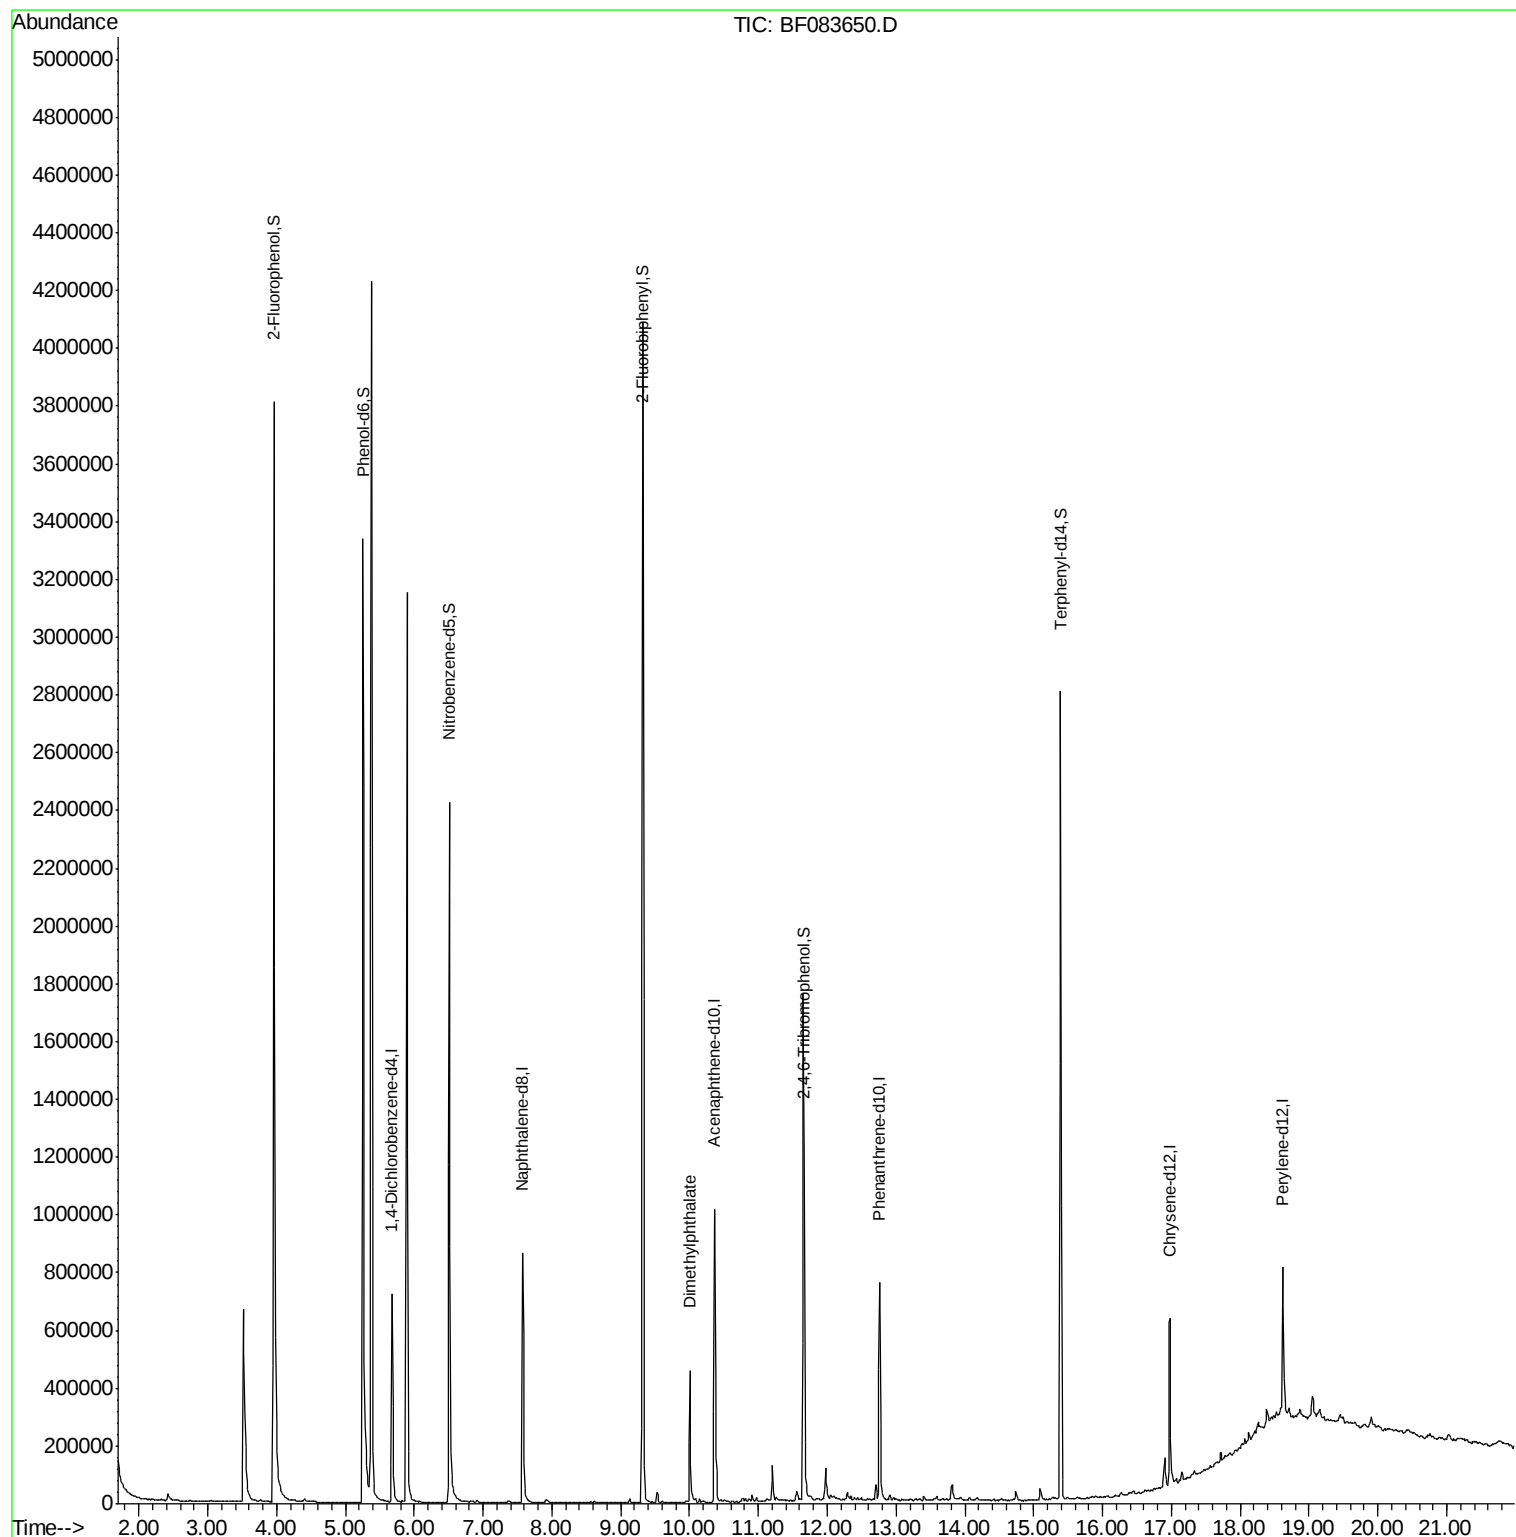

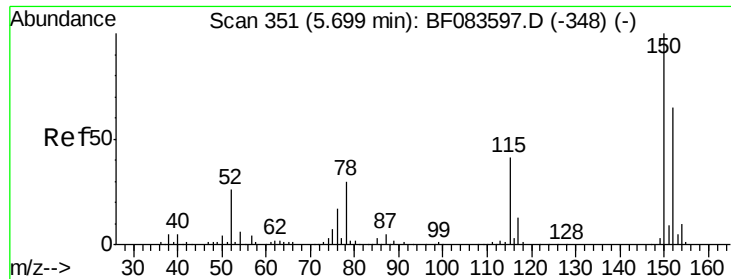


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.68 min Scan# 349
Delta R.T. -0.02 min
Lab File: BF083650.D
Acq: 9 Dec 2015 20:31

Instrument :
BNA_F
ClientSampleId :
NC-HC-006

Tot Ion:152 Resp: 149557
Ion Ratio Lower Upper
152 100
150 157.5 126.5 189.7
115 63.4 52.3 78.5

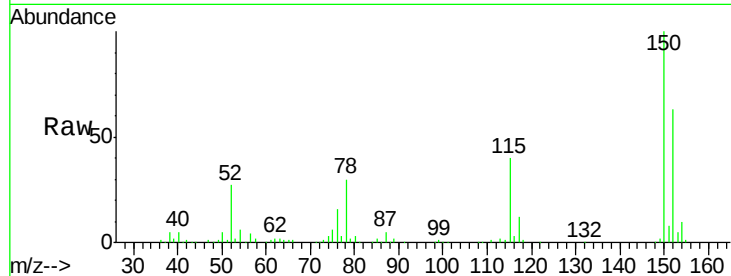


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

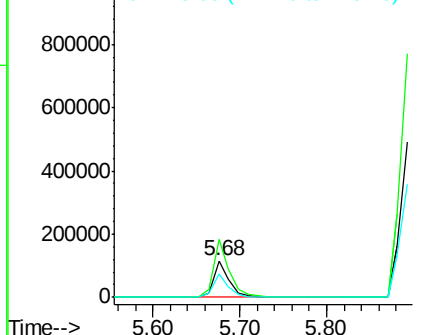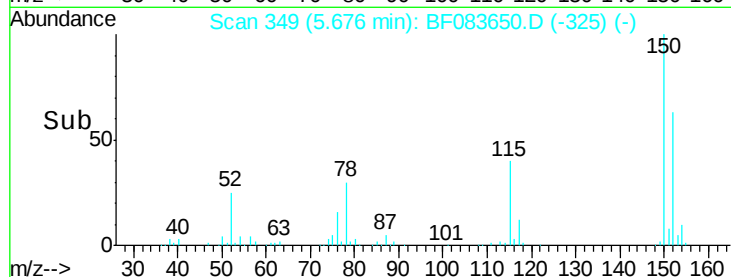



#5


2-Fluorophenol
Concen: 144.14 ng
RT: 3.96 min Scan# 199
Delta R.T. -0.01 min
Lab File: BF083650.D
Acq: 9 Dec 2015 20:31

Tgt Ion:112 Resp: 1421338
Ion Ratio Lower Upper
112 100
64 70.6 50.5 75.7
63 36.5 25.8 38.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

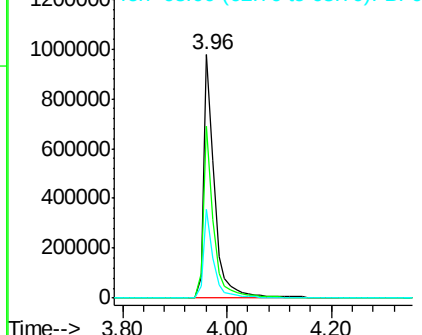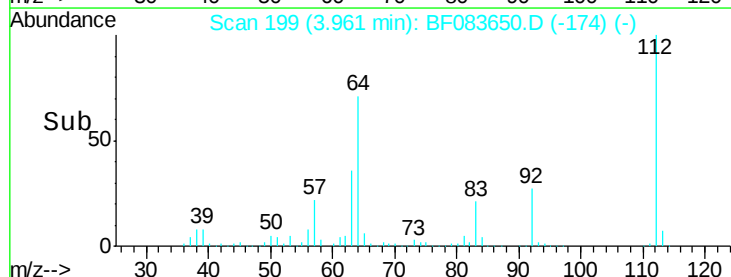

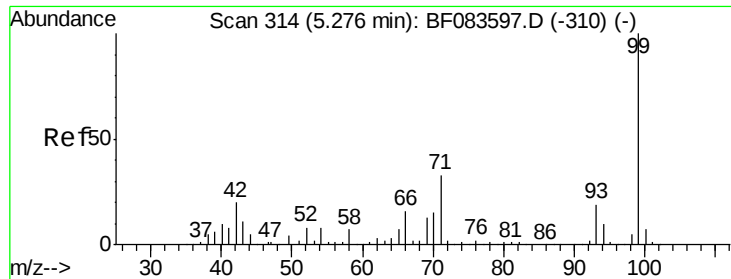

#7

Phenol-d6

Concen: 156.87 ng

RT: 5.25 min Scan# 312

Delta R.T. -0.02 min

Lab File: BF083650.D

Acq: 9 Dec 2015 20:31

Instrument :

BNA_F

ClientSampleId :

NC-HC-006


Tot Ion: 99 Resp: 2066771

Ion Ratio Lower Upper

99 100

42 21.4 17.3 25.9




71 35.2 26.6 40.0

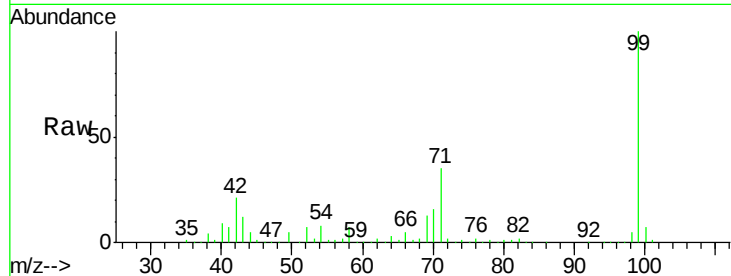

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

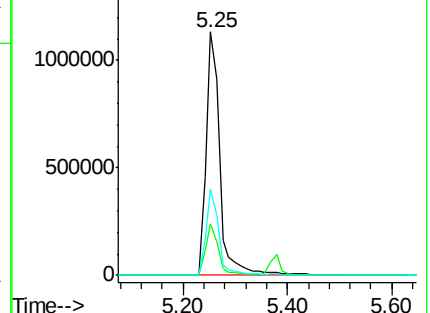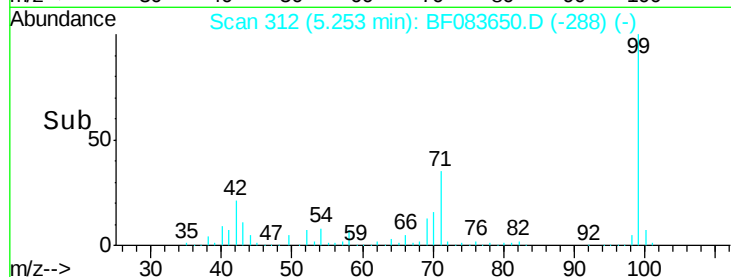

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.57 min Scan# 515

Delta R.T. -0.03 min

Lab File: BF083650.D

Acq: 9 Dec 2015 20:31

Tgt Ion: 136 Resp: 582692


Ion Ratio Lower Upper

136 100

137 11.8 8.7 13.1

54 11.4 7.8 11.6

68 7.6 5.7 8.5






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



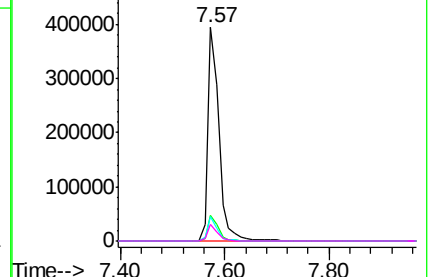
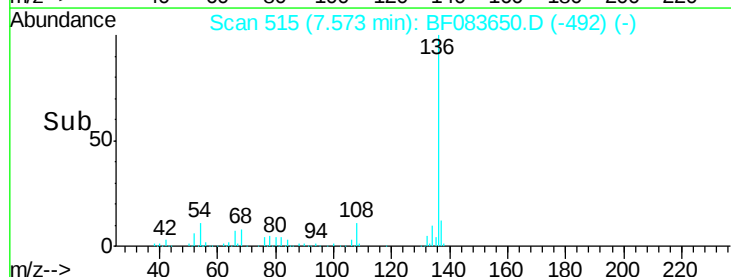


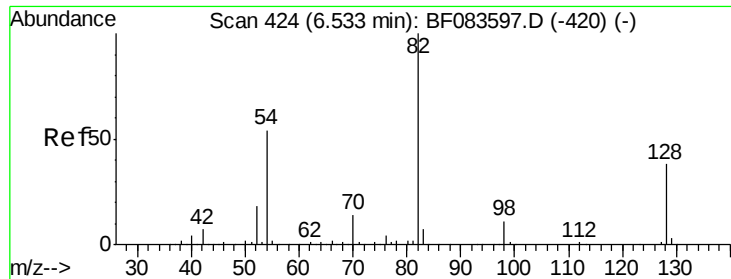

#23
 Nitrobenzene-d5
 Concen: 97.83 ng
 RT: 6.51 min Scan# 422
 Delta R.T. -0.02 min
 Lab File: BF083650.D
 Acq: 9 Dec 2015 20:31




Instrument :
 BNA_F
 ClientSampled :
 NC-HC-006


Tot Ion: 82 Resp: 1221636
 Ion Ratio Lower Upper
 82 100
 128 38.3 30.7 46.1
 54 55.2 42.5 63.7

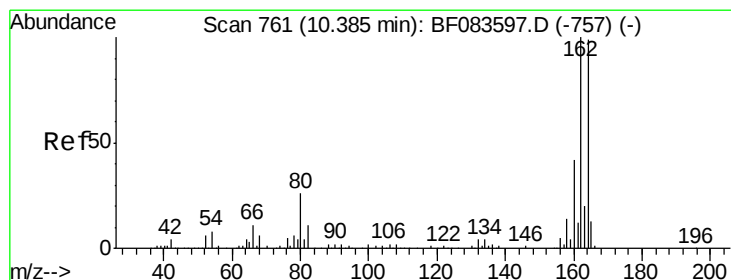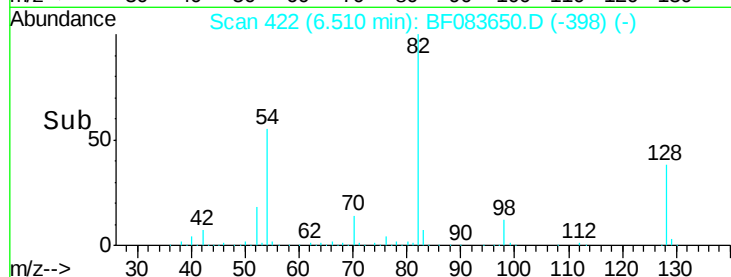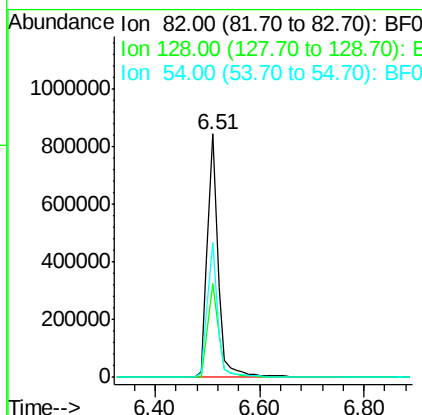

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.36 min Scan# 759
 Delta R.T. -0.02 min
 Lab File: BF083650.D
 Acq: 9 Dec 2015 20:31

Tgt Ion: 164 Resp: 267704
 Ion Ratio Lower Upper
 164 100
 162 102.8 78.8 118.2
 160 44.6 33.4 50.2


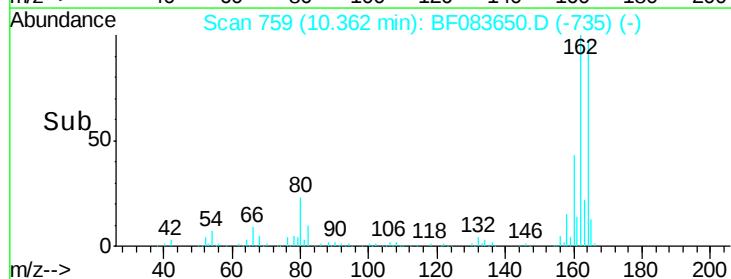
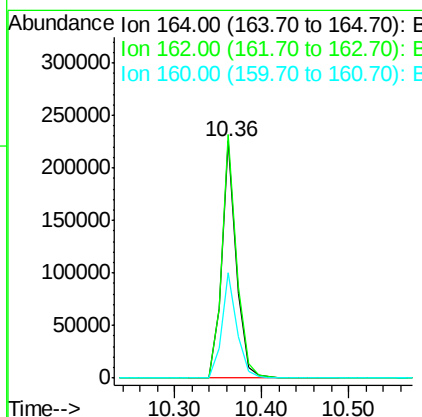
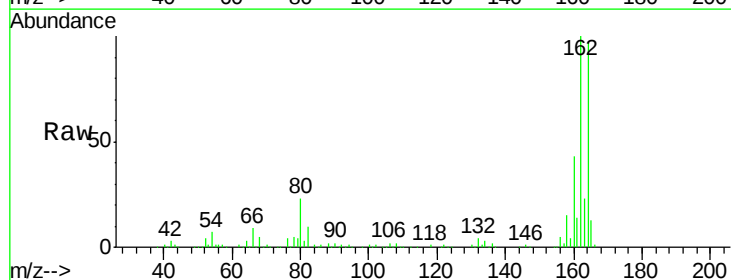


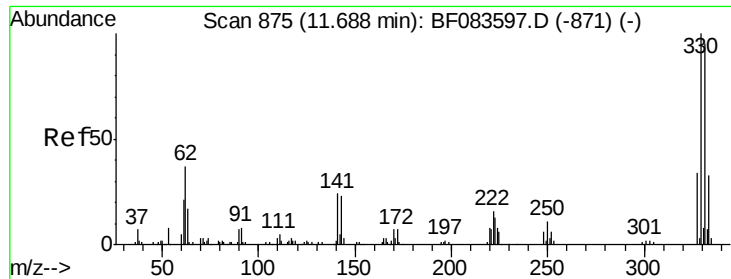

#41
 2,4,6-Tribromophenol
 Concen: 125.92 ng
 RT: 11.66 min Scan# 873
 Delta R.T. -0.02 min
 Lab File: BF083650.D
 Acq: 9 Dec 2015 20:31




Instrument :
 BNA_F
 ClientSampleId :
 NC-HC-006


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	0.0	0.0#
141	38.3	0.0	0.0#

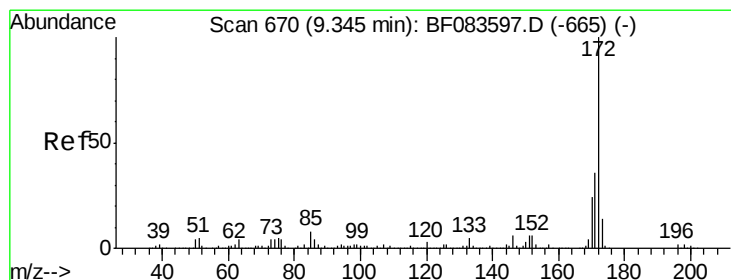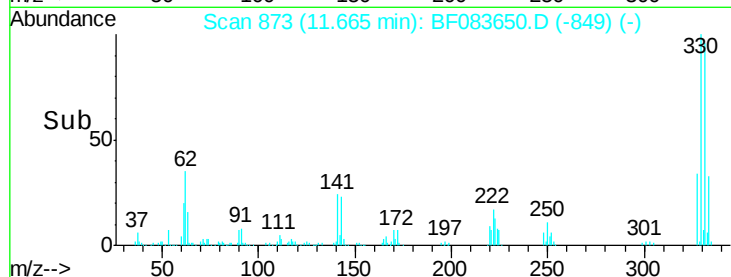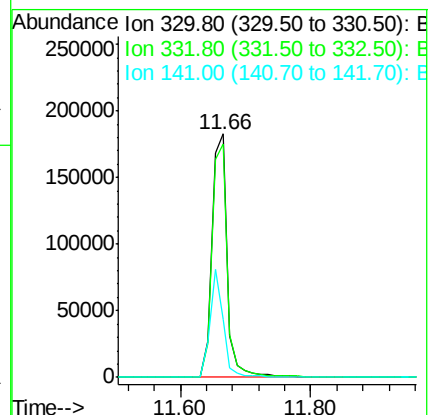

#44
 2-Fluorobiphenyl
 Concen: 97.28 ng
 RT: 9.32 min Scan# 668
 Delta R.T. -0.02 min
 Lab File: BF083650.D
 Acq: 9 Dec 2015 20:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	28.6	42.8
170	25.0	19.4	29.0

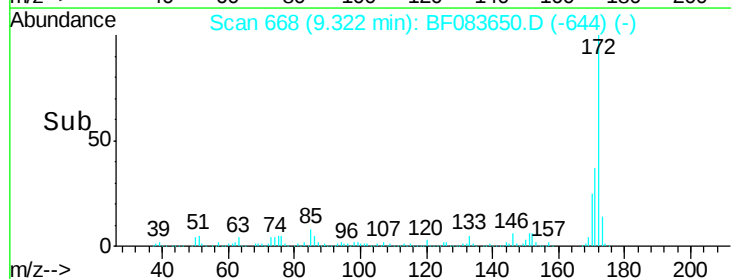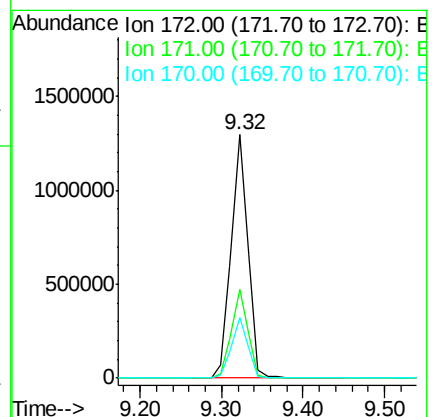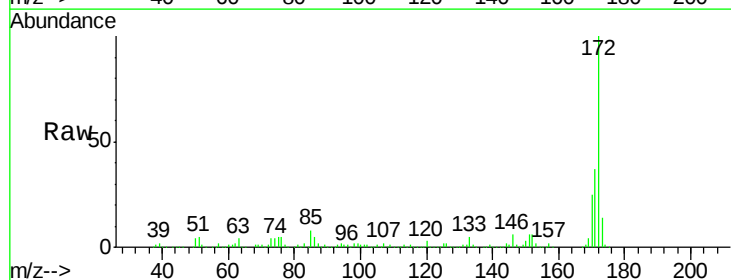

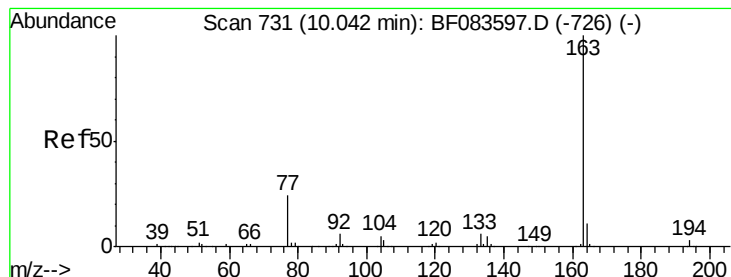

#49

Dimethylphthalate

Concen: 12.25 ng

RT: 10.01 min Scan# 728

Delta R.T. -0.03 min

Lab File: BF083650.D

Acq: 9 Dec 2015 20:31

Instrument :

BNA_F

ClientSampled :

NC-HC-006


Tot Ion:163 Resp: 261039

Ion Ratio Lower Upper

163 100

194 3.4 2.8 4.2




164 10.0 8.6 13.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

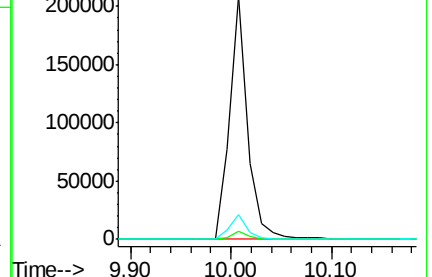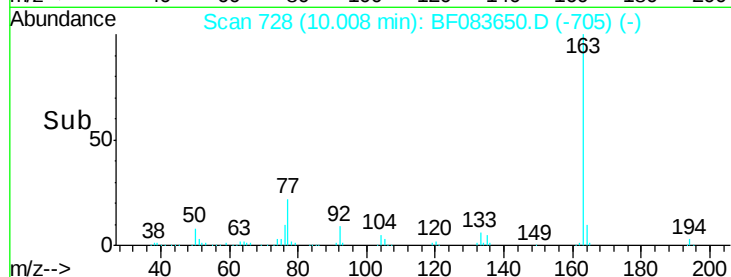

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.76 min Scan# 969

Delta R.T. -0.02 min

Lab File: BF083650.D

Acq: 9 Dec 2015 20:31


Tgt Ion:188 Resp: 421503

Ion Ratio Lower Upper

188 100

94 9.8 9.4 14.2



80 11.0 10.6 16.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

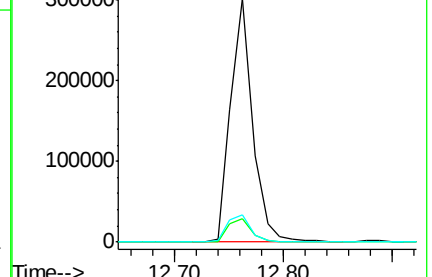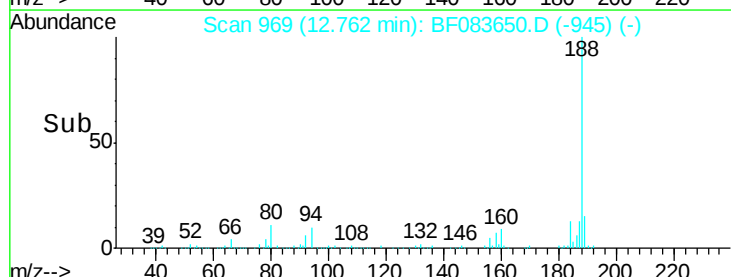

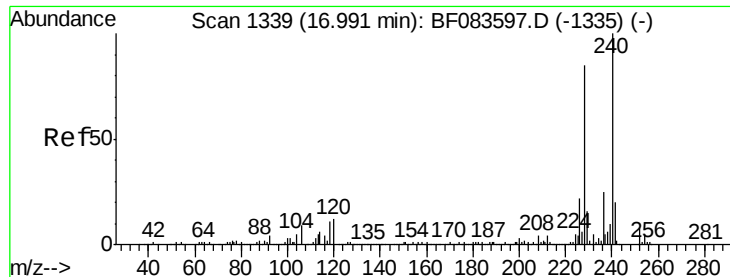

#75

Chrysene-d12

Concen: 20.00 ng

RT: 16.98 min Scan# 1338

Delta R.T. -0.01 min

Lab File: BF083650.D

Acq: 9 Dec 2015 20:31

Instrument :

BNA_F

ClientSampleId :

NC-HC-006


Tot Ion:240 Resp: 340031

Ion Ratio Lower Upper

240 100

120 8.5 8.1 12.1


236 24.8 20.8 31.2

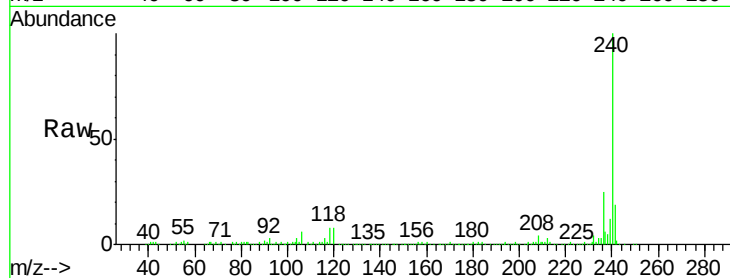



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

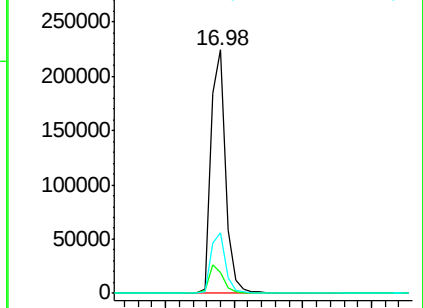

Time-->

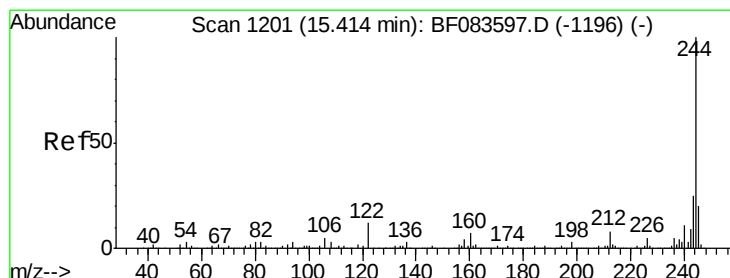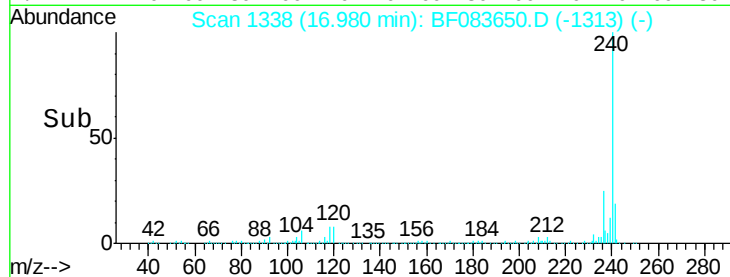

#78

Terphenyl-d14

Concen: 88.24 ng

RT: 15.39 min Scan# 1199

Delta R.T. -0.02 min

Lab File: BF083650.D

Acq: 9 Dec 2015 20:31


Tgt Ion:244 Resp: 1275222

Ion Ratio Lower Upper

244 100

212 7.5 6.1 9.1


122 12.7 11.0 16.6

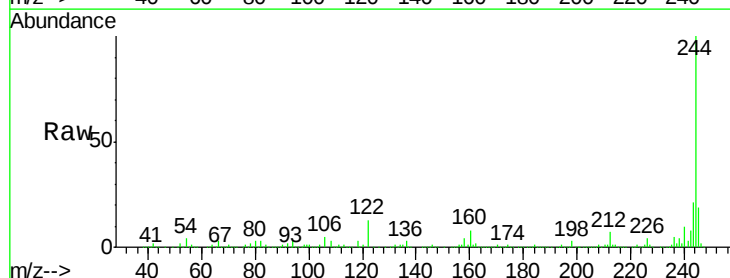


Abundance Ion 244.00 (243.70 to 244.70): E


Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

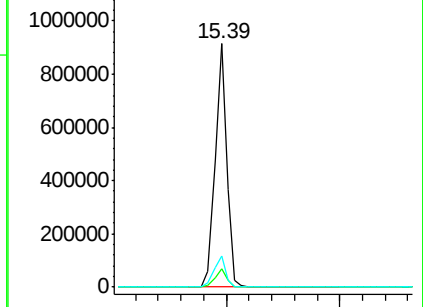

Time-->

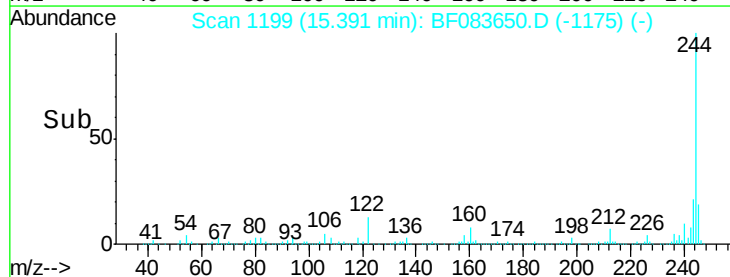


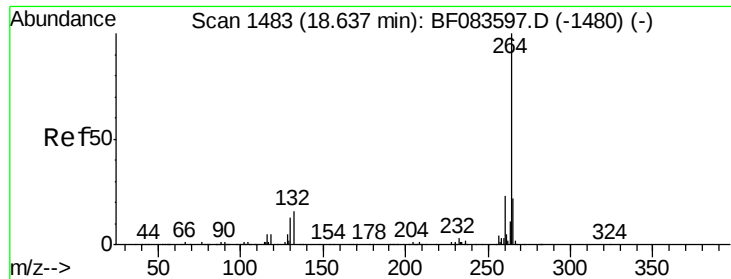

#86
Pervlene-d12
Concen: 20.00 ng
RT: 18.61 min Scan# 1481
Delta R.T. -0.02 min
Lab File: BF083650.D
Acq: 9 Dec 2015 20:31

Instrument :
BNA_F
ClientSampleId :
NC-HC-006

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.4	29.0
265	21.8	17.8	26.6



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

