


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120915\
 Data File : BF083635.D
 Acq On : 9 Dec 2015 12:42
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 00:23:35 2015

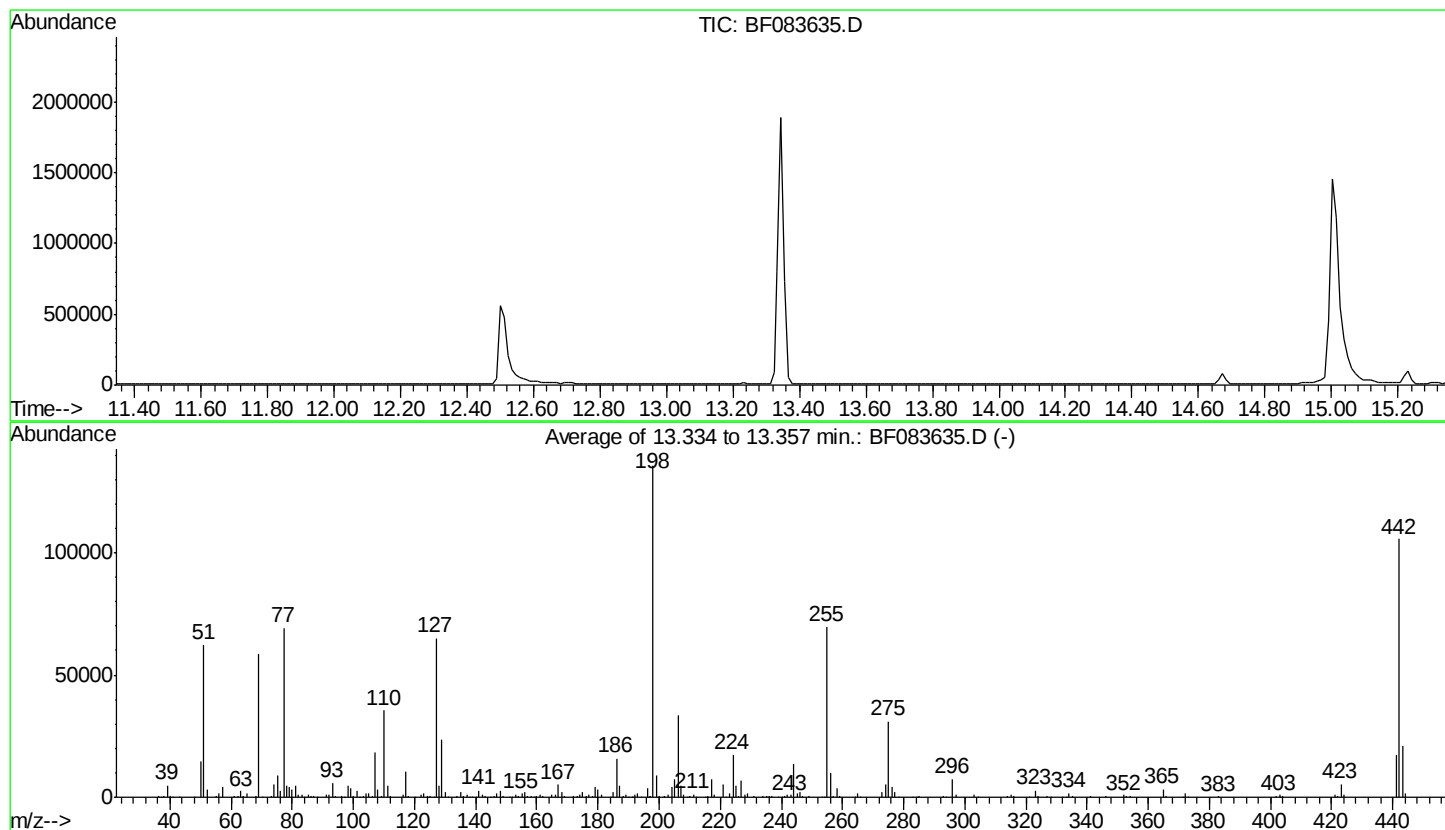

AutoFind: Scans 1019, 1020, 1021; Background Corrected with Scan 1015

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	62573	PASS
68	69	0.00	2	1.3	759	PASS
69	198	0.00	100	43.1	58488	PASS
70	69	0.00	2	0.3	160	PASS
127	198	10	80	48.0	65098	PASS
197	198	0.00	2	0.6	763	PASS
198	198	100	100	100.0	135656	PASS
199	198	5	9	6.7	9039	PASS
275	198	10	60	23.0	31152	PASS
365	198	1	100	2.5	3335	PASS
441	442	0.01	24	16.5	17454	PASS
442	198	50	100	77.9	105696	PASS
443	442	15	24	19.8	20878	PASS