


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120915\
 Data File : BF083658.D
 Acq On : 10 Dec 2015 1:16
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 00:23:35 2015

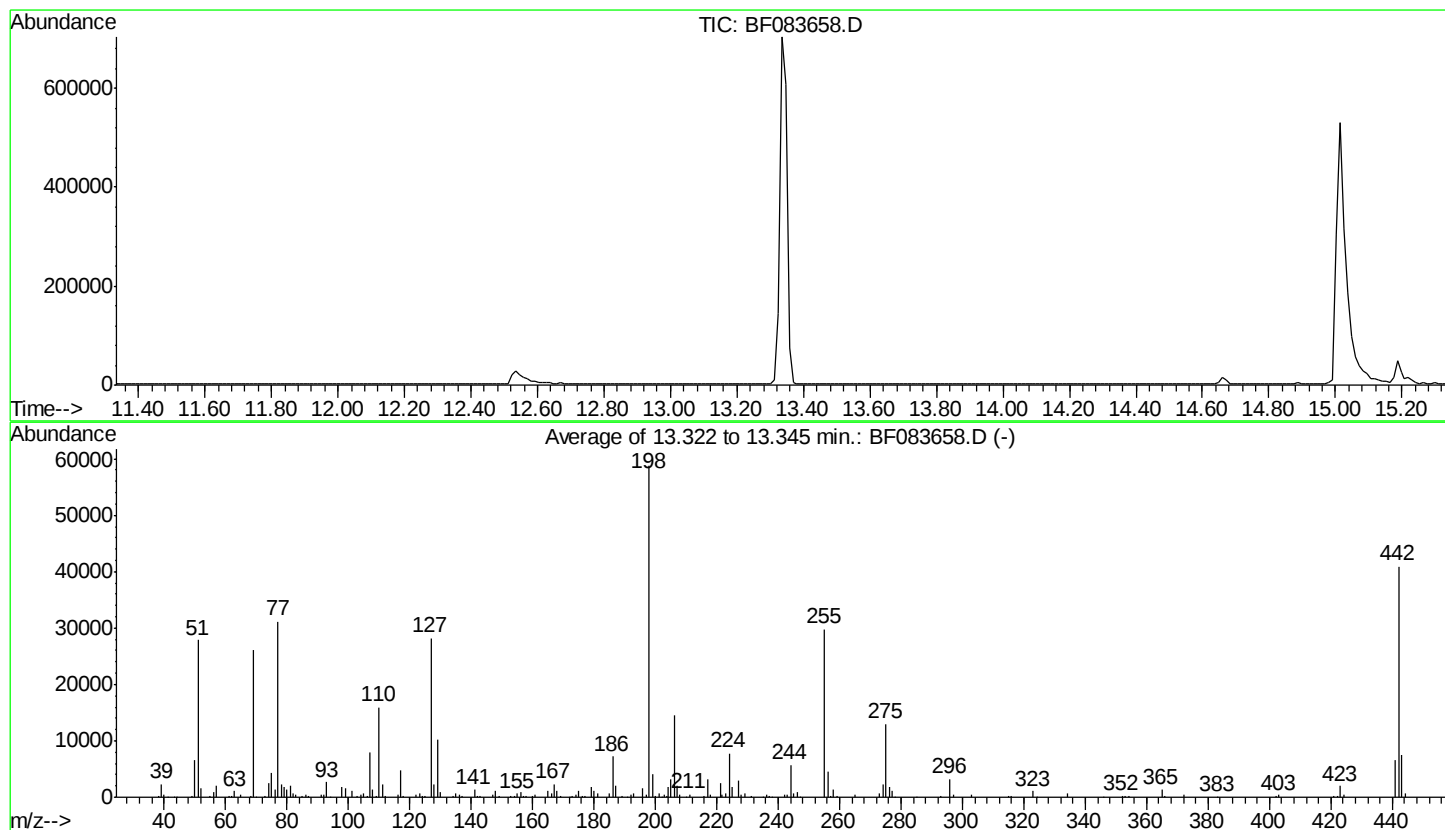

AutoFind: Scans 1018, 1019, 1020; Background Corrected with Scan 1014

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	27840	PASS
68	69	0.00	2	1.3	341	PASS
69	198	0.00	100	44.5	26182	PASS
70	69	0.00	2	0.4	114	PASS
127	198	10	80	48.0	28246	PASS
197	198	0.00	2	0.7	396	PASS
198	198	100	100	100.0	58794	PASS
199	198	5	9	7.1	4183	PASS
275	198	10	60	22.1	12999	PASS
365	198	1	100	2.2	1292	PASS
441	442	0.01	24	16.3	6683	PASS
442	198	50	100	69.6	40917	PASS
443	442	15	24	18.4	7513	PASS