
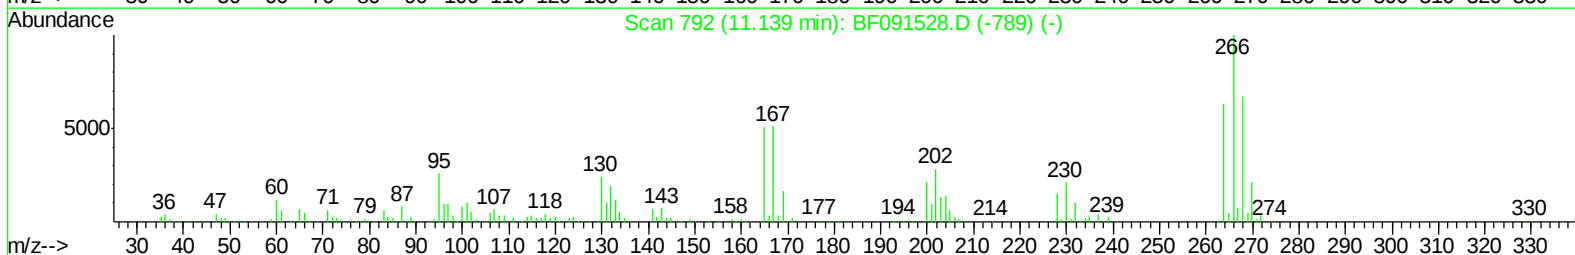
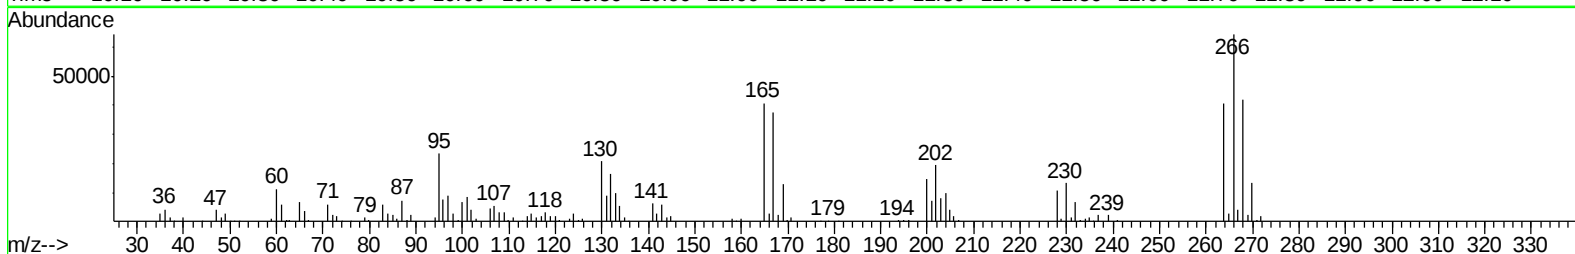


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120916\
Data File : BF091524.D
Acq On : 9 Dec 2016 13:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 07:09:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 19:00:21 2016
Response via : Initial Calibration

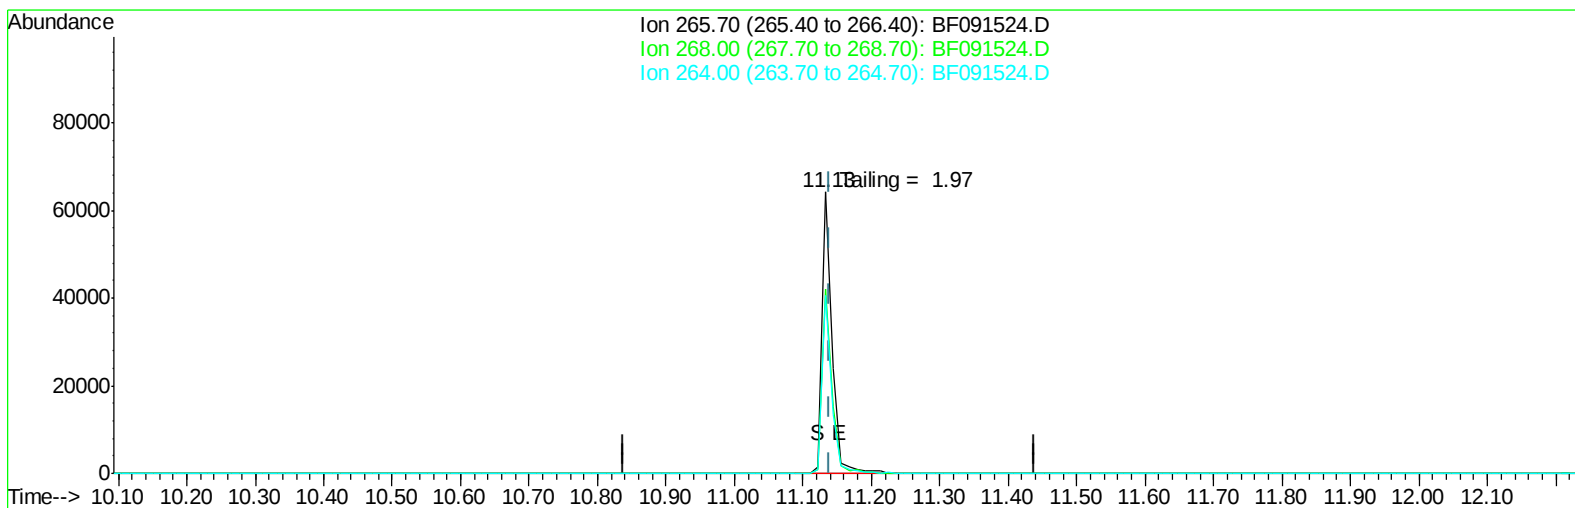

TIC: BF091524.D

(69) Pentachlorophenol (C)




11.134min (-0.006) 21250.87ng

response 65789

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	65.44
264.00	60.20	63.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF120916\
Data File : BF091524.D
Acq On : 9 Dec 2016 13:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 07:09:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 19:00:21 2016
Response via : Initial Calibration

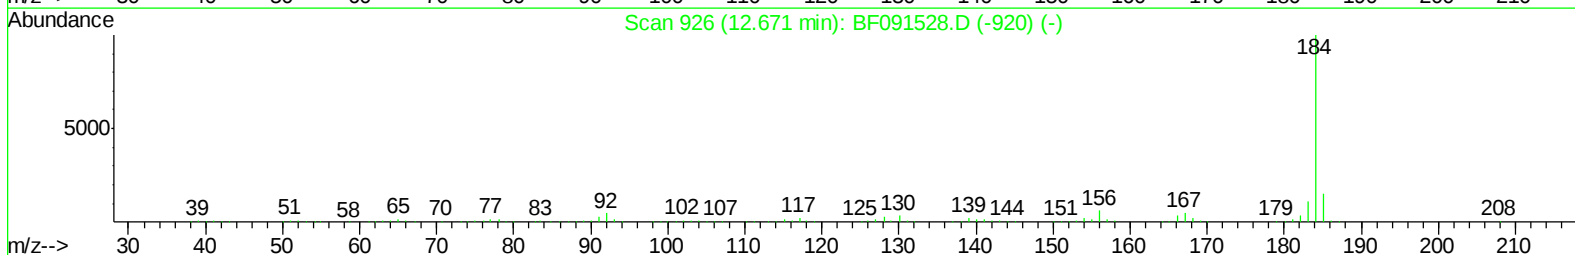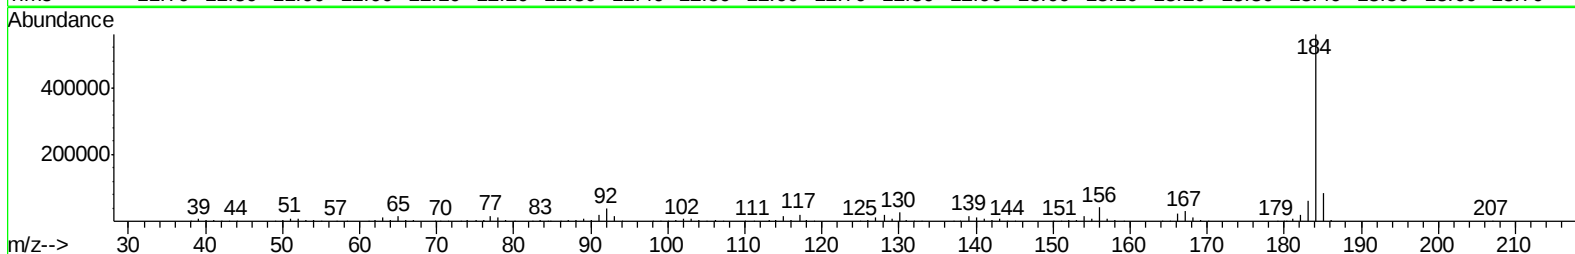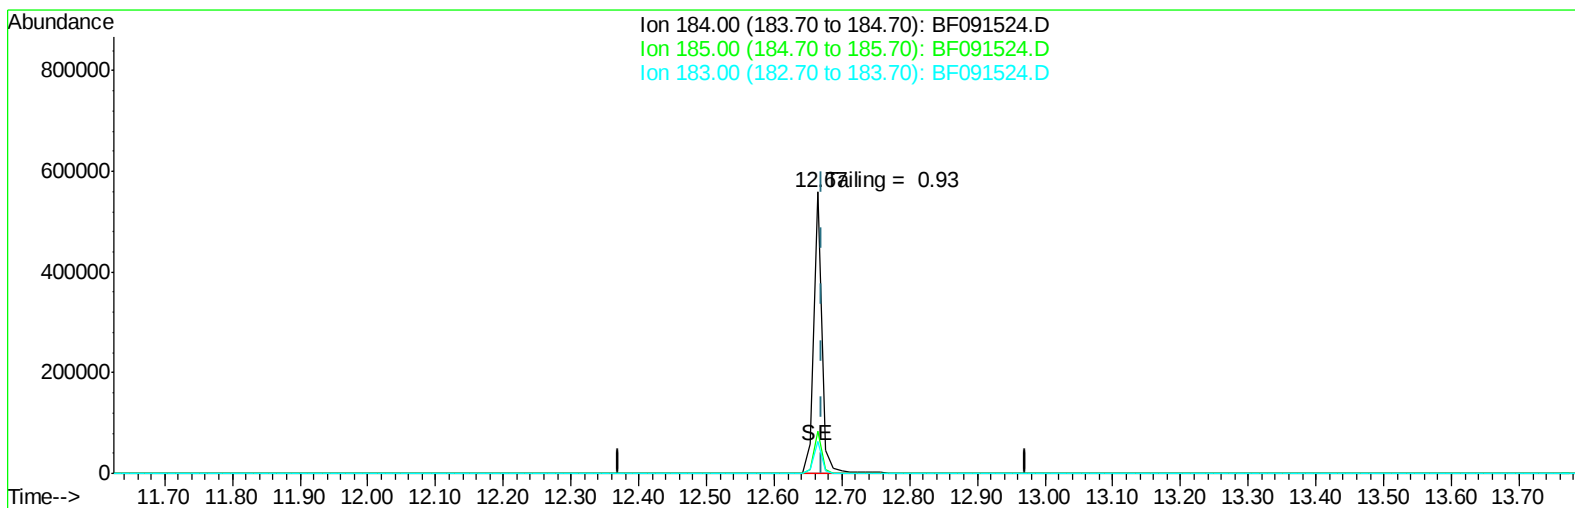

TIC: BF091524.D

(76) Benzidine

12.665min (-0.006) 25594.89ng

response 474841

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.84
183.00	11.10	11.18
0.00	0.00	0.00