




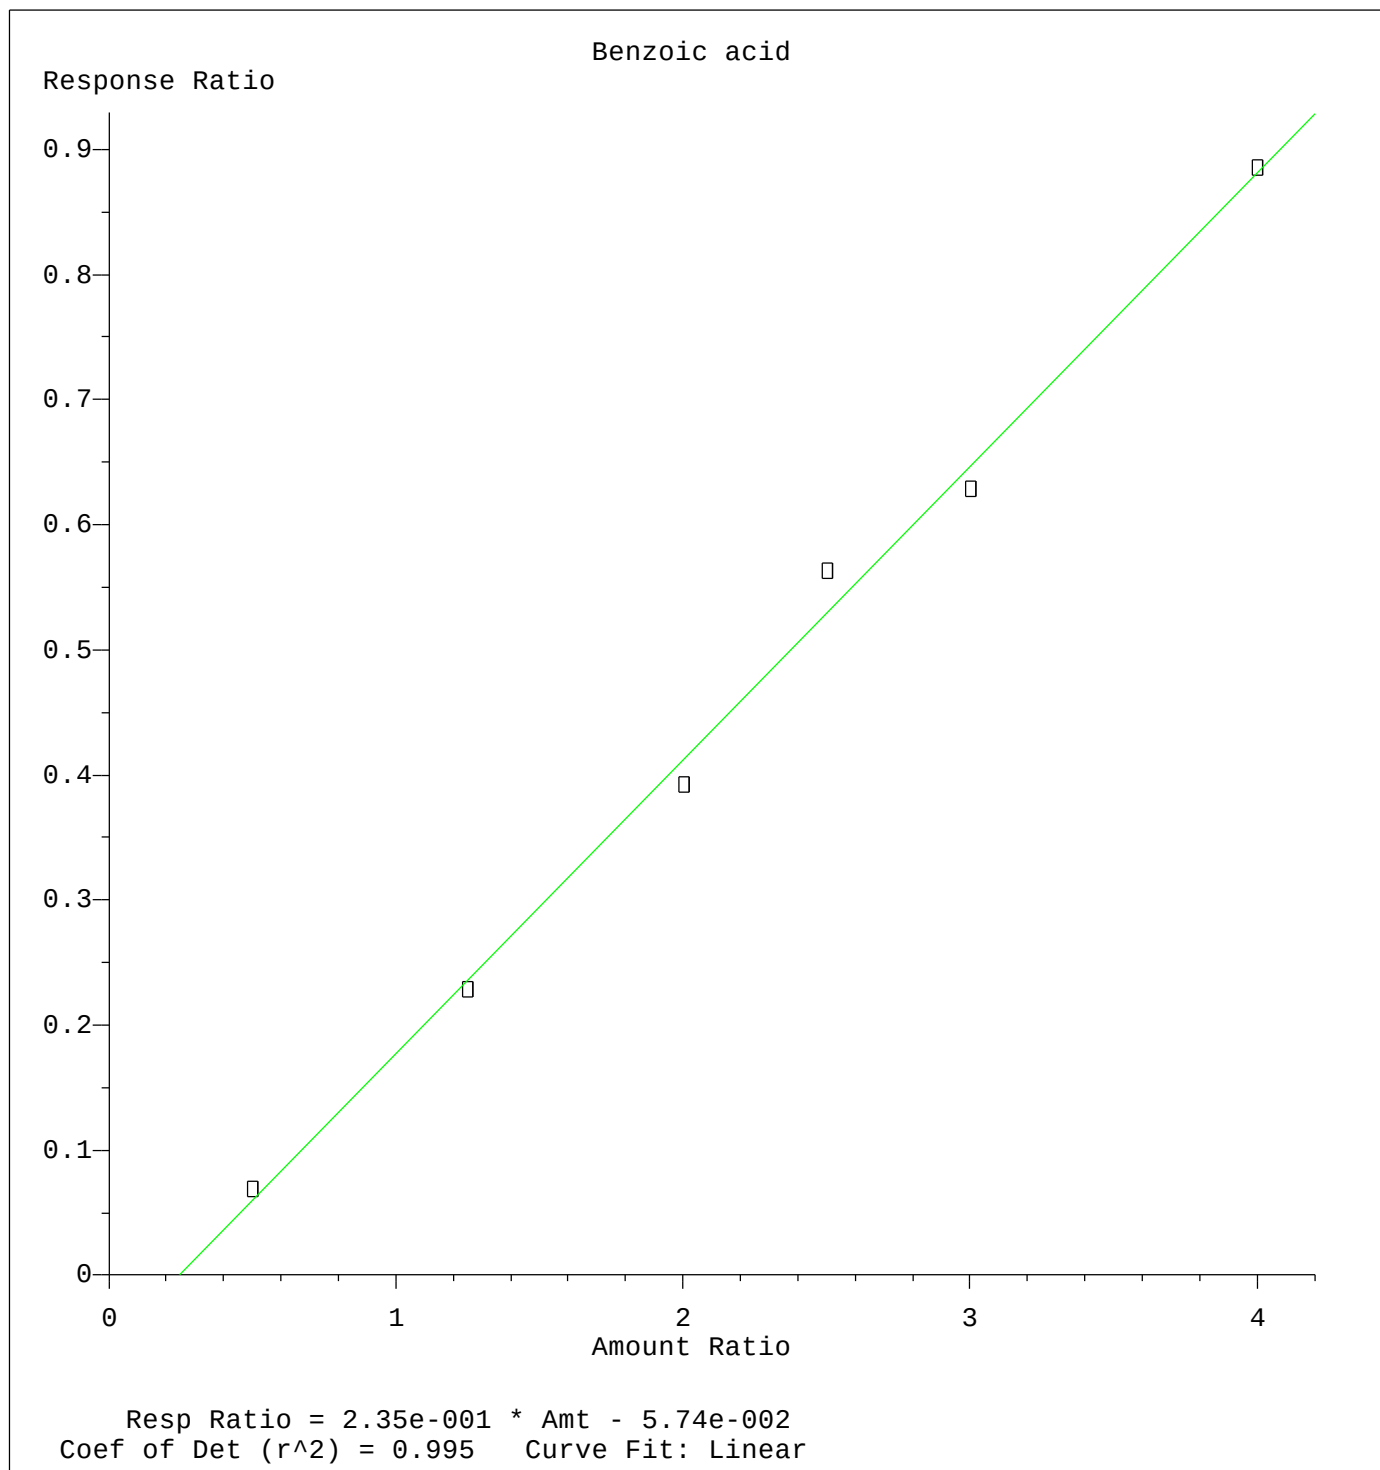

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Calibration Table Last Updated: Fri Dec 16 00:35:41 2016

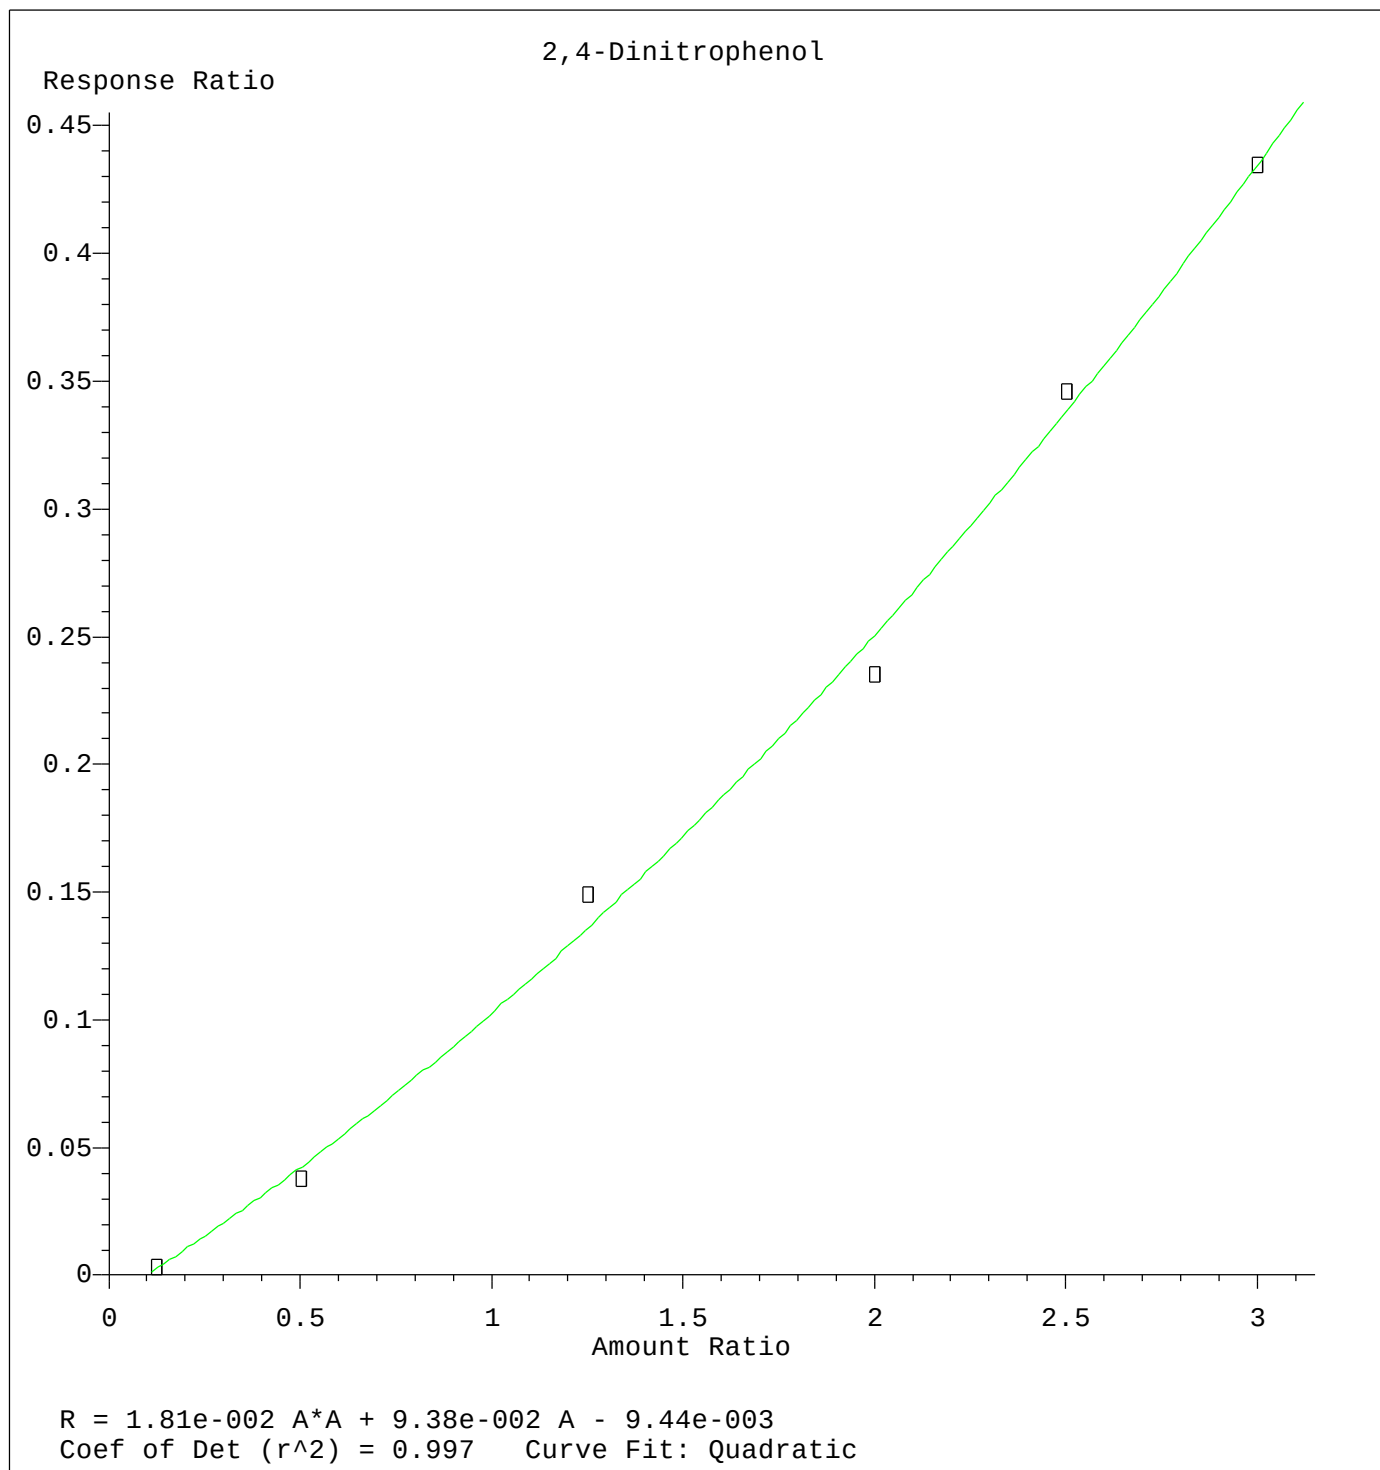


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Calibration Table Last Updated: Fri Dec 16 00:35:41 2016

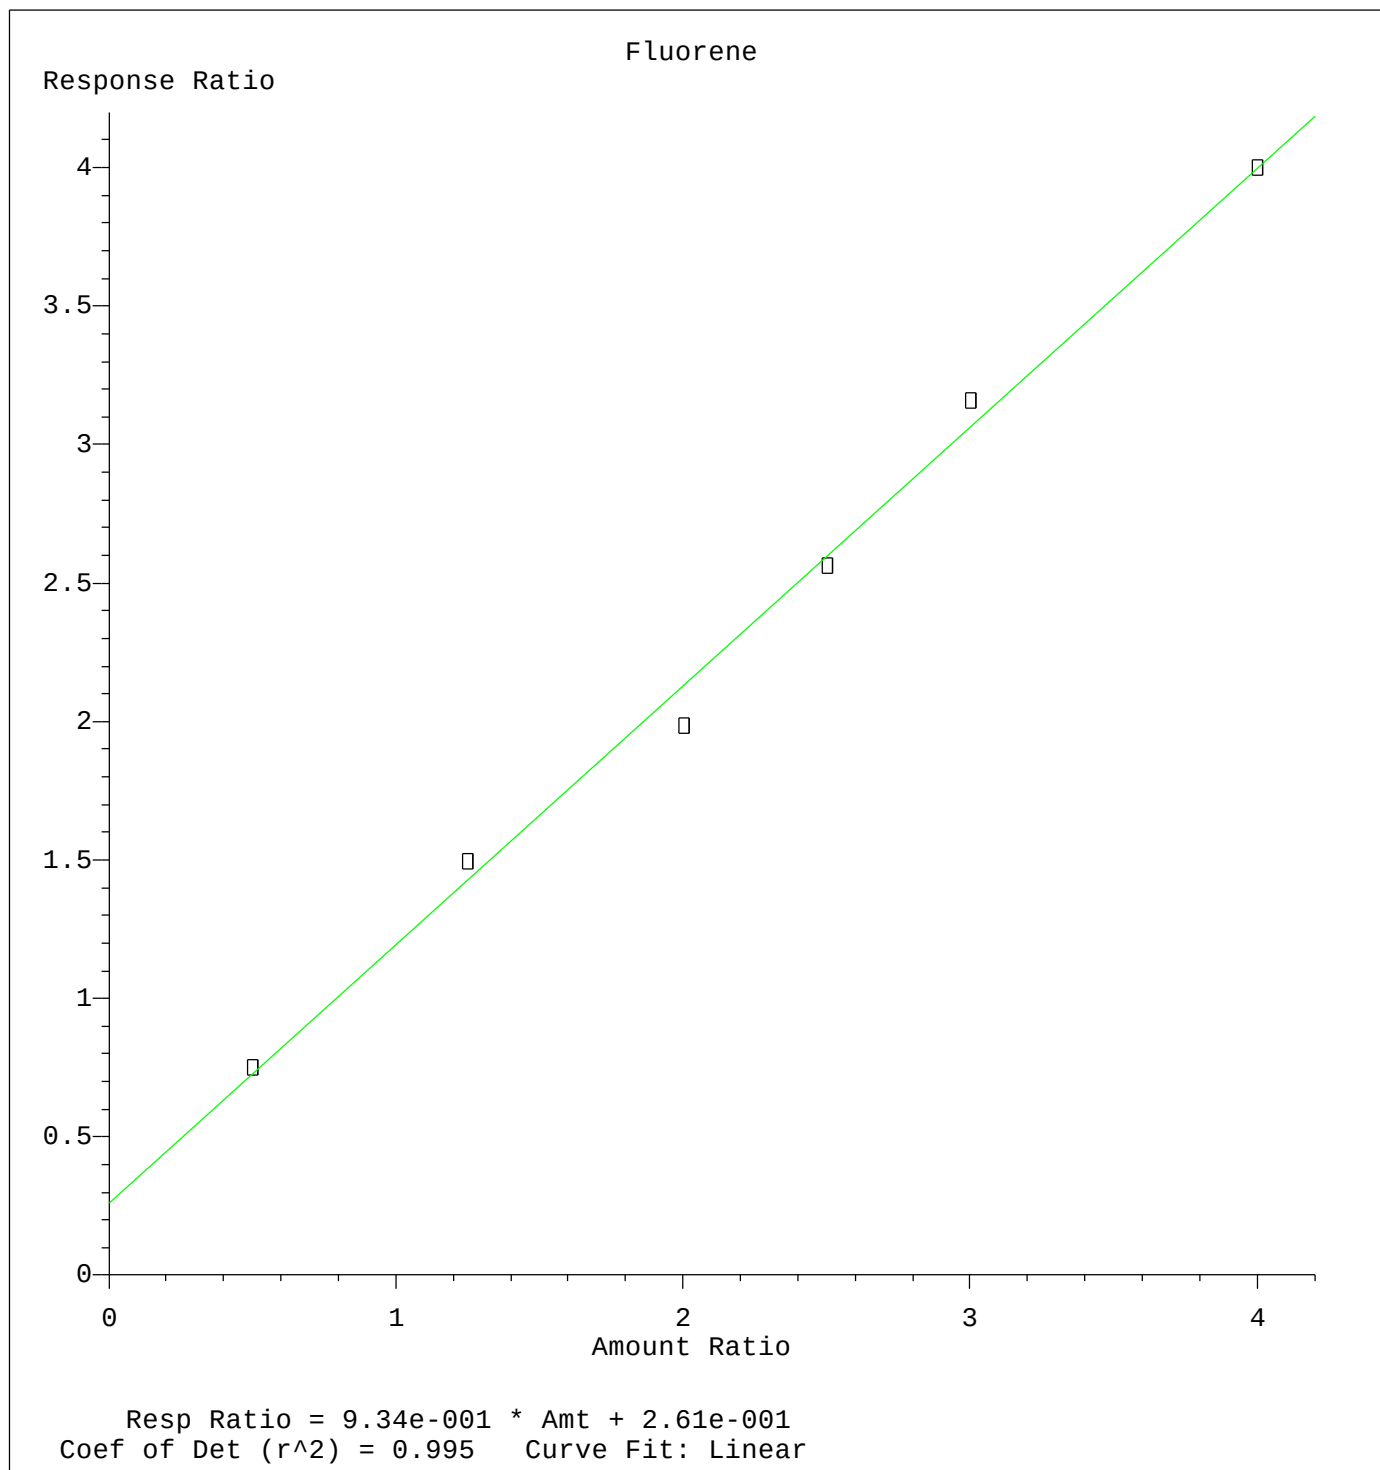


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Calibration Table Last Updated: Fri Dec 16 00:35:41 2016

4,6-Dinitro-2-methylphenol

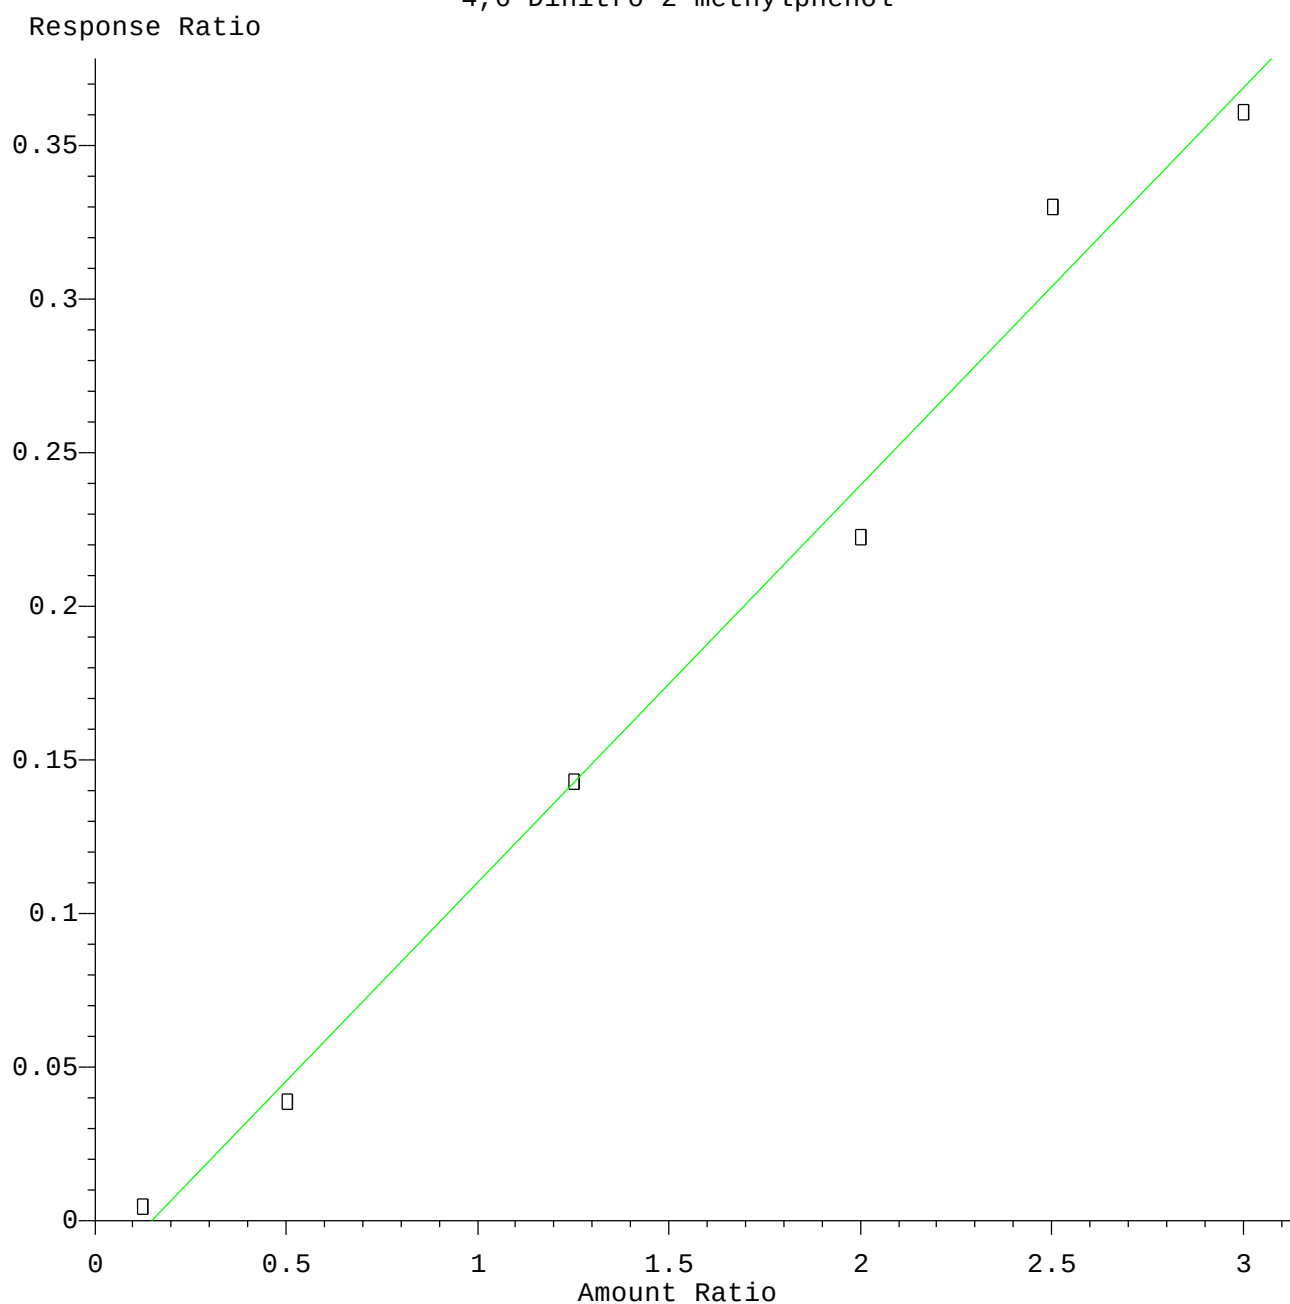

Resp Ratio = $1.29 \times 10^{-1} \times \text{Amt} - 1.91 \times 10^{-2}$
Coef of Det (r^2) = 0.990 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Calibration Table Last Updated: Fri Dec 16 00:35:41 2016

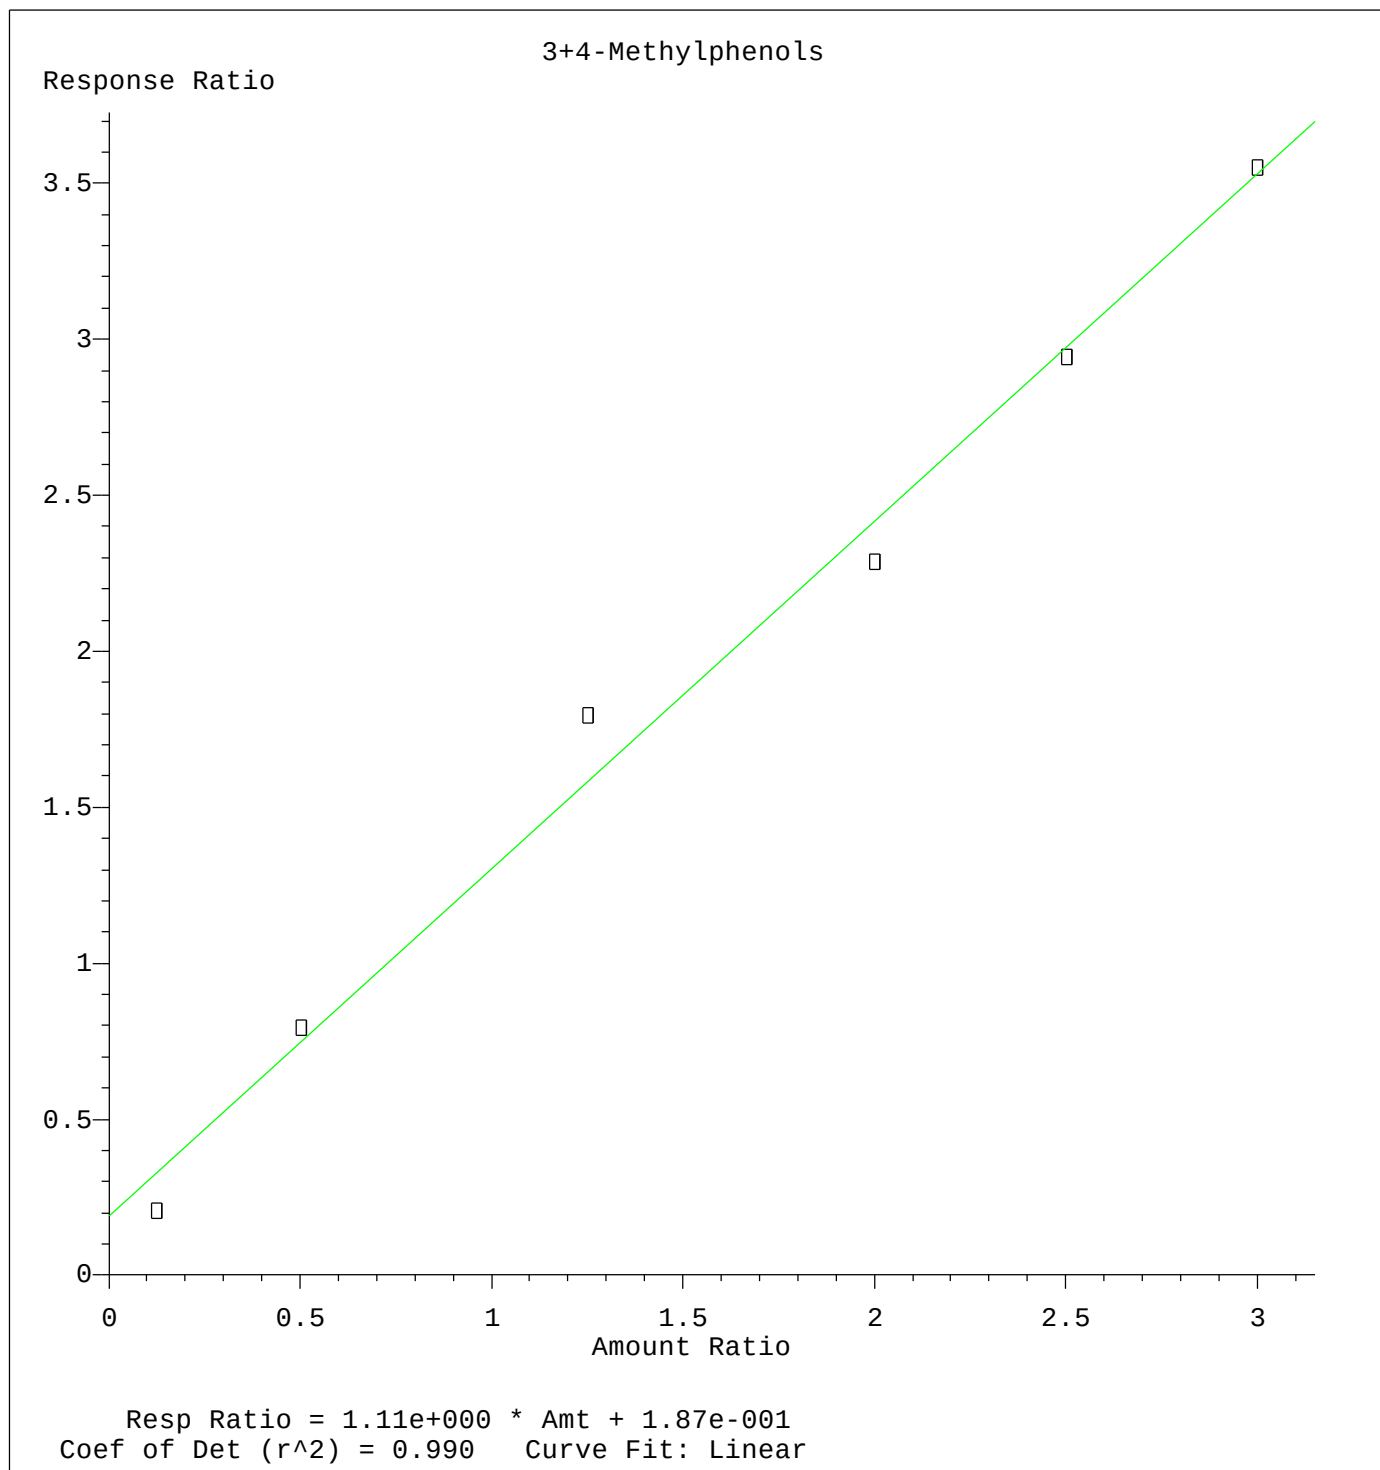

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Calibration Table Last Updated: Fri Dec 16 00:35:41 2016