

Data Path : Z:\HPCHEM1\BNA F\DATA\BF120916\
 Data File : BF091542.D
 Acq On : 9 Dec 2016 22:11
 Operator : UM/SJ
 Sample : H5886-02RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VW-01RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.978	250	253	255	rBV	204854	273787	1.14%	0.428%
2	5.413	288	291	293	rBV	1451469	1280357	5.32%	2.002%
3	6.453	379	382	384	rBV	1029289	1006793	4.18%	1.574%
4	6.579	391	393	396	rBV	2562912	2203907	9.15%	3.446%
5	6.807	411	413	416	rBV	2390957	2716454	11.28%	4.248%
6	6.967	424	427	429	rVB	2284659	1972604	8.19%	3.084%
7	7.367	460	462	465	rBV	1248946	1474251	6.12%	2.305%
8	8.099	523	526	528	rBV	4300787	3807720	15.82%	5.954%
9	9.173	618	620	622	rBV	3329154	2802517	11.64%	4.382%
10	9.848	677	679	682	rBV	3815276	3722131	15.46%	5.820%
11	10.636	745	748	750	rBV	1648902	1592203	6.61%	2.490%
12	11.333	806	809	811	rBV	3943589	3675926	15.27%	5.748%
13	11.871	854	856	861	rVB	226269	255760	1.06%	0.400%
14	12.659	922	925	930	rBV	279072	411558	1.71%	0.644%
15	12.911	945	947	950	rVB	2099512	2014595	8.37%	3.150%
16	13.962	1036	1039	1041	rBV	3002058	2890367	12.01%	4.520%
17	14.008	1041	1043	1059	rVB2	259962	1081304	4.49%	1.691%
18	14.865	1114	1118	1121	rBV3	279227	960373	3.99%	1.502%
19	15.071	1124	1136	1160	rVB	3660099	24073965	100.00%	37.643%
20	15.380	1160	1163	1166	rBV	1985353	2428103	10.09%	3.797%
21	16.865	1288	1293	1298	rBV3	135303	692976	2.88%	1.084%
22	18.523	1434	1438	1459	rVB6	373667	2614899	10.86%	4.089%


Sum of corrected areas: 63952550

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120916\
Data File : BF091542.D
Acq On : 9 Dec 2016 22:11
Operator : UM/SJ
Sample : H5886-02RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VW-01RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

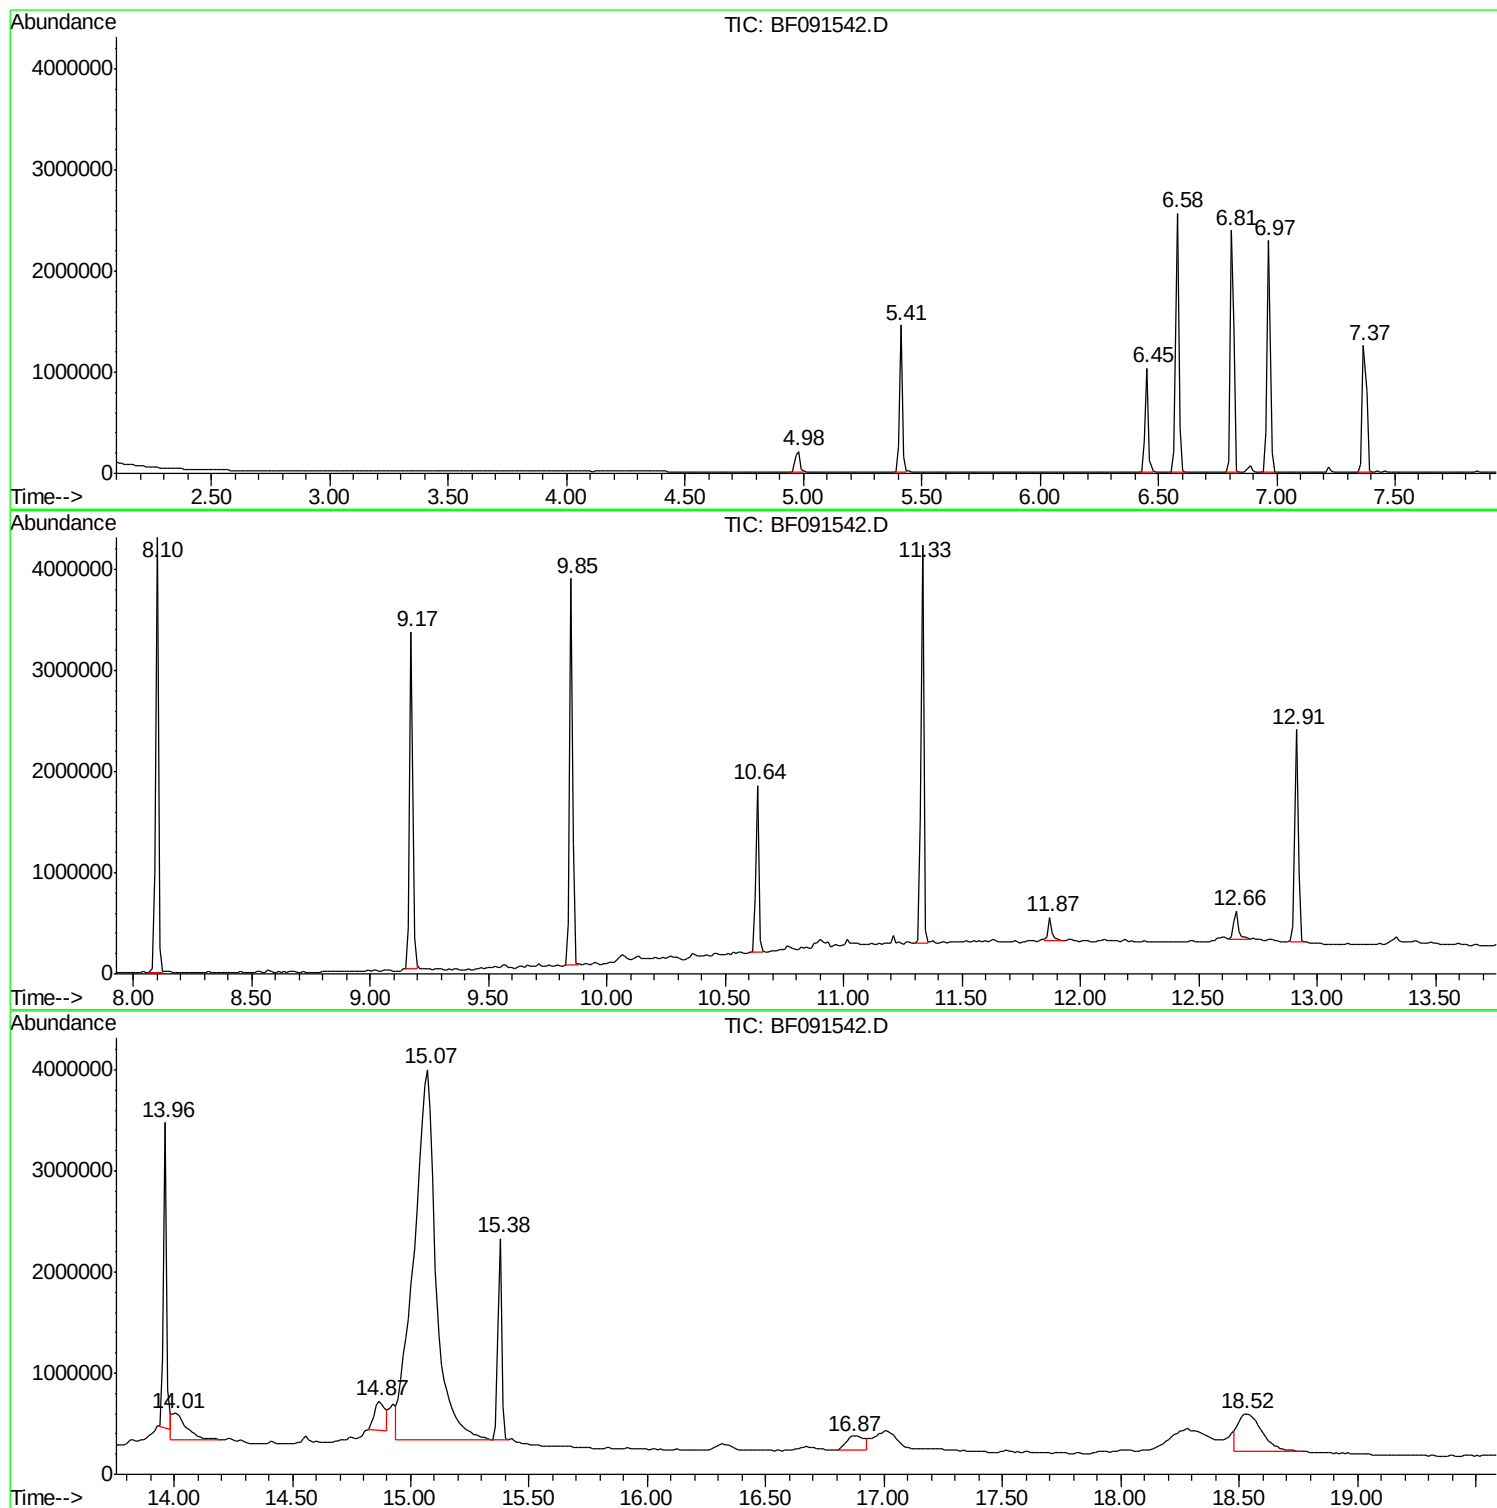

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF120916\
Data_File : BF091542.D
Acq_On : 9_Dec_2016 22:111
Operator : UM/SJJ
Sample : H5886-02REE
Misc :
ALS_Vial : 17 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
VW-01RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
