


Data Path : Z:\HPCHEM1\BNA_F\Data\BF120916\
 Data File : BF091524.D
 Acq On : 9 Dec 2016 13:24
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 19:00:21 2016

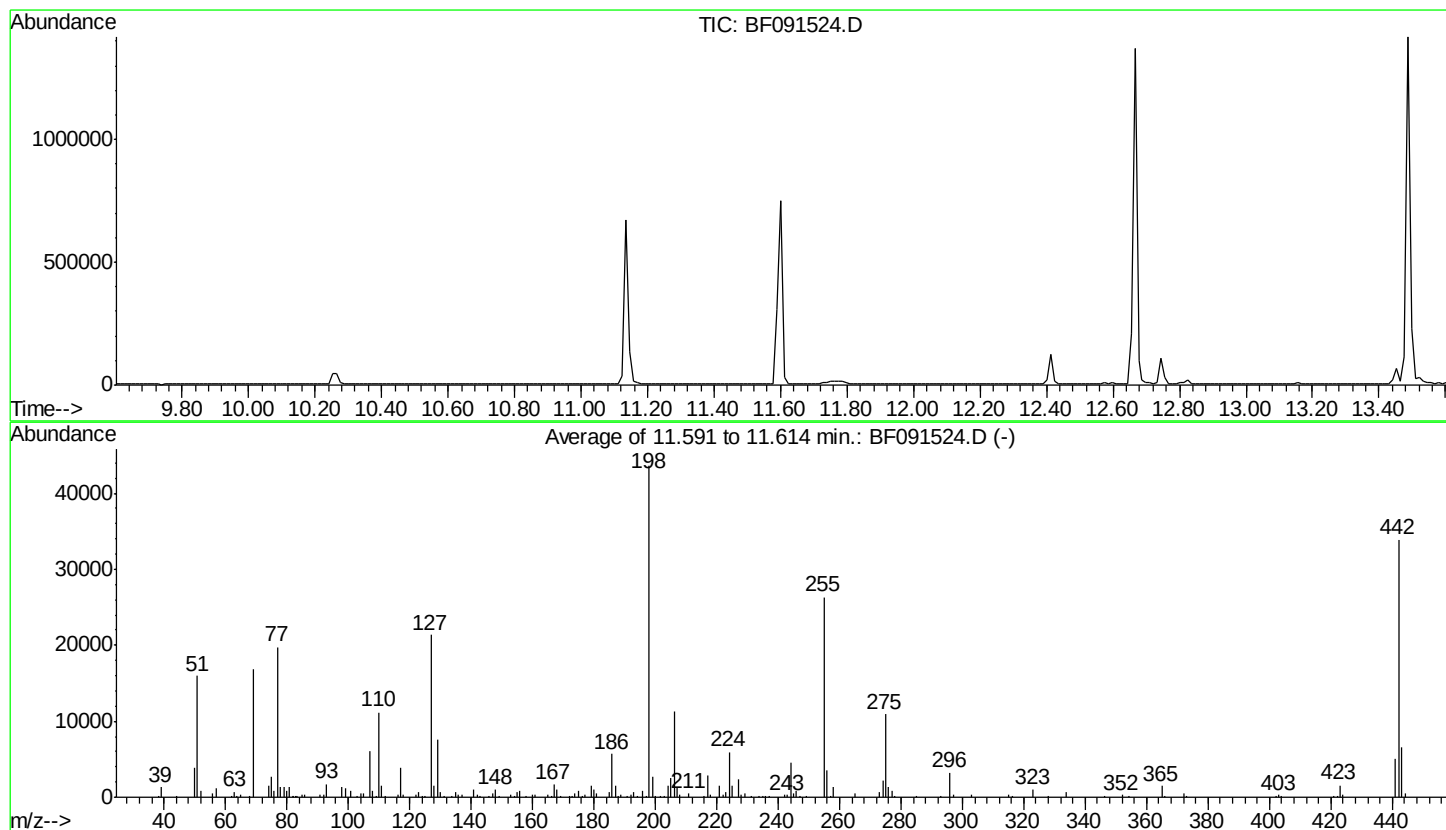

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	16001	PASS
68	69	0.00	2	1.4	238	PASS
69	198	0.00	100	38.7	16877	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	21327	PASS
197	198	0.00	2	0.4	167	PASS
198	198	100	100	100.0	43643	PASS
199	198	5	9	6.2	2712	PASS
275	198	10	60	24.9	10878	PASS
365	198	1	100	3.4	1490	PASS
441	442	0.01	24	15.1	5133	PASS
442	198	50	100	77.8	33937	PASS
443	442	15	24	19.5	6603	PASS