


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF120916\
Data File : BF091533.D
Acq On : 9 Dec 2016 18:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 09 19:00:21 2016

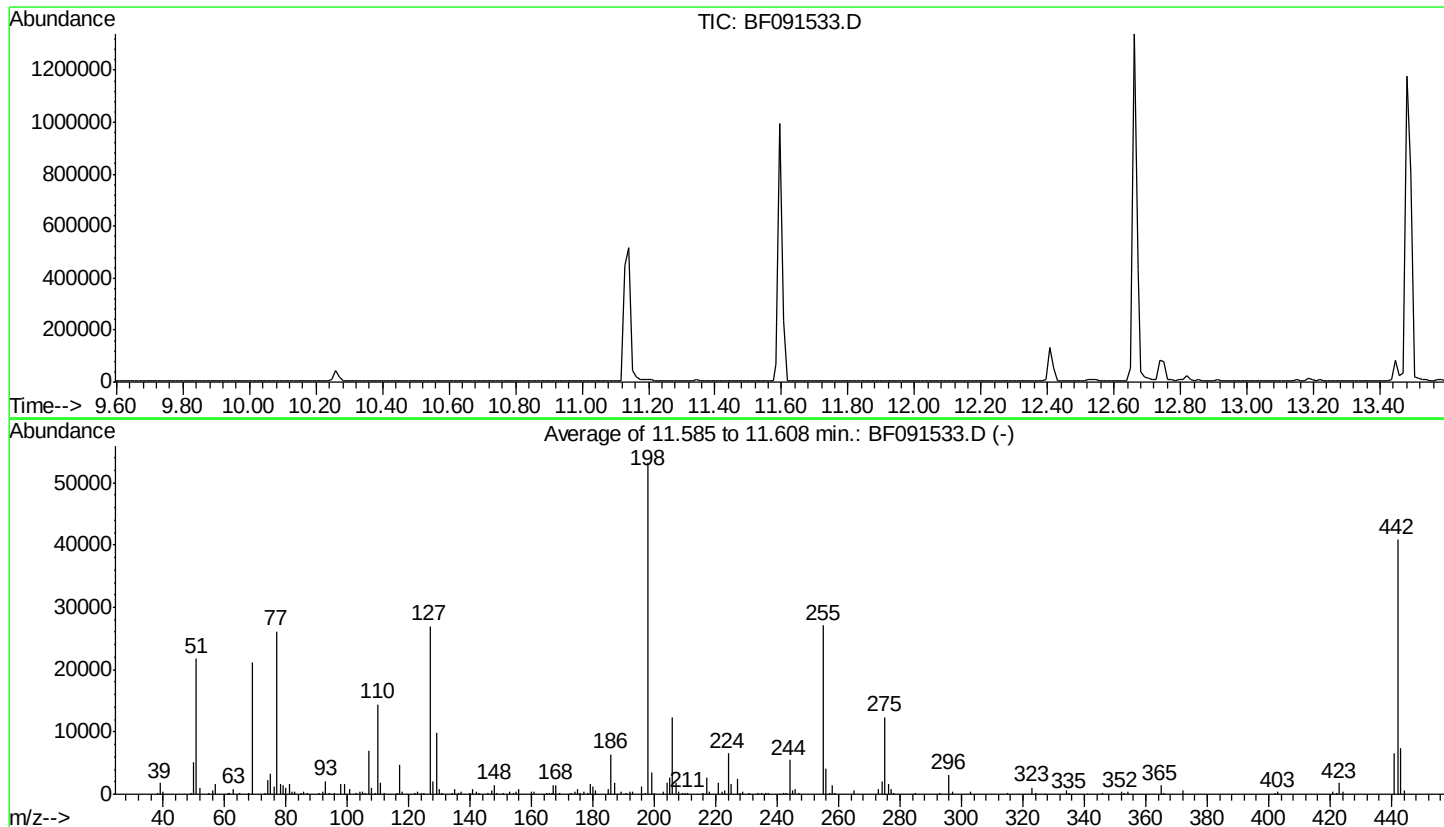

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	21704	PASS
68	69	0.00	2	1.0	206	PASS
69	198	0.00	100	39.7	21118	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.6	26930	PASS
197	198	0.00	2	0.5	243	PASS
198	198	100	100	100.0	53219	PASS
199	198	5	9	6.6	3531	PASS
275	198	10	60	23.2	12357	PASS
365	198	1	100	2.5	1347	PASS
441	442	0.01	24	16.2	6610	PASS
442	198	50	100	76.8	40865	PASS
443	442	15	24	17.9	7302	PASS