
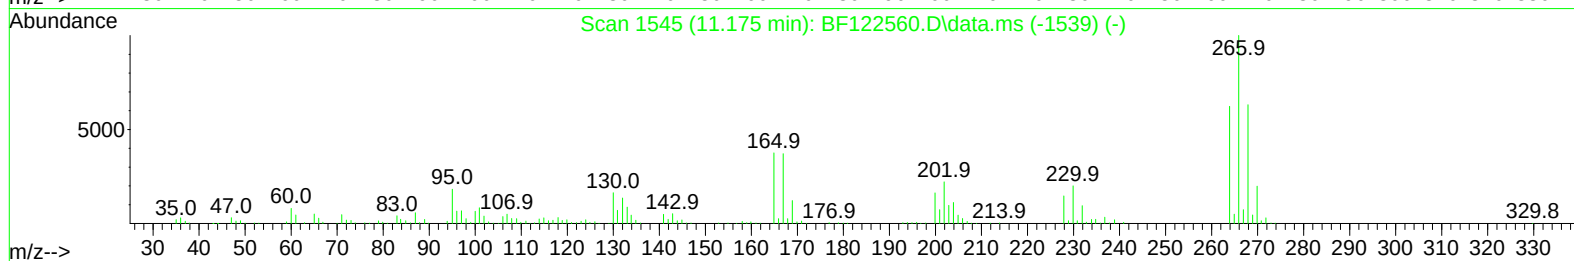
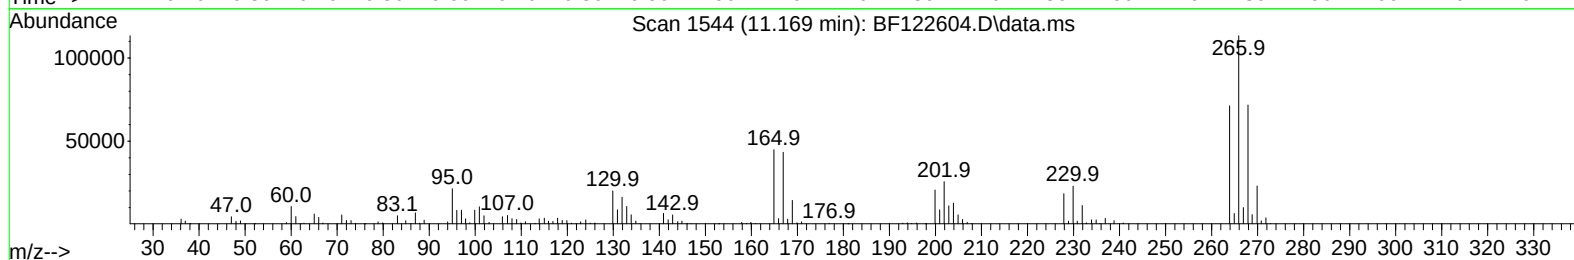


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122604.D
Acq On : 9 Dec 2020 8:40
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 11:12:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

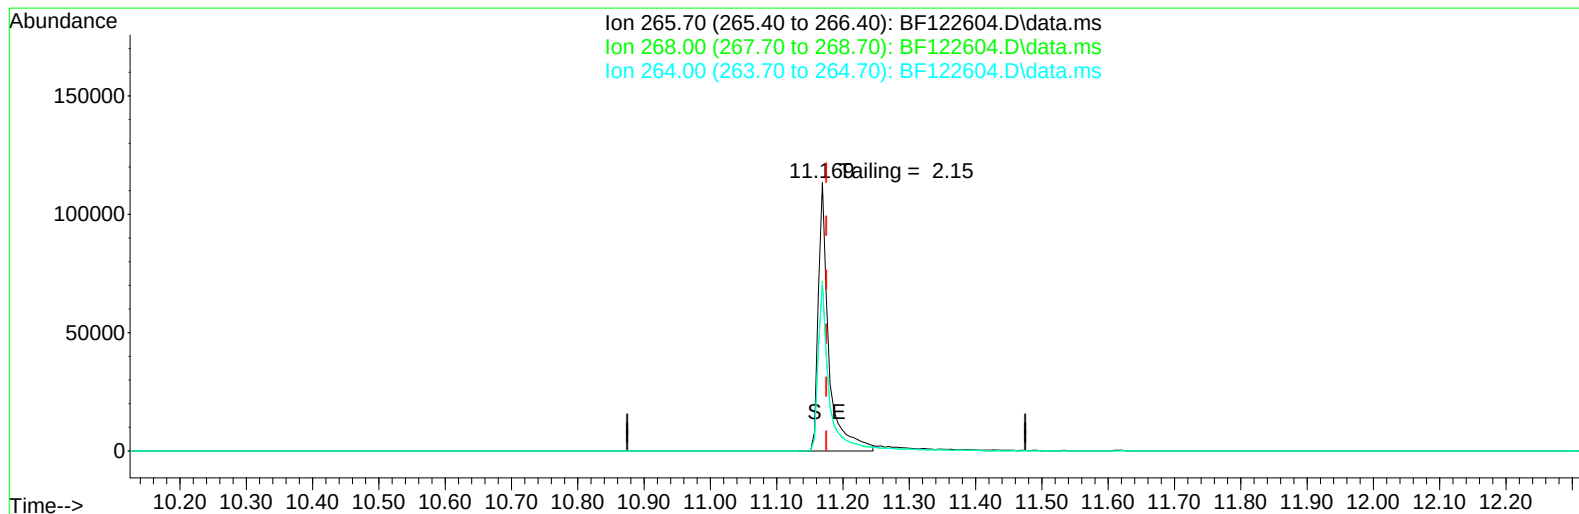

TIC: BF122604.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 32519.70 ng

response 132147

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.29
264.00	62.30	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122604.D
Acq On : 9 Dec 2020 8:40
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 11:12:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

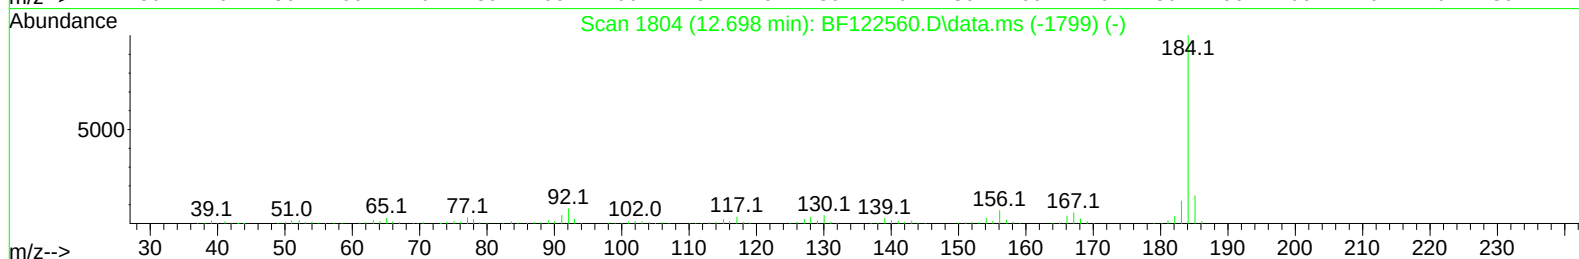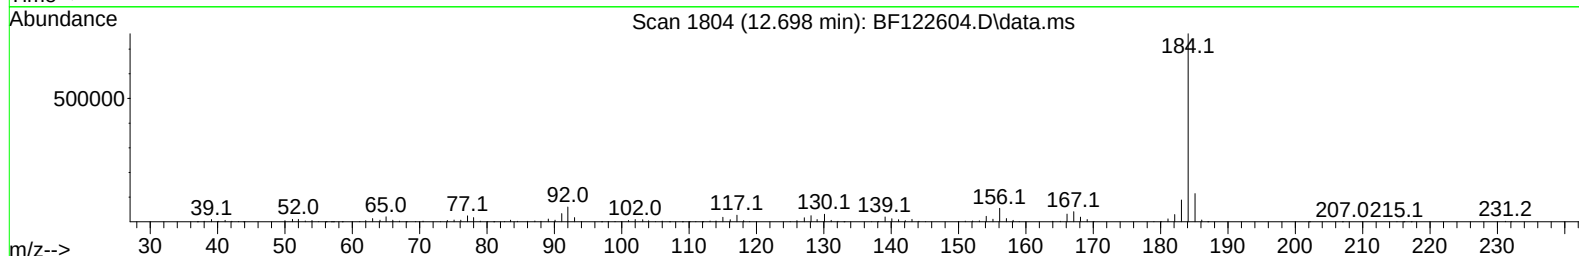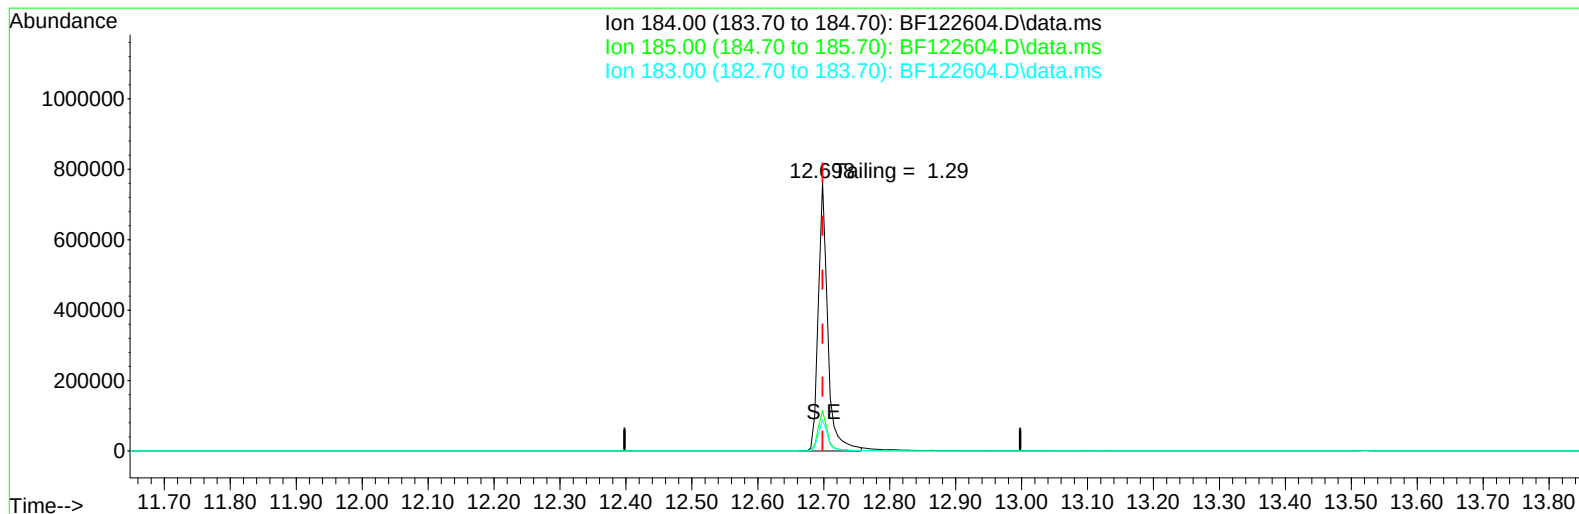

TIC: BF122604.D\data.ms

(77) Benzidine

12.698min (+ 0.000) 0.00 ng

response 777595

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.04
183.00	12.10	11.63
0.00	0.00	0.00