

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
 Data File : BF122611.D
 Acq On : 9 Dec 2020 14:05
 Operator : JU/CG
 Sample : L4969-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NORTH-BRANFORD-02

Quant Time: Dec 09 17:12:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 12:08:49 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.839	152	171083	20.00	ng	0.00
21) Naphthalene-d8	8.122	136	659427	20.00	ng	0.00
39) Acenaphthene-d10	9.880	164	337547	20.00	ng	0.00
64) Phenanthrene-d10	11.363	188	566649	20.00	ng	0.00
76) Chrysene-d12	14.004	240	427547	20.00	ng	0.00
86) Perylene-d12	15.468	264	452660	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	934881	86.51	ng	0.00
7) Phenol-d6	6.469	99	1169485	81.60	ng	-0.01
23) Nitrobenzene-d5	7.398	82	741839	56.36	ng	-0.01
42) 2,4,6-Tribromophenol	10.663	330	248623	56.27	ng	-0.01
45) 2-Fluorobiphenyl	9.198	172	1392479	55.80	ng	0.00
79) Terphenyl-d14	12.951	244	1271757	52.07	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	9.592	163	90369	3.35	ng	99
78) Pyrene	12.804	202	74123	2.24	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122611.D
Acq On : 9 Dec 2020 14:05
Operator : JU/CG
Sample : L4969-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02


Quant Time: Dec 09 17:12:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

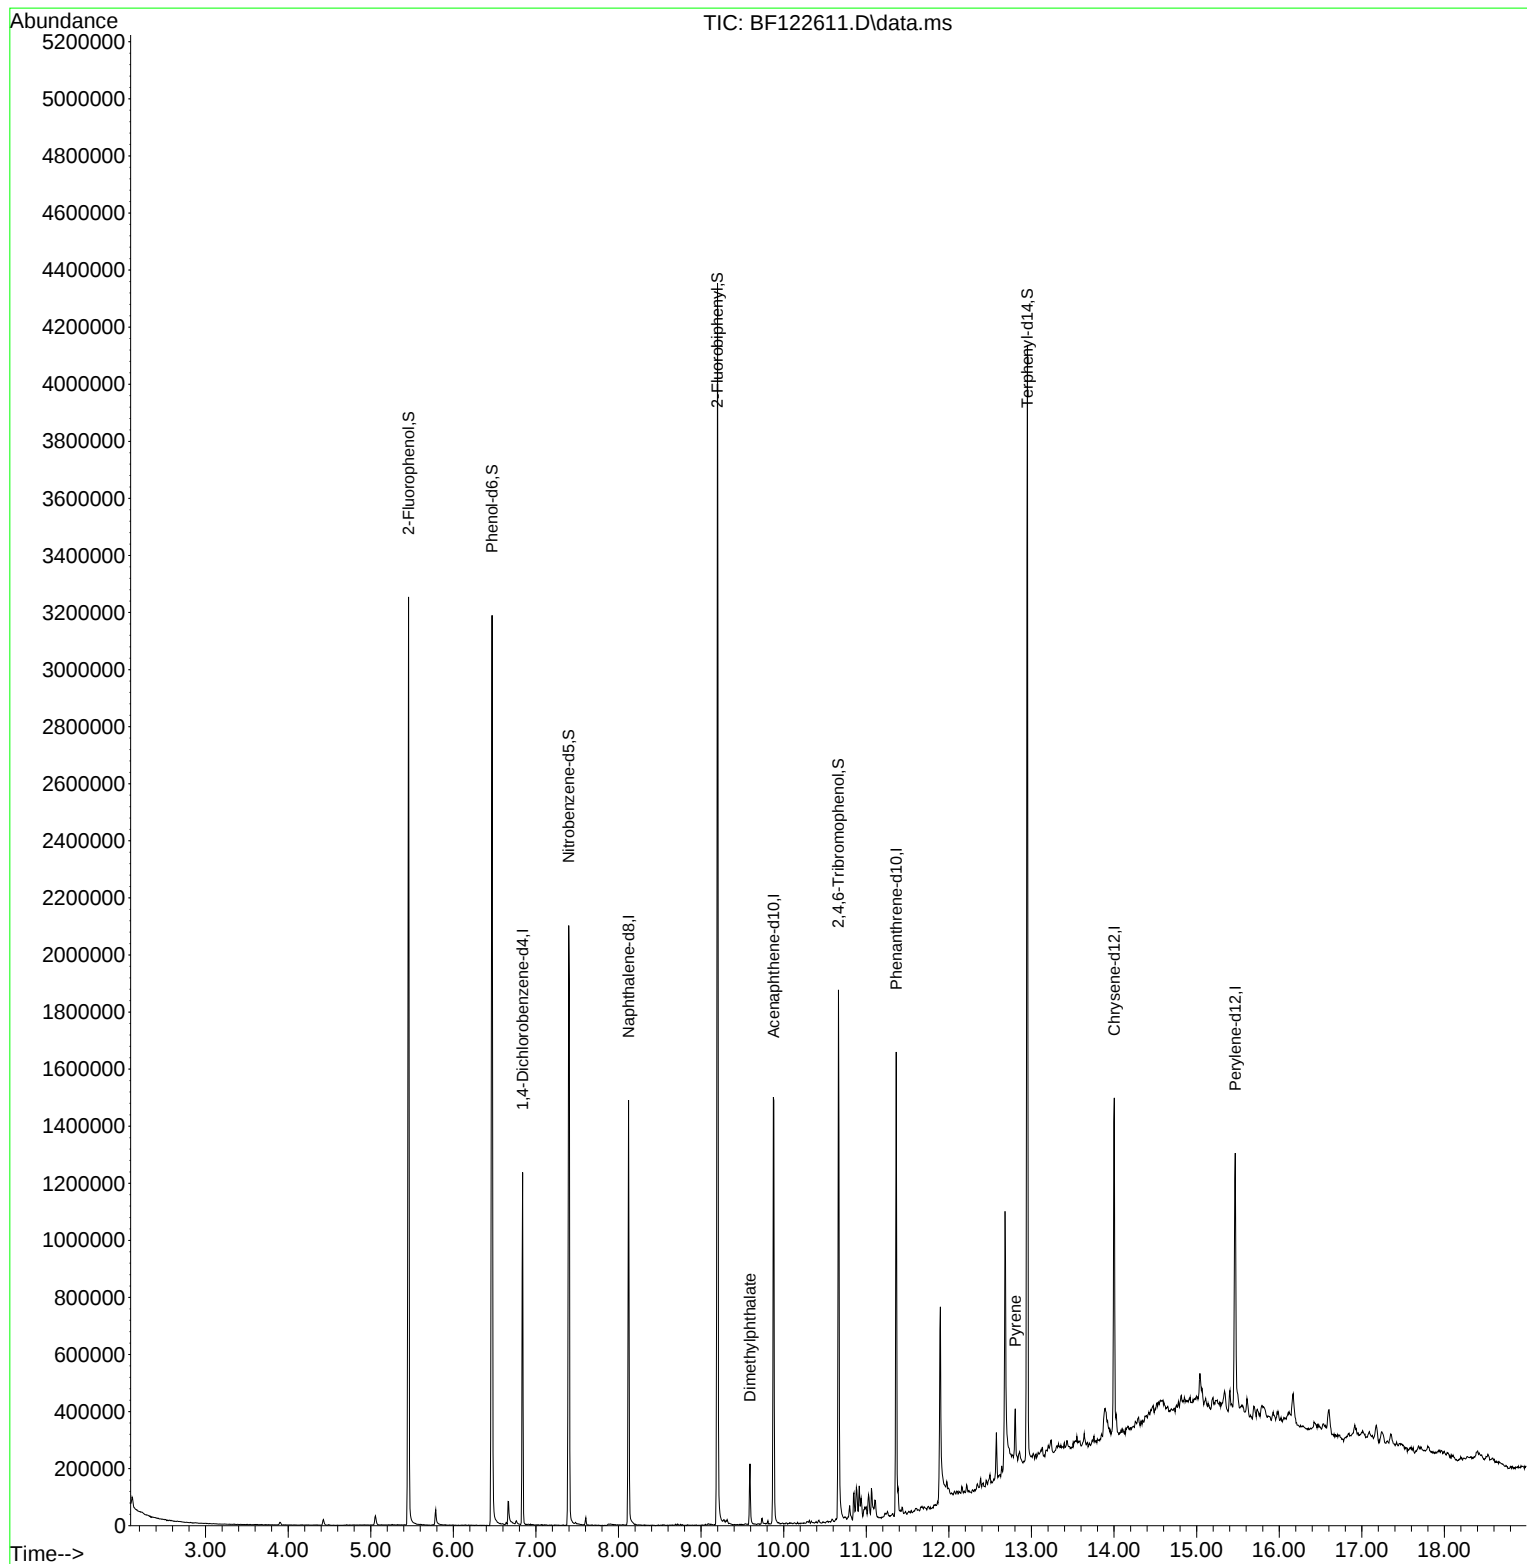



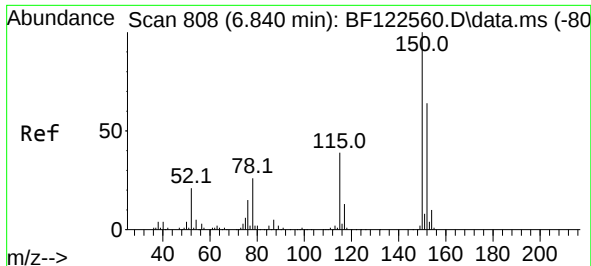


#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.839 min Scan# 808
Delta R.T. -0.001 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05


Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02

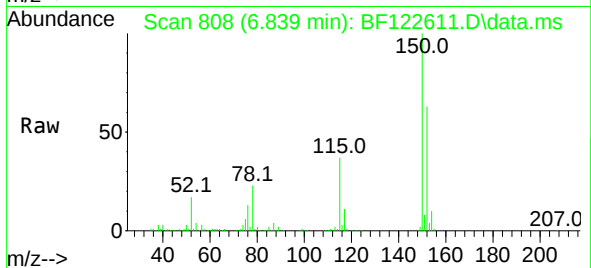



Tgt Ion:152 Resp: 171083
Ion Ratio Lower Upper
152 100
150 159.9 125.8 188.6
115 59.0 49.3 73.9

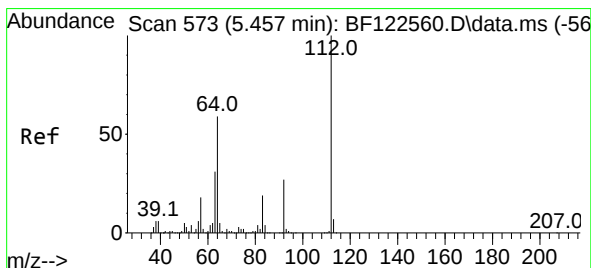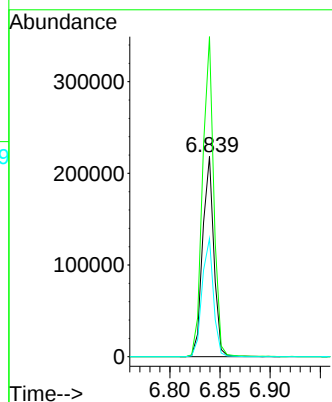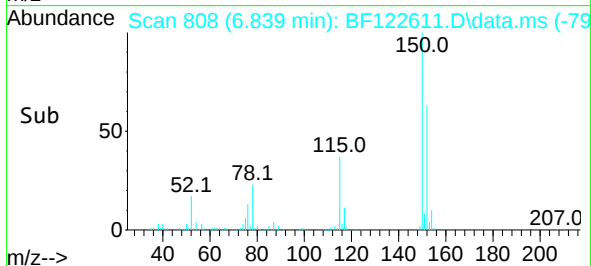

#5
2-Fluorophenol
Concen: 86.51 ng
RT: 5.457 min Scan# 573
Delta R.T. -0.000 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

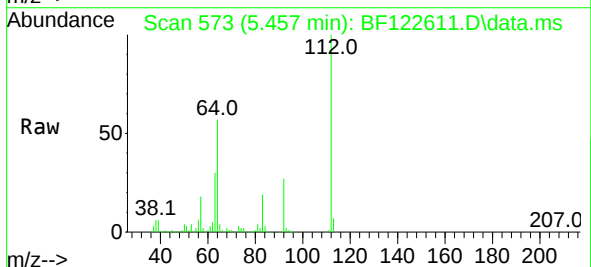

Tgt Ion:112 Resp: 934881
Ion Ratio Lower Upper
112 100
64 57.2 46.9 70.3
63 29.8 24.5 36.7

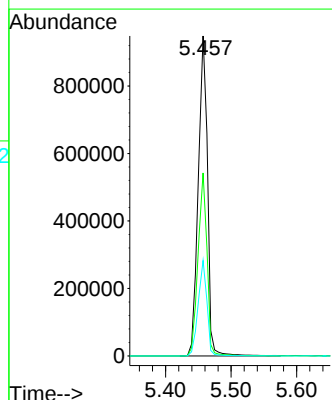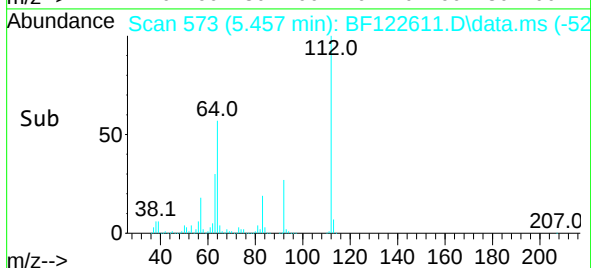







#7
Phenol-d6
Concen: 81.60 ng
RT: 6.469 min Scan# 745
Delta R.T. -0.012 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02

Tgt Ion: 99 Resp: 1169485




Ion	Ratio	Lower	Upper
99	100		
42	17.8	13.8	20.6
71	34.8	26.9	40.3

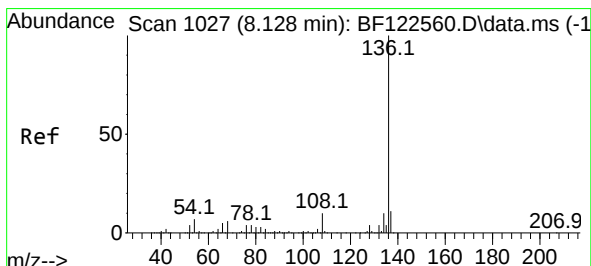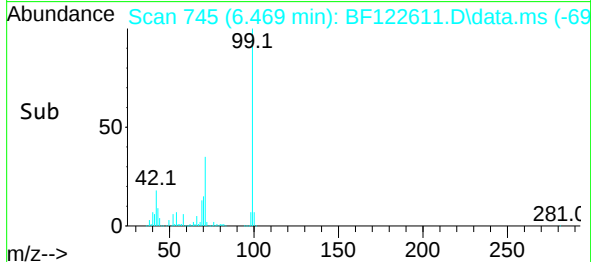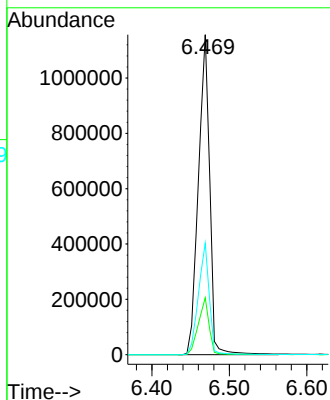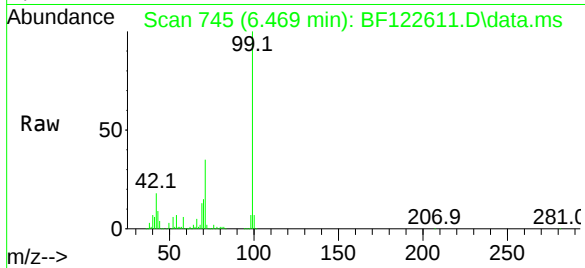


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

Tgt Ion: 136 Resp: 659427

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.8	13.2
54	7.3	5.5	8.3
68	6.3	4.6	6.8

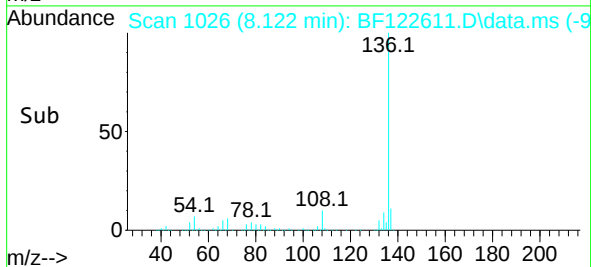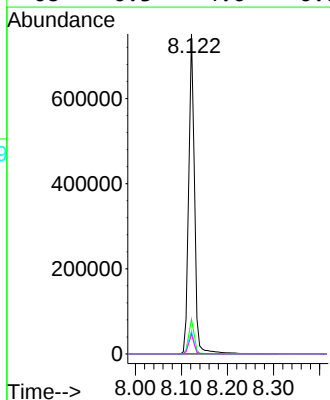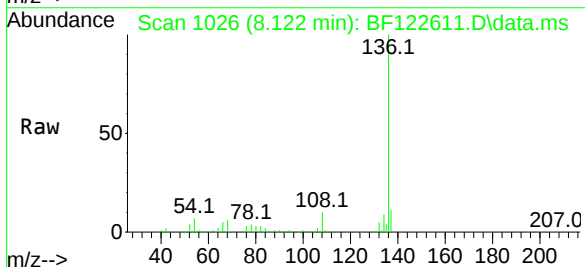

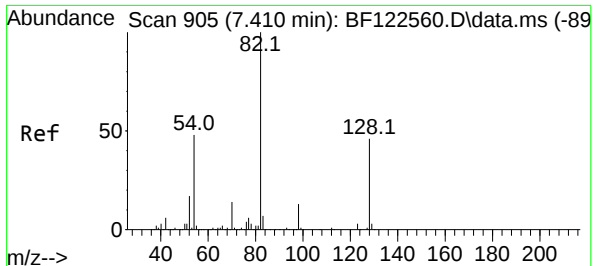

#23

Nitrobenzene-d5

Concen: 56.36 ng

RT: 7.398 min Scan# 903





Delta R.T. -0.012 min

Lab File: BF122611.D

Acq: 9 Dec 2020 14:05

Tgt Ion: 82 Resp: 741839

Ion	Ratio	Lower	Upper
82	100		
128	44.2	37.0	55.4
54	47.9	38.4	57.6

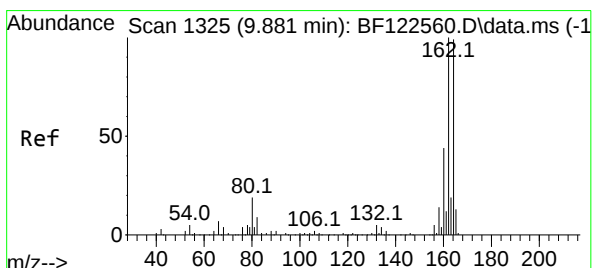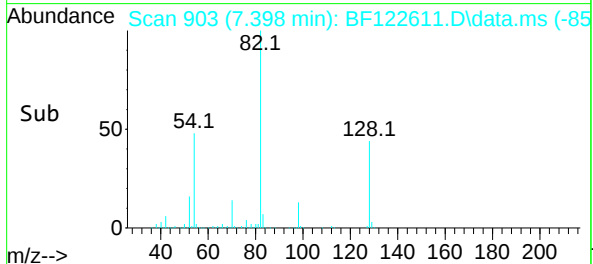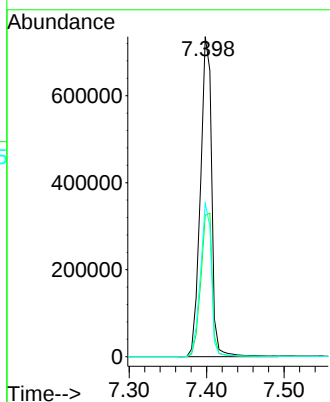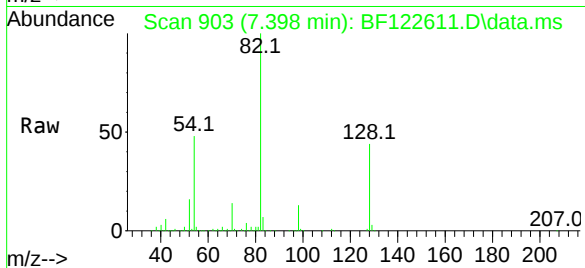

#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.880 min Scan# 1325




Delta R.T. -0.001 min

Lab File: BF122611.D

Acq: 9 Dec 2020 14:05

Tgt Ion: 164 Resp: 337547

Ion	Ratio	Lower	Upper
164	100		
162	101.4	80.8	121.2
160	45.3	35.4	53.0

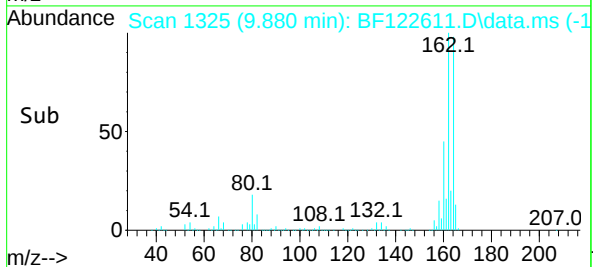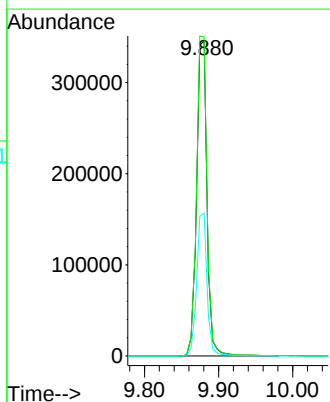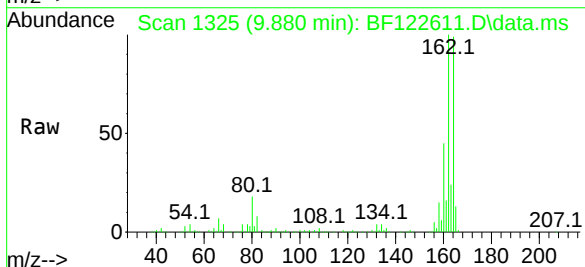


Instrument :

BNA_F


ClientSampleId :

NORTH-BRANFORD-02



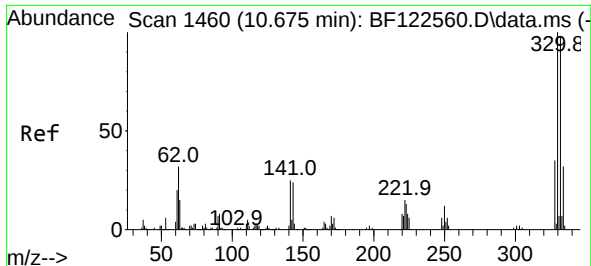


#42
2,4,6-Tribromophenol
Concen: 56.27 ng
RT: 10.663 min Scan# 1458
Delta R.T. -0.012 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02



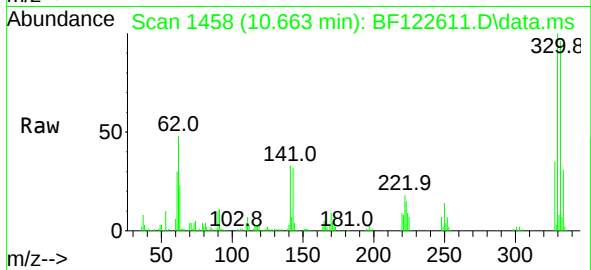



Tgt Ion:330 Resp: 248623
Ion Ratio Lower Upper
330 100
332 96.8 77.5 116.3
141 29.3 23.8 35.8

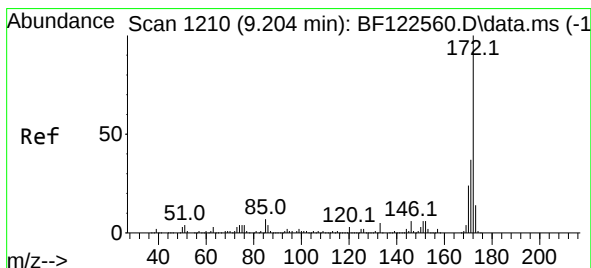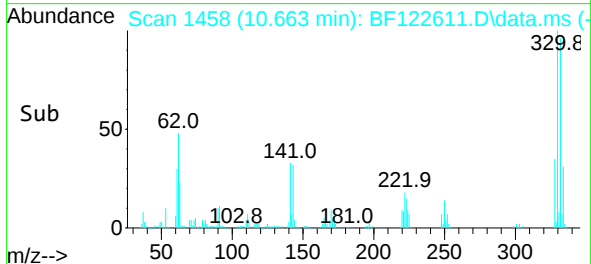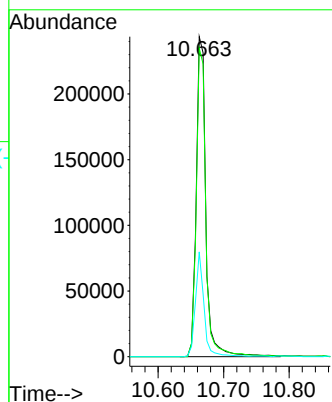

#45
2-Fluorobiphenyl
Concen: 55.80 ng
RT: 9.198 min Scan# 1209
Delta R.T. -0.006 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

Tgt Ion:172 Resp: 1392479
Ion Ratio Lower Upper
172 100
171 36.5 29.6 44.4
170 24.0 19.5 29.3


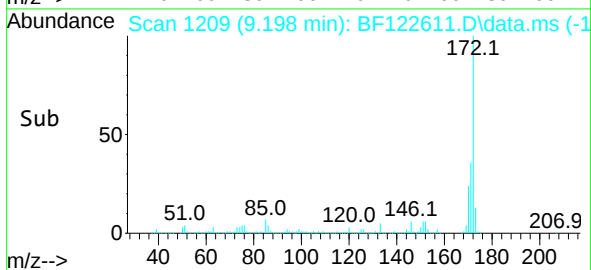
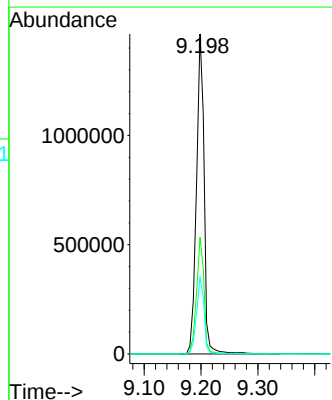
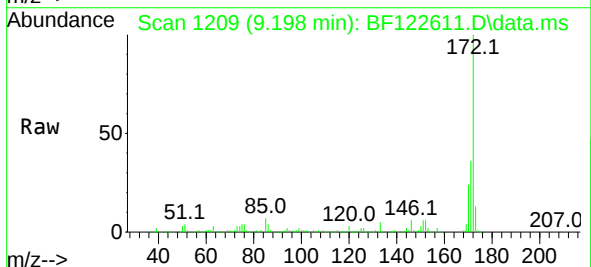


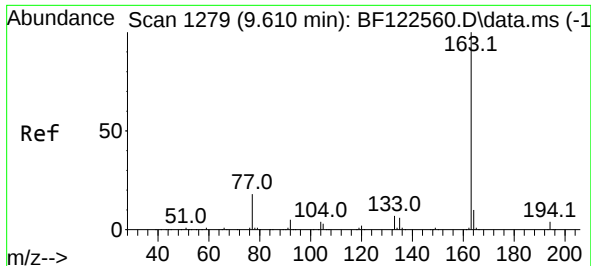

#50
Dimethylphthalate
Concen: 3.35 ng
RT: 9.592 min Scan# 1276
Delta R.T. -0.018 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05




Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02


Tgt Ion:163 Resp: 90369
Ion Ratio Lower Upper
163 100
194 4.2 3.4 5.0
164 10.6 8.1 12.1

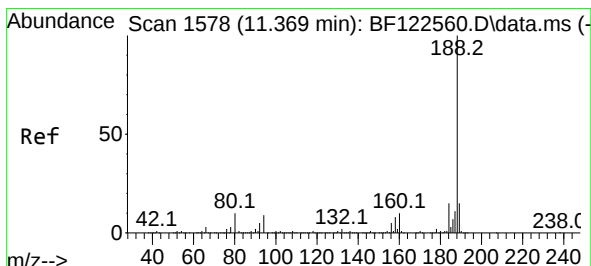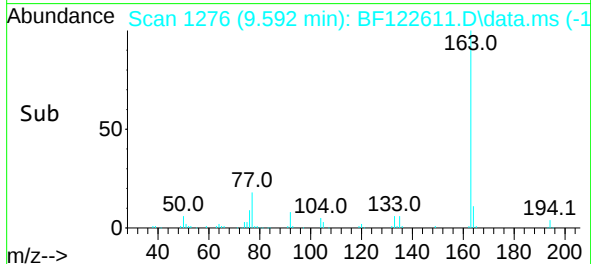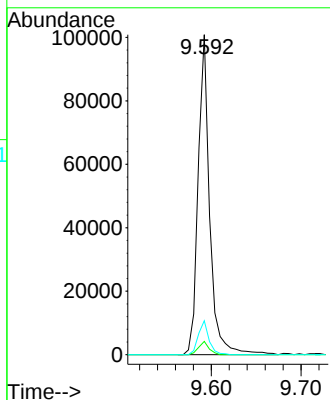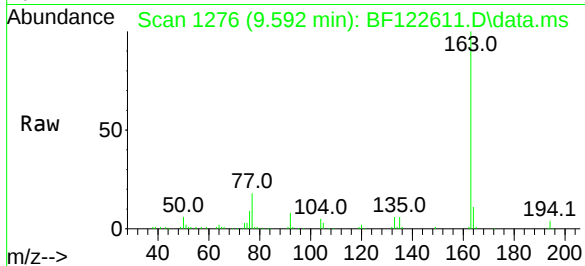

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.363 min Scan# 1577
Delta R.T. -0.006 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

Tgt Ion:188 Resp: 566649
Ion Ratio Lower Upper
188 100
94 9.8 7.4 11.2
80 10.5 8.2 12.4

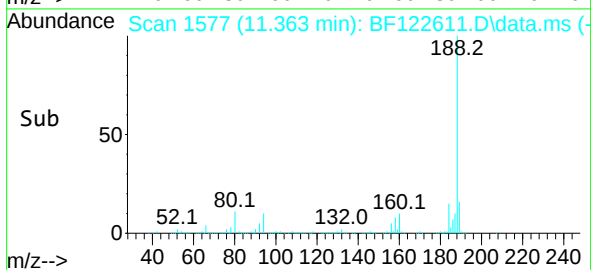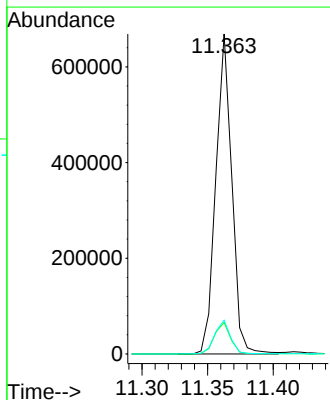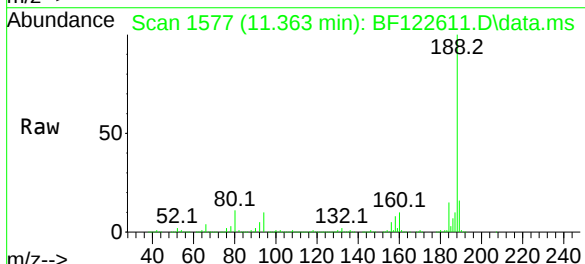

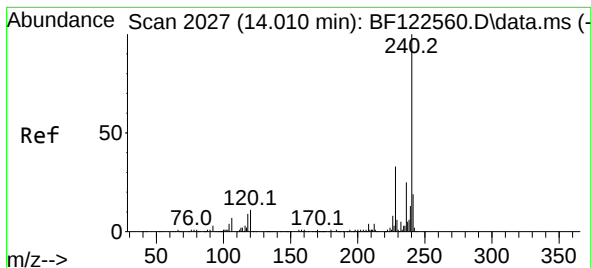

#76

Chrysene-d12

Concen: 20.00 ng

RT: 14.004 min Scan# 2026

Delta R.T. -0.006 min

Lab File: BF122611.D

Acq: 9 Dec 2020 14:05

Tgt Ion:240 Resp: 427547

Ion Ratio Lower Upper

240 100

120 9.9 8.6 12.8





236 25.3 20.3 30.5

Instrument :

BNA_F

ClientSampleId :

NORTH-BRANFORD-02

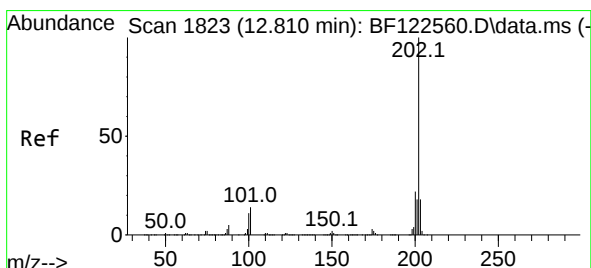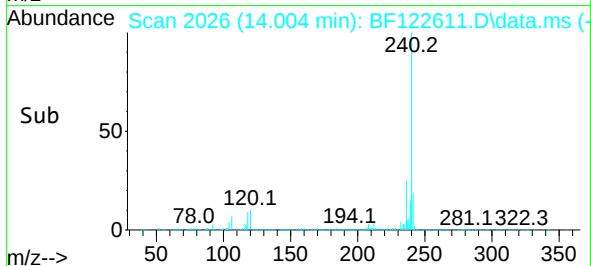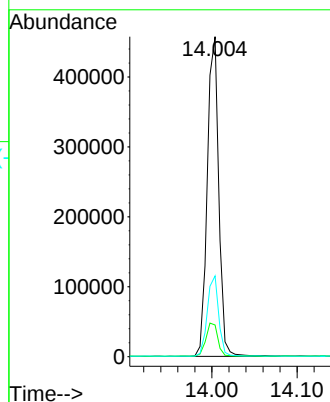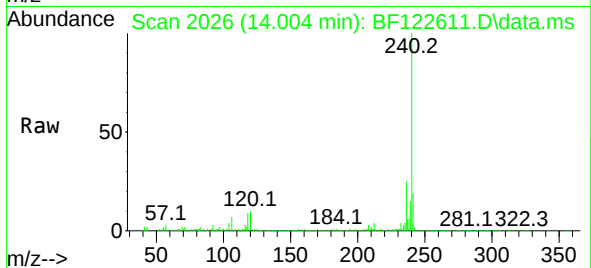

#78

Pyrene

Concen: 2.24 ng

RT: 12.804 min Scan# 1822

Delta R.T. -0.006 min

Lab File: BF122611.D

Acq: 9 Dec 2020 14:05




Tgt Ion:202 Resp: 74123


Ion Ratio Lower Upper

202 100

200 20.9 17.6 26.4

203 17.9 14.6 21.8


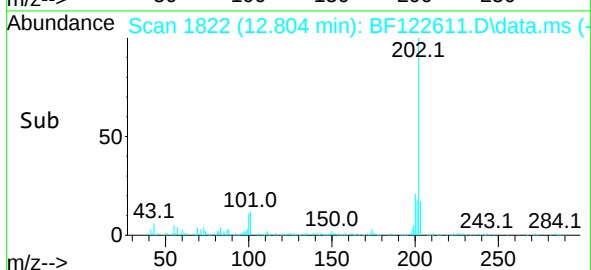
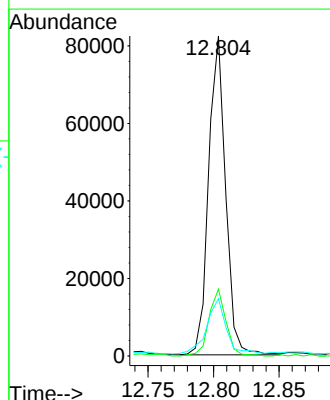
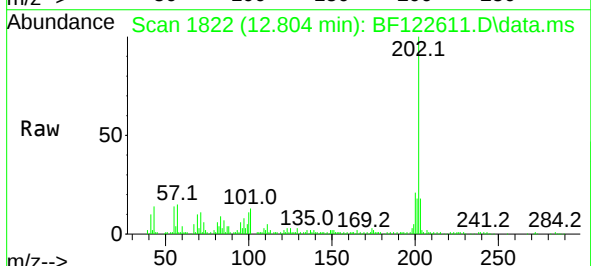


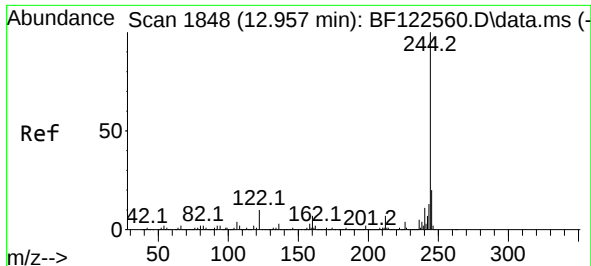

#79
Terphenyl-d14
Concen: 52.07 ng
RT: 12.951 min Scan# 1847
Delta R.T. -0.006 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02

Tgt Ion:244 Resp: 1271757
Ion Ratio Lower Upper
244 100
212 6.9 5.7 8.5
122 10.1 8.3 12.5

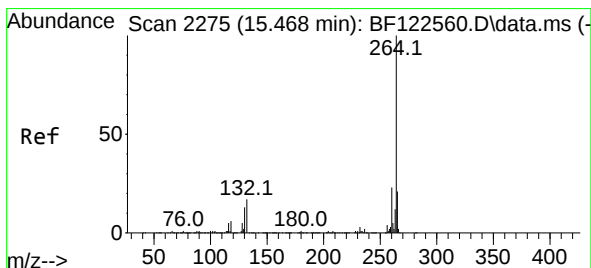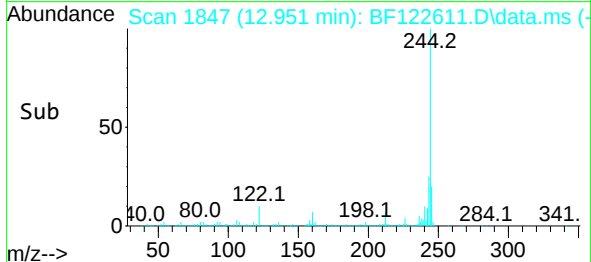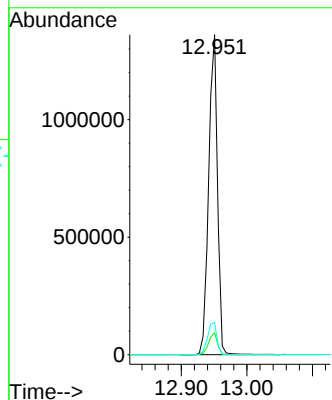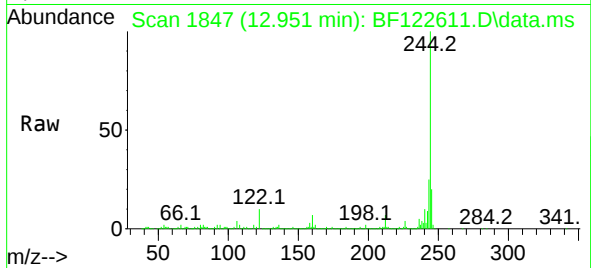

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.468 min Scan# 2275
Delta R.T. -0.000 min
Lab File: BF122611.D
Acq: 9 Dec 2020 14:05

Tgt Ion:264 Resp: 452660
Ion Ratio Lower Upper
264 100
260 24.1 18.6 28.0
265 21.4 17.0 25.6

