

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
 Data File : BF122633.D
 Acq On : 10 Dec 2020 3:08
 Operator : JU/CG
 Sample : L4972-01 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-01-120820

Manual Integrations
 APPROVED

mohammad
 12/10/2020 2:43:36 PM

Quant Time: Dec 10 06:21:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 12:08:49 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.840	152	210628	20.00	ng	0.00
21) Naphthalene-d8	8.122	136	817638	20.00	ng	0.00
39) Acenaphthene-d10	9.875	164	413791	20.00	ng	0.00
64) Phenanthrene-d10	11.363	188	673484	20.00	ng	0.00
76) Chrysene-d12	14.004	240	498586	20.00	ng	0.00
86) Perylene-d12	15.468	264	529560	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.451	112	561854	42.23	ng	0.00
7) Phenol-d6	6.463	99	696868	39.49	ng	-0.02
23) Nitrobenzene-d5	7.398	82	430089	26.35	ng	-0.01
42) 2,4,6-Tribromophenol	10.663	330	173687	32.07	ng	-0.01
45) 2-Fluorobiphenyl	9.198	172	815468	26.66	ng	0.00
79) Terphenyl-d14	12.945	244	674256	23.67	ng	-0.01
Target Compounds						Qvalue
50) Dimethylphthalate	9.592	163	80728	2.44	ng	99
71) Phenanthrene	11.386	178	237658	5.94	ng	98
75) Fluoranthene	12.575	202	364773	8.69	ng	98
78) Pyrene	12.804	202	344563	8.94	ng	97
81) Benzo(a)anthracene	13.992	228	153394	4.60	ng	94
83) Chrysene	14.027	228	170094	5.13	ng	96
87) Indeno(1,2,3-cd)pyrene	16.915	276	85028	2.45	ng	97
88) Benzo(b)fluoranthene	15.039	252	211630m	5.70	ng	
89) Benzo(k)fluoranthene	15.063	252	69184m	2.04	ng	
90) Benzo(a)pyrene	15.404	252	151793	4.67	ng	98
92) Benzo(g,h,i)perylene	17.357	276	85178	3.09	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122633.D
Acq On : 10 Dec 2020 3:08
Operator : JU/CG
Sample : L4972-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
SU-01-120820

Manual Integrations
APPROVED


mohammad
12/10/2020 2:43:36 PM

Quant Time: Dec 10 06:21:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration



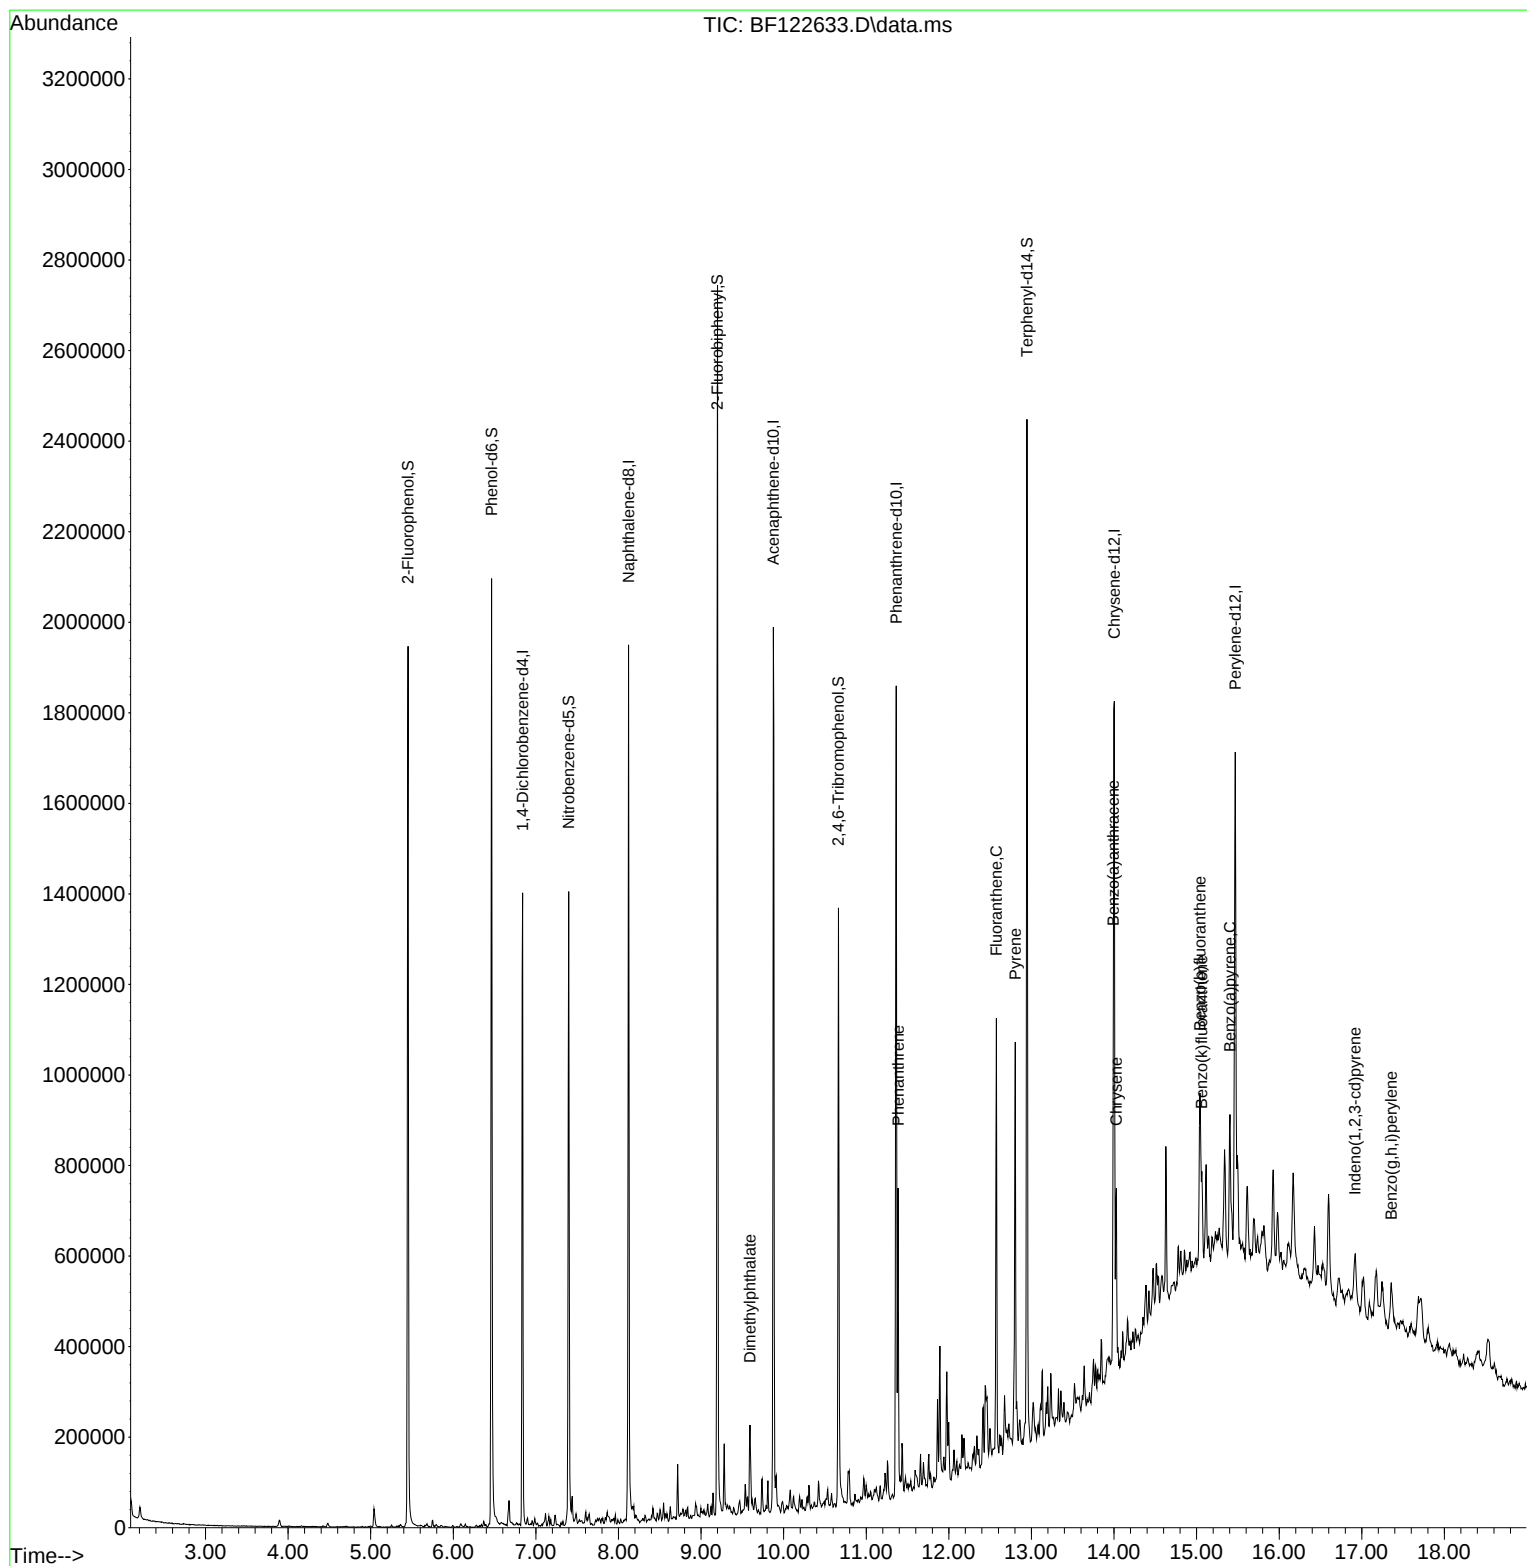





#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.840 min Scan# 808
Delta R.T. -0.000 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08





Tgt Ion:152 Resp: 210628
Ion Ratio Lower Upper
152 100
150 154.8 125.8 188.6
115 57.1 49.3 73.9

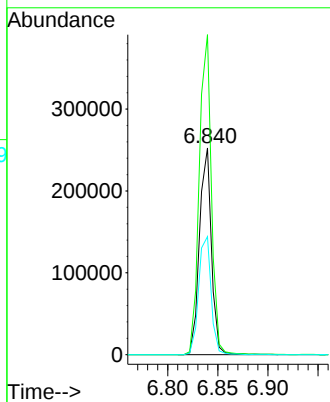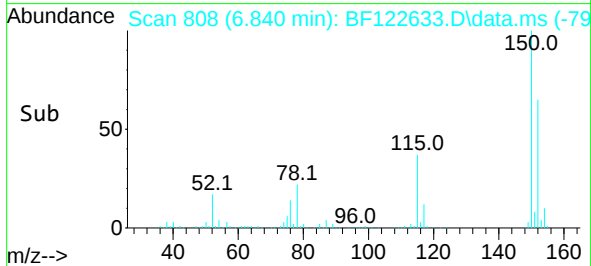

#5
2-Fluorophenol
Concen: 42.23 ng
RT: 5.451 min Scan# 572
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

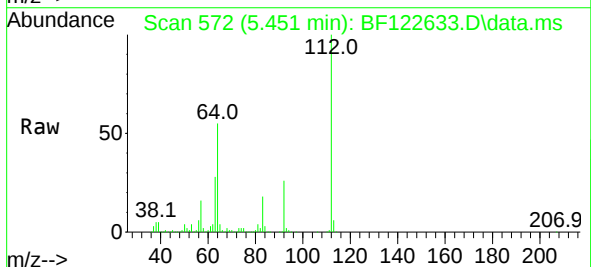

Tgt Ion:112 Resp: 561854
Ion Ratio Lower Upper
112 100
64 54.6 46.9 70.3
63 27.7 24.5 36.7

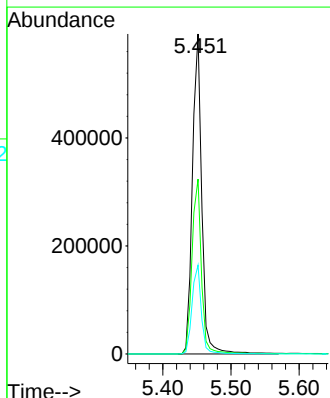

Instrument :
BNA_F
ClientSampleId :
SU-01-120820

Manual Integrations
APPROVED

mohammad
12/10/2020 2:43:36 PM







#7
Phenol-d6
Concen: 39.49 ng
RT: 6.463 min Scan# 744
Delta R.T. -0.018 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

Tgt Ion:	99	Resp:	696868
Ion Ratio	Lower	Upper	
99	100		
42	17.0	13.8	20.6
71	33.1	26.9	40.3

Instrument :
BNA_F
ClientSampleId :
SU-01-120820




Manual Integrations
APPROVED


mohammad
12/10/2020 2:43:36 PM

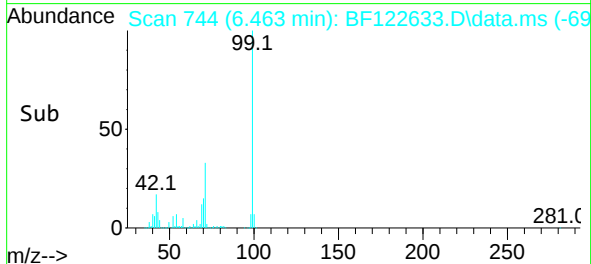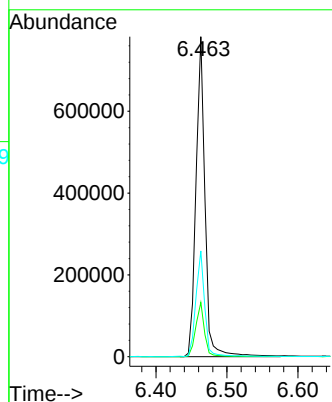

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

Tgt Ion:	136	Resp:	817638
Ion Ratio	Lower	Upper	
136	100		
137	11.0	8.8	13.2
54	7.4	5.5	8.3
68	6.0	4.6	6.8

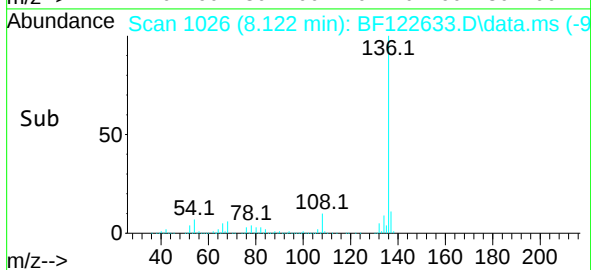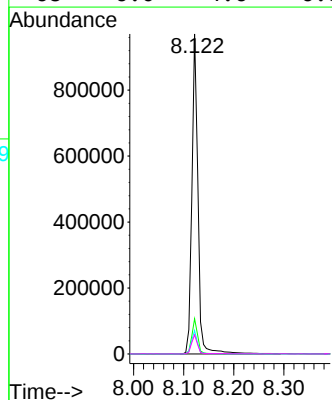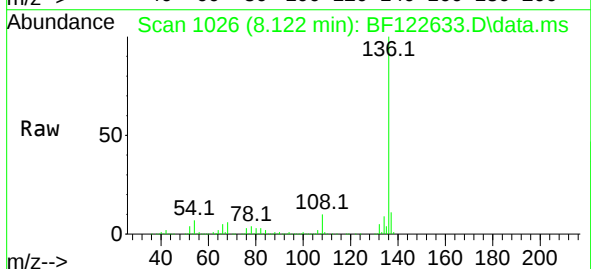

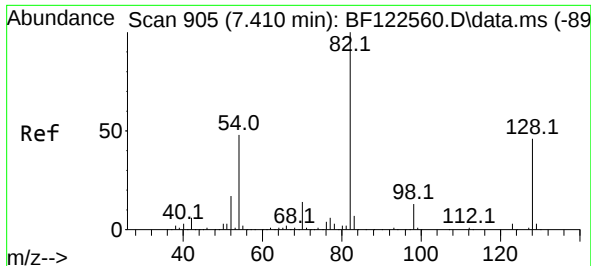

#23

Nitrobenzene-d5

Concen: 26.35 ng

RT: 7.398 min Scan# 903

Delta R.T. -0.012 min

Lab File: BF122633.D

Acq: 10 Dec 2020 3:08

Tgt Ion: 82 Resp: 430089

Ion Ratio Lower Upper

82 100

128 46.0 37.0 55.4

54 46.0 38.4 57.6

Instrument :

BNA_F

ClientSampleId :





SU-01-120820

Manual Integrations

APPROVED

mohammad

12/10/2020 2:43:36 PM

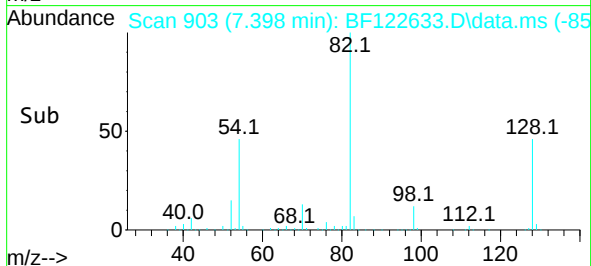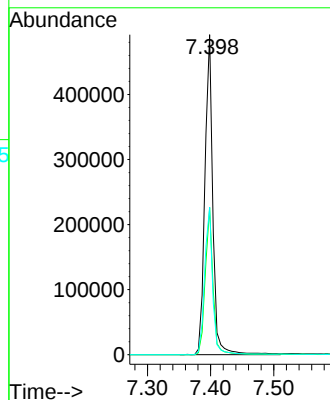

#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.875 min Scan# 1324

Delta R.T. -0.006 min

Lab File: BF122633.D

Acq: 10 Dec 2020 3:08




Tgt Ion:164 Resp: 413791


Ion Ratio Lower Upper

164 100

162 101.7 80.8 121.2


160 44.6 35.4 53.0

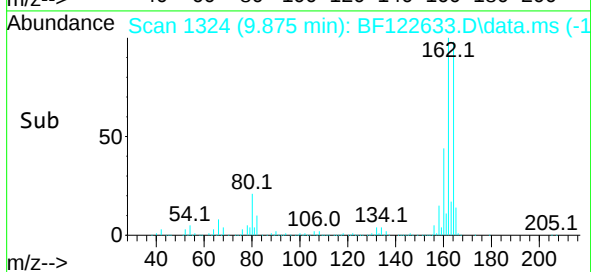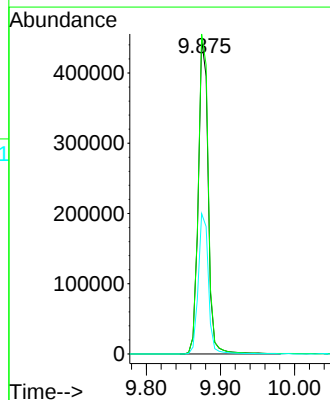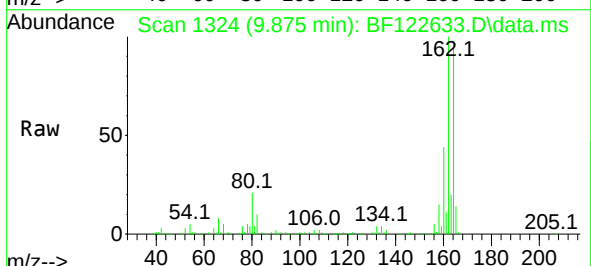



#42
2,4,6-Tribromophenol
Concen: 32.07 ng
RT: 10.663 min Scan# 1458
Delta R.T. -0.012 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08




Instrument :
BNA_F
ClientSampleId :
SU-01-120820




Tgt Ion: 330 Resp: 173687
Ion Ratio Lower Upper
330 100
332 94.9 77.5 116.3
141 28.5 23.8 35.8

Manual Integrations
APPROVED



mohammad
12/10/2020 2:43:36 PM

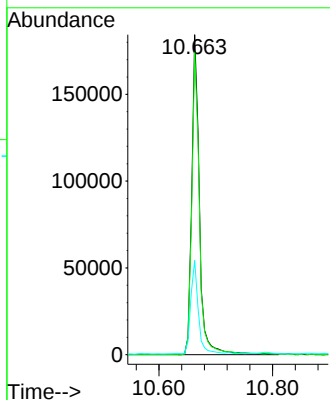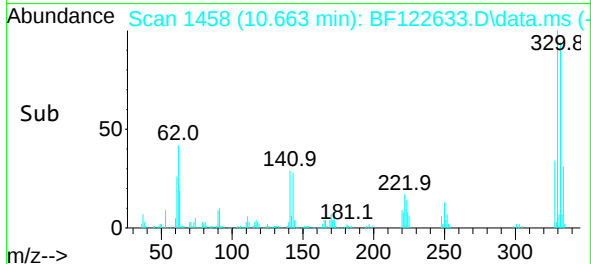


#45
2-Fluorobiphenyl
Concen: 26.66 ng
RT: 9.198 min Scan# 1209
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

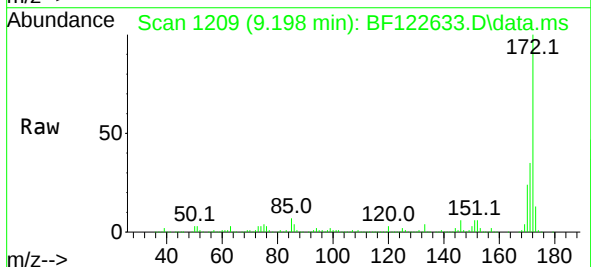


Tgt Ion: 172 Resp: 815468
Ion Ratio Lower Upper
172 100
171 35.5 29.6 44.4
170 23.8 19.5 29.3


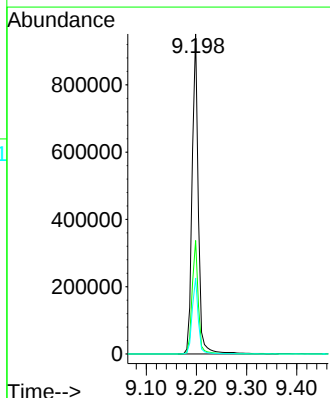



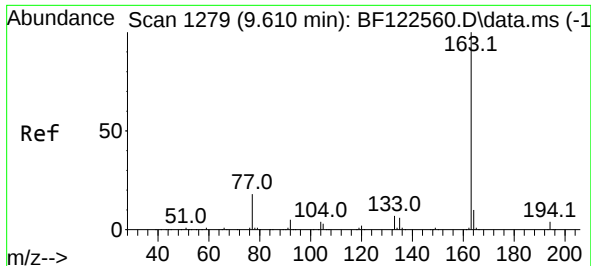


#50
Dimethylphthalate
Concen: 2.44 ng
RT: 9.592 min Scan# 1276
Delta R.T. -0.018 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08





Tgt Ion:163 Resp: 80728
Ion Ratio Lower Upper
163 100
194 3.9 3.4 5.0
164 9.6 8.1 12.1

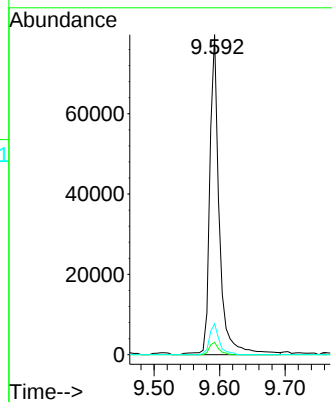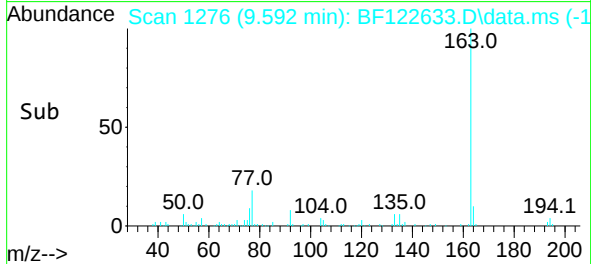

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.363 min Scan# 1577
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

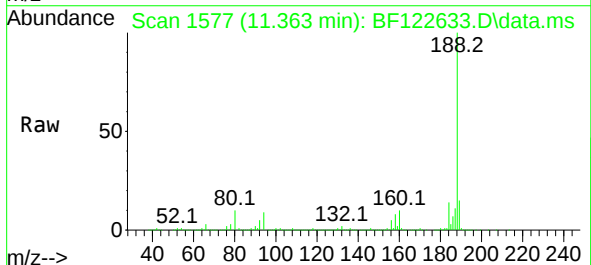


Tgt Ion:188 Resp: 673484
Ion Ratio Lower Upper
188 100
94 9.5 7.4 11.2
80 10.1 8.2 12.4

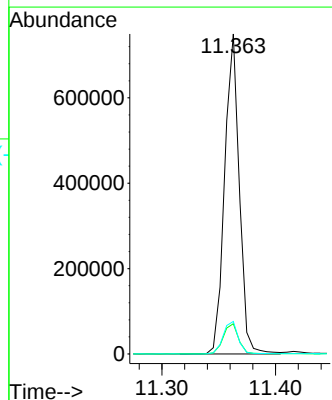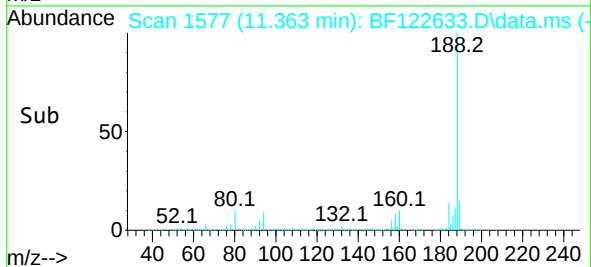

Instrument :
BNA_F
ClientSampleId :
SU-01-120820


Manual Integrations
APPROVED

mohammad
12/10/2020 2:43:36 PM

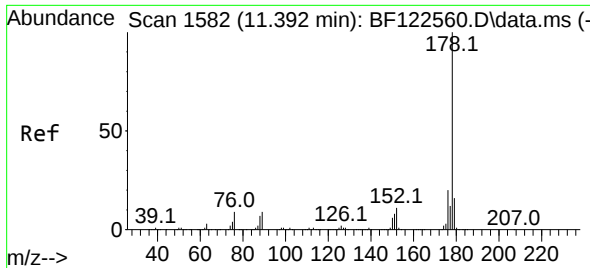

#71
Phenanthrene
Concen: 5.94 ng
RT: 11.386 min Scan# 1581
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08




Instrument :
BNA_F
ClientSampleId :
SU-01-120820

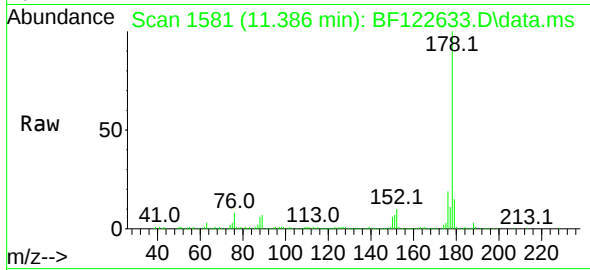


Tgt Ion:178 Resp: 237658
Ion Ratio Lower Upper
178 100
176 19.2 16.2 24.2
179 15.2 12.7 19.1

Manual Integrations
APPROVED



mohammad
12/10/2020 2:43:36 PM

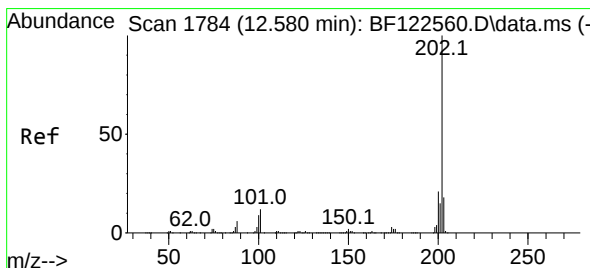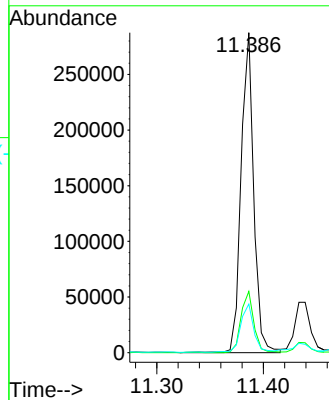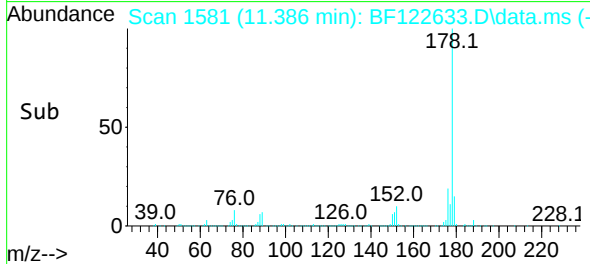


#75
Fluoranthene
Concen: 8.69 ng
RT: 12.575 min Scan# 1783
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

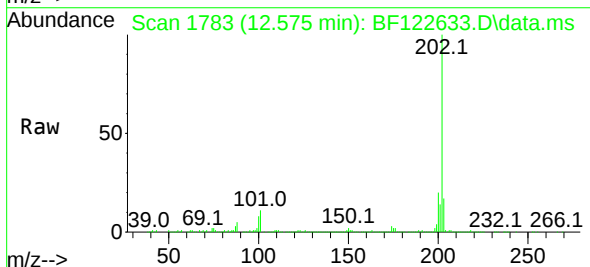


Tgt Ion:202 Resp: 364773
Ion Ratio Lower Upper
202 100
101 11.0 0.0 32.2
203 17.2 0.0 38.1


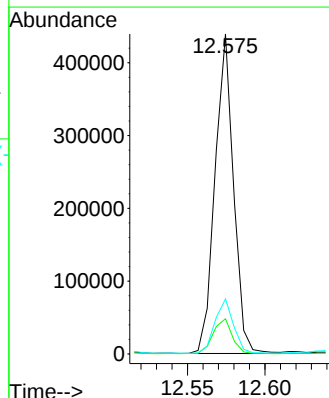
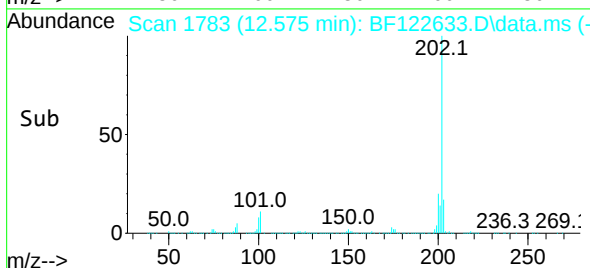





#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.004 min Scan# 2026
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

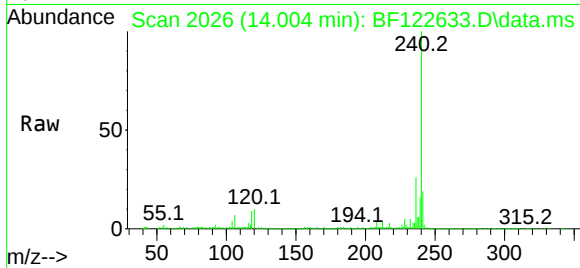



Tgt Ion:240 Resp: 498586
Ion Ratio Lower Upper
240 100
120 9.9 8.6 12.8
236 25.7 20.3 30.5

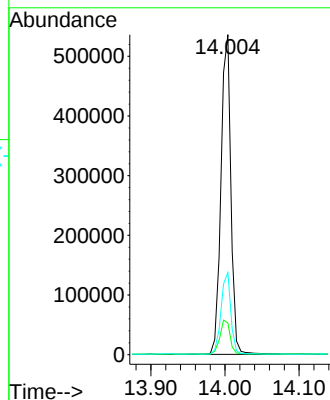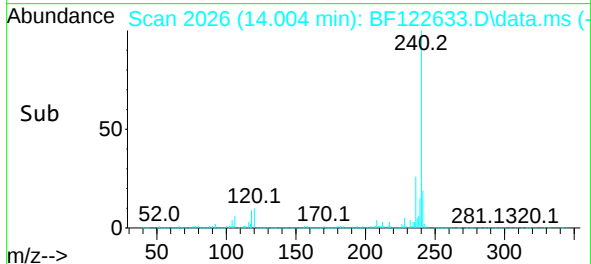

#78
Pyrene
Concen: 8.94 ng
RT: 12.804 min Scan# 1822
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

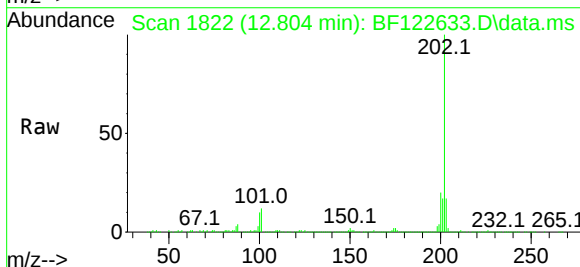


Tgt Ion:202 Resp: 344563
Ion Ratio Lower Upper
202 100
200 20.5 17.6 26.4
203 17.0 14.6 21.8

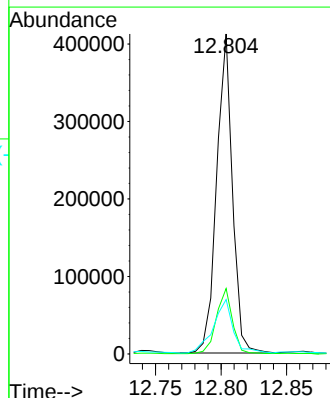

Instrument :
BNA_F
ClientSampleId :
SU-01-120820


Manual Integrations
APPROVED

mohammad
12/10/2020 2:43:36 PM



#79
Terphenyl-d14
Concen: 23.67 ng
RT: 12.945 min Scan# 1846
Delta R.T. -0.012 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08




Instrument :
BNA_F
ClientSampleId :
SU-01-120820




Tgt Ion:244 Resp: 674256
Ion Ratio Lower Upper
244 100
212 6.6 5.7 8.5
122 10.7 8.3 12.5

Manual Integrations
APPROVED



mohammad
12/10/2020 2:43:36 PM

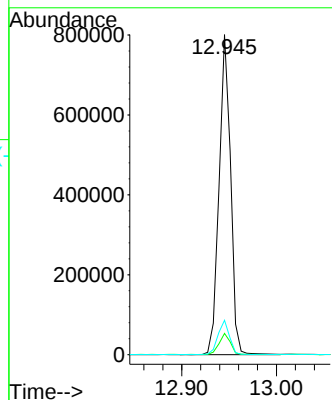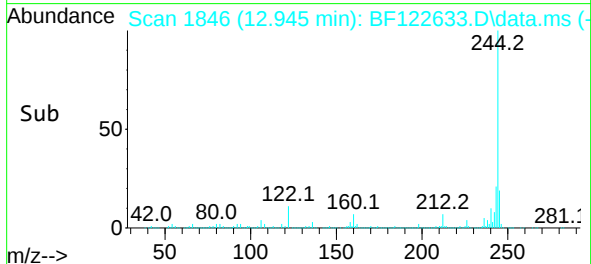


#81
Benzo(a)anthracene
Concen: 4.60 ng
RT: 13.992 min Scan# 2024
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

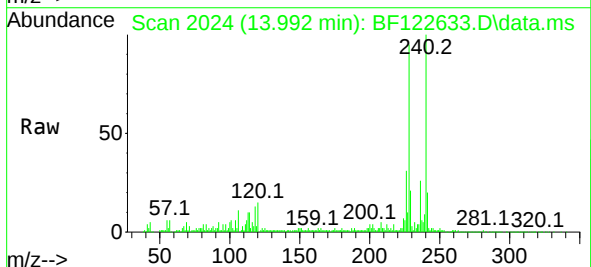


Tgt Ion:228 Resp: 153394
Ion Ratio Lower Upper
228 100
226 32.5 23.0 34.4
229 22.4 16.6 24.8


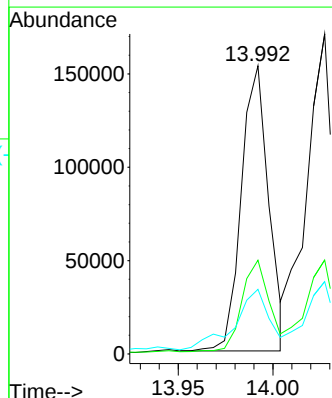



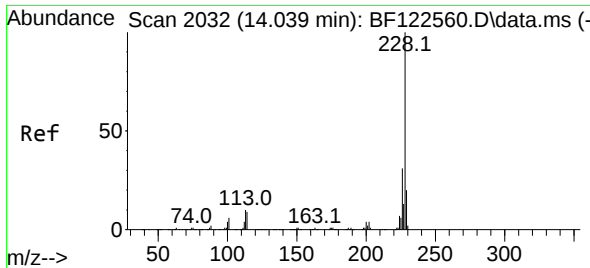


#83
Chrysene
Concen: 5.13 ng
RT: 14.027 min Scan# 2030
Delta R.T. -0.012 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

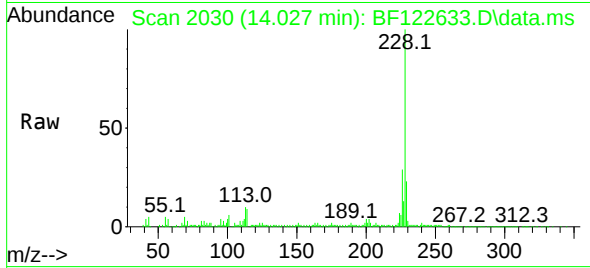



Tgt Ion:228 Resp: 170094
Ion Ratio Lower Upper
228 100
226 29.4 24.6 36.8
229 22.6 15.8 23.6

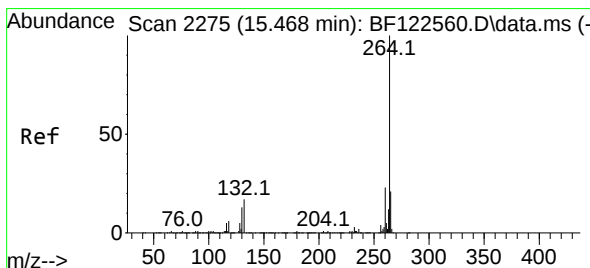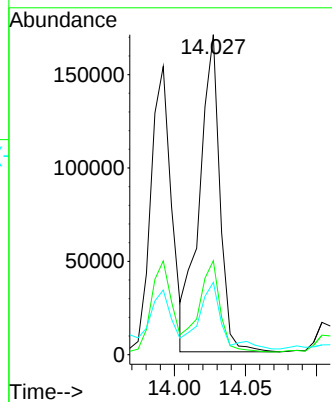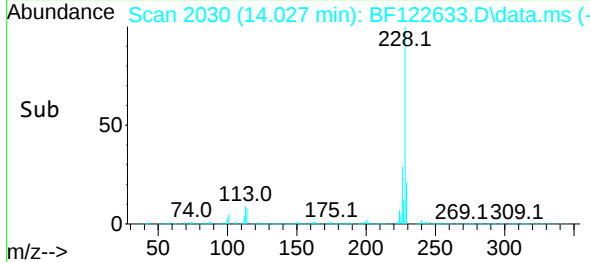

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.468 min Scan# 2275
Delta R.T. 0.000 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

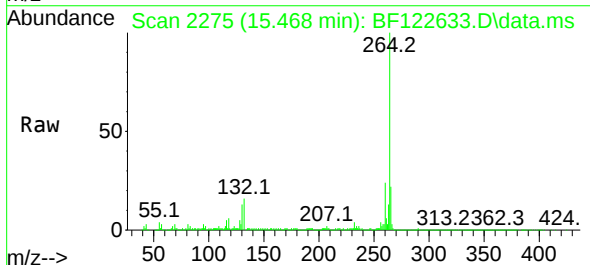


Tgt Ion:264 Resp: 529560
Ion Ratio Lower Upper
264 100
260 23.8 18.6 28.0
265 22.2 17.0 25.6

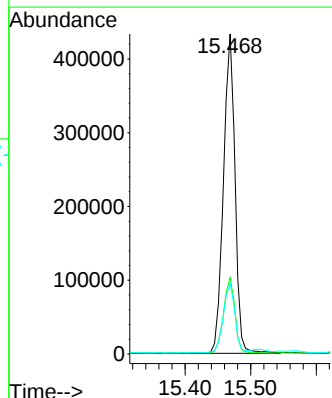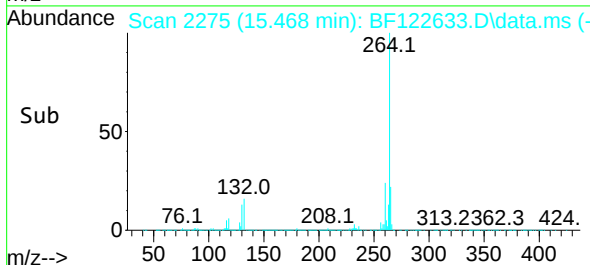

Instrument :
BNA_F
ClientSampleId :
SU-01-120820

Manual Integrations
APPROVED

mohammad
12/10/2020 2:43:36 PM

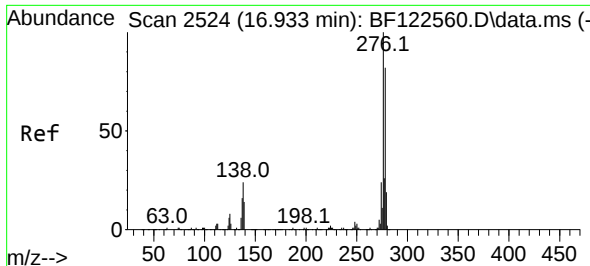





#87
Indeno(1,2,3-cd)pyrene
Concen: 2.45 ng
RT: 16.915 min Scan# 2521
Delta R.T. -0.018 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

Tgt Ion: 276 Resp: 85028
Ion Ratio Lower Upper
276 100
138 21.4 18.7 28.1
277 24.1 20.2 30.4

Instrument :
BNA_F
ClientSampleId :
SU-01-120820




Manual Integrations
APPROVED


mohammad
12/10/2020 2:43:36 PM

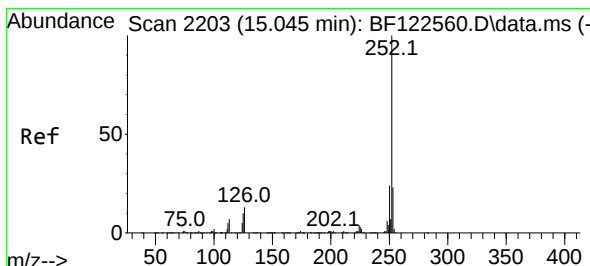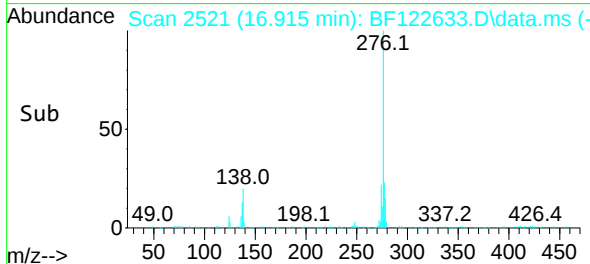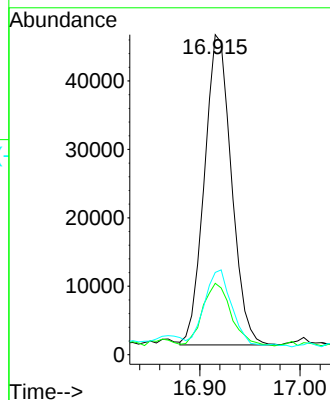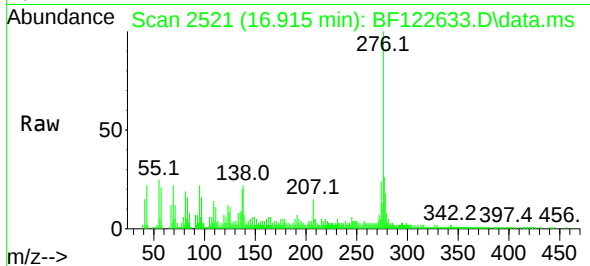

#88
Benzo(b)fluoranthene
Concen: 5.70 ng m
RT: 15.039 min Scan# 2202
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

Tgt Ion: 252 Resp: 211630
Ion Ratio Lower Upper
252 100
253 23.5 18.3 27.5
125 12.2 8.1 12.1#

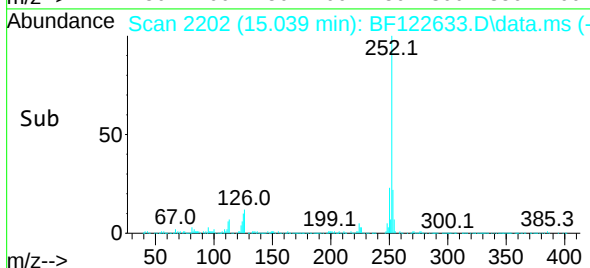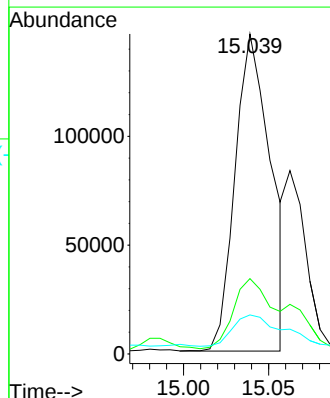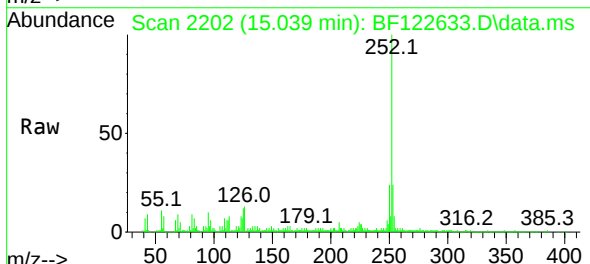

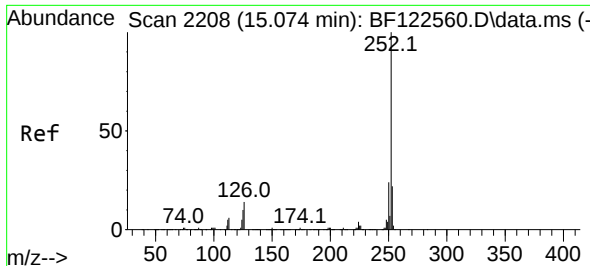





#89
Benzo(k)fluoranthene
Concen: 2.04 ng m
RT: 15.063 min Scan# 2206
Delta R.T. -0.012 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

Tgt Ion:252 Resp: 69184
Ion Ratio Lower Upper
252 100
253 27.1 17.8 26.8#
125 13.5 8.4 12.6#

Instrument :
BNA_F
ClientSampleId :
SU-01-120820




Manual Integrations
APPROVED


mohammad
12/10/2020 2:43:36 PM

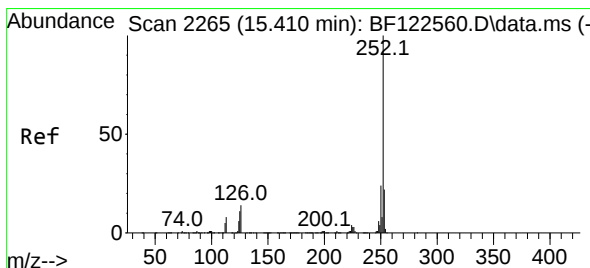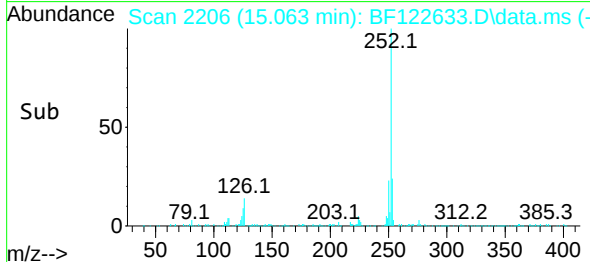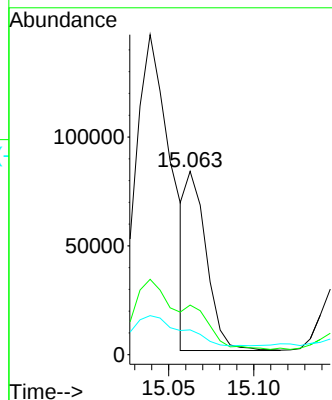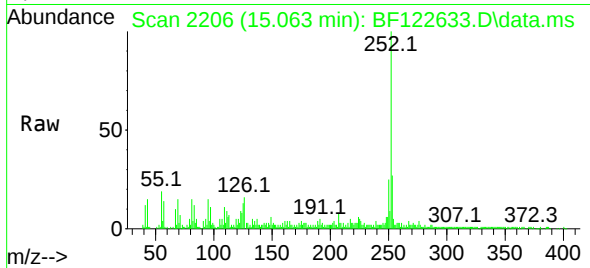

#90
Benzo(a)pyrene
Concen: 4.67 ng
RT: 15.404 min Scan# 2264
Delta R.T. -0.006 min
Lab File: BF122633.D
Acq: 10 Dec 2020 3:08

Tgt Ion:252 Resp: 151793
Ion Ratio Lower Upper
252 100
253 23.1 17.5 26.3
125 11.5 8.6 12.8

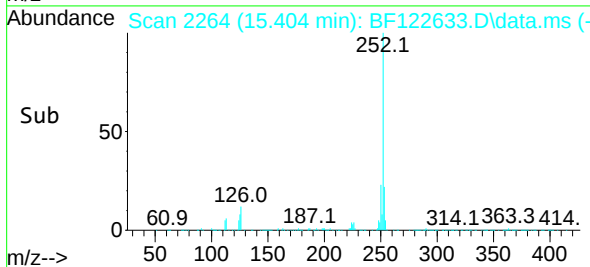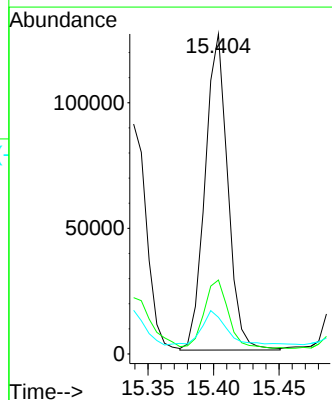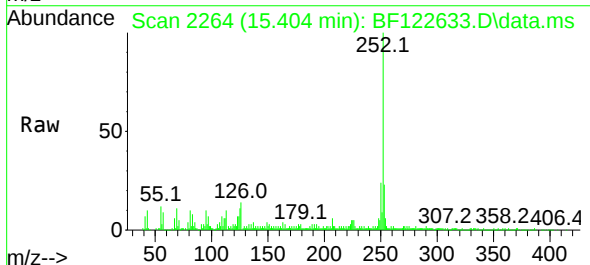

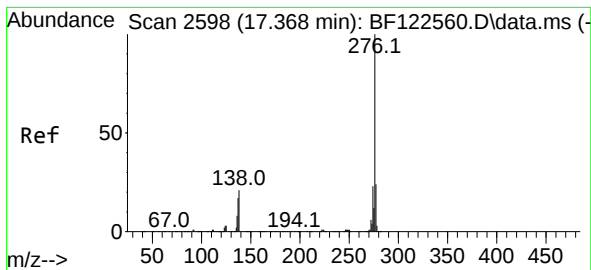

#92

Benzo(g,h,i)perylene

Concen: 3.09 ng

RT: 17.357 min Scan# 2596

Delta R.T. -0.012 min

Lab File: BF122633.D

Acq: 10 Dec 2020 3:08

Tgt Ion:	276	Resp:	85178
Ion Ratio	Lower	Upper	
276	100		
277	25.7	19.3	28.9
138	21.1	16.6	24.8

Instrument :

BNA_F

ClientSampleId :

SU-01-120820

Manual Integrations
APPROVED

mohammad
12/10/2020 2:43:36 PM

