

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122606.D
Acq On : 9 Dec 2020 11:00
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	570	576	579	rBV	5372030	6495009	72.66%	13.190%
2	6.481	740	747	750	rBV	4895058	6510259	72.83%	13.221%
3	6.840	804	808	811	rBV	1412217	1088143	12.17%	2.210%
4	7.404	898	904	907	rBV	3587523	4445016	49.73%	9.027%
5	8.122	1021	1026	1039	rBV	1581883	1476168	16.51%	2.998%
6	9.204	1203	1210	1213	rBV	6682745	7665497	85.75%	15.567%
7	9.875	1319	1324	1328	rBV	1800403	1744352	19.51%	3.542%
8	10.669	1453	1459	1484	rBV	4563463	5543222	62.01%	11.257%
9	11.363	1572	1577	1584	rBV	2080268	1832247	20.50%	3.721%
10	12.957	1841	1848	1851	rBV2	7298291	8938879	100.00%	18.152%
11	14.004	2021	2026	2040	rVB	1797651	1829714	20.47%	3.716%
12	15.463	2269	2274	2299	rBV	1115113	1674780	18.74%	3.401%




Sum of corrected areas: 49243286

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122606.D
Acq On : 9 Dec 2020 11:00
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

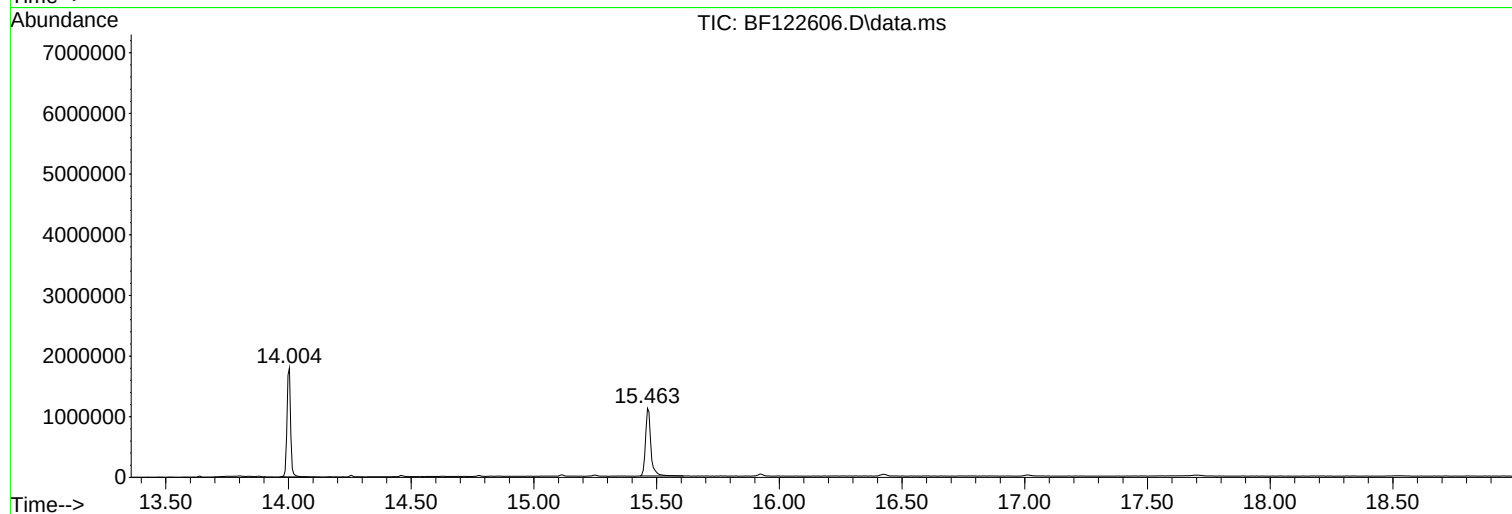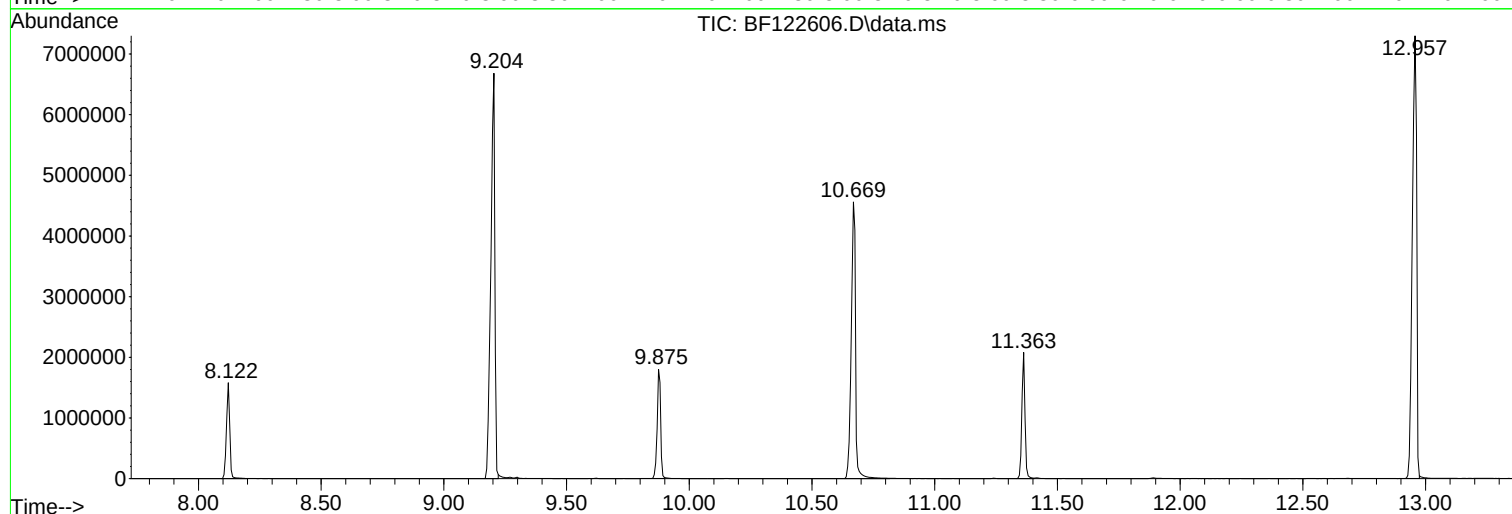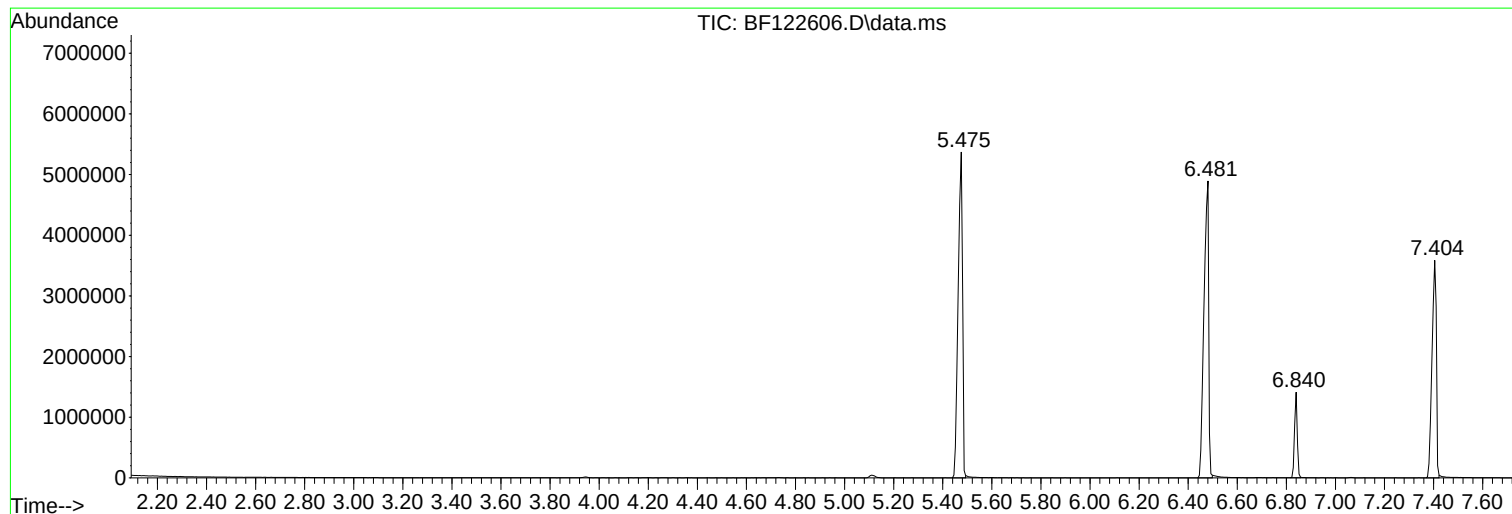

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122606.D
Acq On : 9 Dec 2020 11:00
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122606.D
Acq On : 9 Dec 2020 11:00
Operator : JU/CG
Sample : PB133460BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133460BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------