

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
 Data File : BF122610.D
 Acq On : 9 Dec 2020 13:34
 Operator : JU/CG
 Sample : L4969-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NORTH-BRANFORD-01

Integration Parameters: rteint.p

Integrator: RTE

Smothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	4	6	13	rVB2	49346	68487	1.56%	0.203%
2	5.457	568	573	577	rBV	3312790	3469521	79.27%	10.305%
3	5.787	624	629	640	rBV	60711	75530	1.73%	0.224%
4	6.469	740	745	762	rBV	3318793	3693091	84.37%	10.969%
5	6.663	776	778	792	rVB	89353	118985	2.72%	0.353%
6	6.839	804	808	811	rBV	1188392	995493	22.74%	2.957%
7	7.398	898	903	906	rBV	2326985	2349735	53.68%	6.979%
8	7.869	978	983	992	rBV5	15873	52790	1.21%	0.157%
9	8.122	1022	1026	1043	rVB	1533772	1330443	30.40%	3.952%
10	9.198	1204	1209	1212	rBV	4805755	4377052	100.00%	13.001%
11	9.592	1272	1276	1279	rBV	218816	224707	5.13%	0.667%
12	9.875	1320	1324	1328	rBV	1745956	1507541	34.44%	4.478%
13	10.663	1454	1458	1469	rBV	2206930	2061211	47.09%	6.122%
14	11.257	1556	1559	1562	rBV2	70516	72841	1.66%	0.216%
15	11.363	1573	1577	1579	rBV	1661598	1462945	33.42%	4.345%
16	11.386	1579	1581	1587	rVB	190860	198925	4.54%	0.591%
17	11.516	1599	1603	1605	rBV4	50544	69875	1.60%	0.208%
18	11.545	1605	1608	1611	rBV2	52333	67488	1.54%	0.200%
19	11.898	1663	1668	1675	rBV	1201831	1525311	34.85%	4.531%
20	12.069	1695	1697	1700	rBV	85851	83746	1.91%	0.249%
21	12.216	1720	1722	1724	rBV2	84764	83979	1.92%	0.249%
22	12.345	1742	1744	1748	rBV2	98063	133323	3.05%	0.396%
23	12.386	1748	1751	1753	rVB	138520	134539	3.07%	0.400%
24	12.457	1760	1763	1765	rBV2	114320	141895	3.24%	0.421%
25	12.574	1780	1783	1785	rBV	342086	309667	7.07%	0.920%
26	12.639	1792	1794	1797	rBV2	115966	97525	2.23%	0.290%
27	12.686	1797	1802	1807	rBV	1369225	1693699	38.69%	5.031%
28	12.804	1819	1822	1824	rBV	352427	285709	6.53%	0.849%
29	12.951	1842	1847	1850	rBV	4446141	4224190	96.51%	12.547%
30	14.004	2021	2026	2029	rBV	1277873	1308372	29.89%	3.886%
31	15.039	2199	2202	2205	rBV	138637	181837	4.15%	0.540%
32	15.468	2270	2275	2283	rVB	913795	1266646	28.94%	3.762%


Sum of corrected areas: 33667098

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122610.D
Acq On : 9 Dec 2020 13:34
Operator : JU/CG
Sample : L4969-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

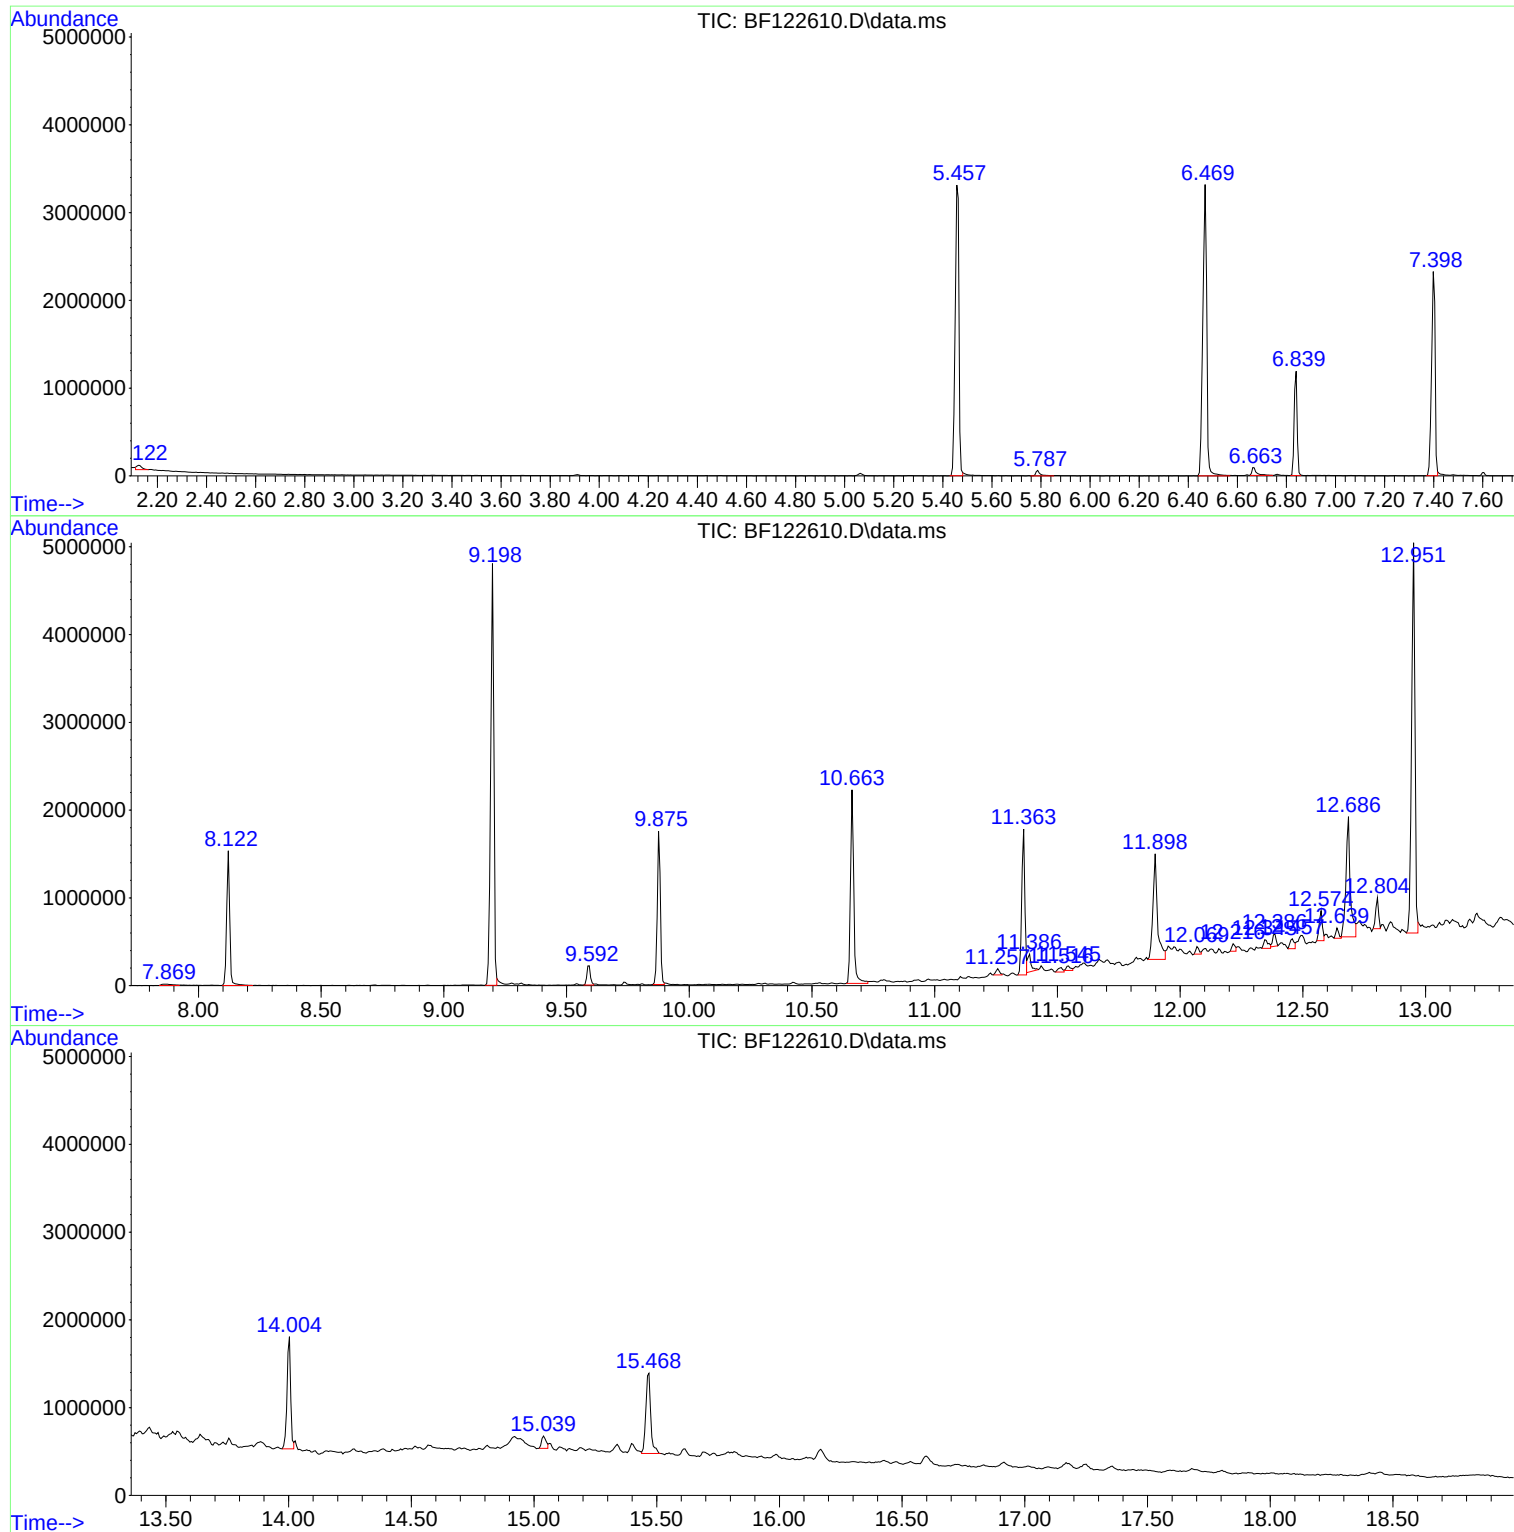

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122610.D
Acq On : 9 Dec 2020 13:34
Operator : JU/CG
Sample : L4969-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122610.D
Acq On : 9 Dec 2020 13:34
Operator : JU/CG
Sample : L4969-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------