

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
 Data File : BF122611.D
 Acq On : 9 Dec 2020 14:05
 Operator : JU/CG
 Sample : L4969-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NORTH-BRANFORD-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	500	505	511	rBV	32027	42412	1.08%	0.147%
2	5.457	568	573	576	rBV	3251706	3062193	78.15%	10.629%
3	5.787	625	629	640	rBV	53070	61127	1.56%	0.212%
4	6.469	740	745	748	rBV	3189458	3185163	81.29%	11.056%
5	6.663	776	778	792	rBV	79699	108445	2.77%	0.376%
6	6.839	804	808	811	rBV	1233384	976164	24.91%	3.388%
7	7.398	898	903	906	rBV	2101544	2084469	53.20%	7.235%
8	8.122	1022	1026	1038	rBV	1488753	1285972	32.82%	4.464%
9	9.198	1204	1209	1212	rBV	4351436	3918323	100.00%	13.601%
10	9.592	1272	1276	1284	rBV	212872	195331	4.99%	0.678%
11	9.874	1320	1324	1334	rVB	1492217	1463814	37.36%	5.081%
12	10.663	1454	1458	1469	rBV	1855759	1739998	44.41%	6.040%
13	10.798	1475	1481	1487	rVB	50626	66179	1.69%	0.230%
14	10.851	1487	1490	1492	rBV	95212	101577	2.59%	0.353%
15	10.880	1492	1495	1499	rVV2	106388	143413	3.66%	0.498%
16	10.916	1499	1501	1503	rVV	109337	101896	2.60%	0.354%
17	10.939	1503	1505	1508	rVB2	64015	59161	1.51%	0.205%
18	11.027	1517	1520	1524	rBV3	68666	82089	2.10%	0.285%
19	11.063	1524	1526	1531	rVV	96186	117158	2.99%	0.407%
20	11.104	1531	1533	1538	rVB2	59312	69399	1.77%	0.241%
21	11.363	1573	1577	1580	rBV	1627697	1398352	35.69%	4.854%
22	11.898	1660	1668	1679	rBV	695459	1049684	26.79%	3.643%
23	12.574	1780	1783	1786	rBV	161202	137220	3.50%	0.476%
24	12.680	1796	1801	1812	rBV2	912445	1256935	32.08%	4.363%
25	12.804	1819	1822	1825	rVB	165300	138619	3.54%	0.481%
26	12.951	1842	1847	1850	rBV	3907907	3652733	93.22%	12.679%
27	14.004	2022	2026	2029	rBV	1151966	1135380	28.98%	3.941%
28	15.468	2270	2275	2284	rVB	893755	1176620	30.03%	4.084%




Sum of corrected areas: 28809826

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122611.D
Acq On : 9 Dec 2020 14:05
Operator : JU/CG
Sample : L4969-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

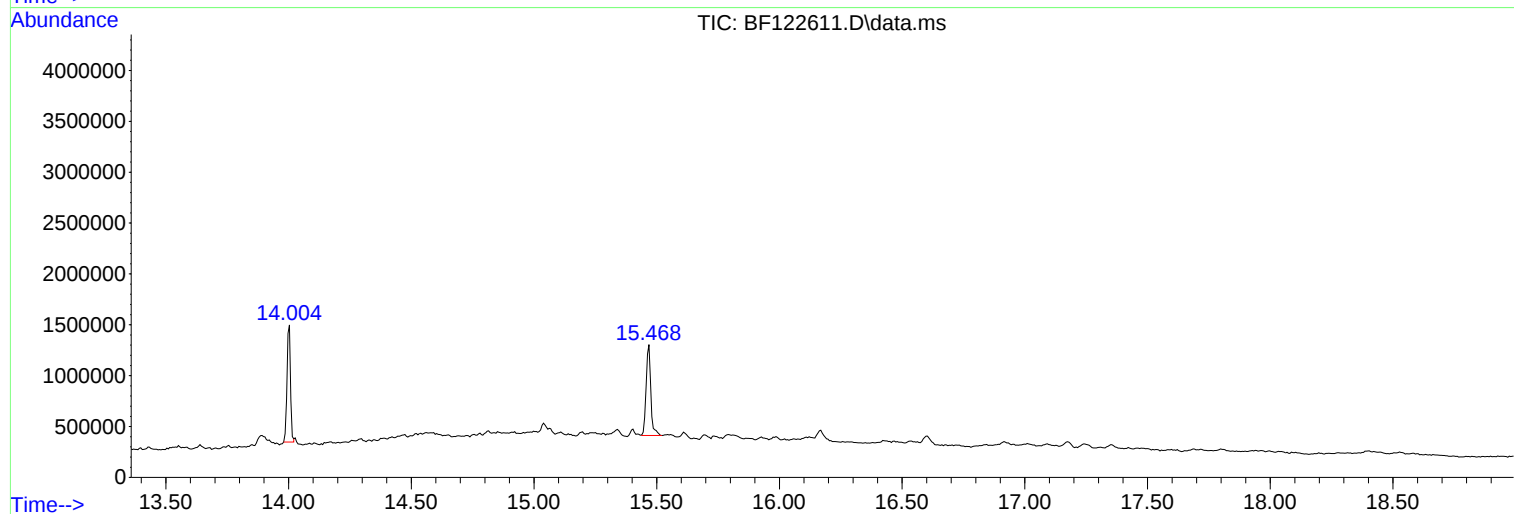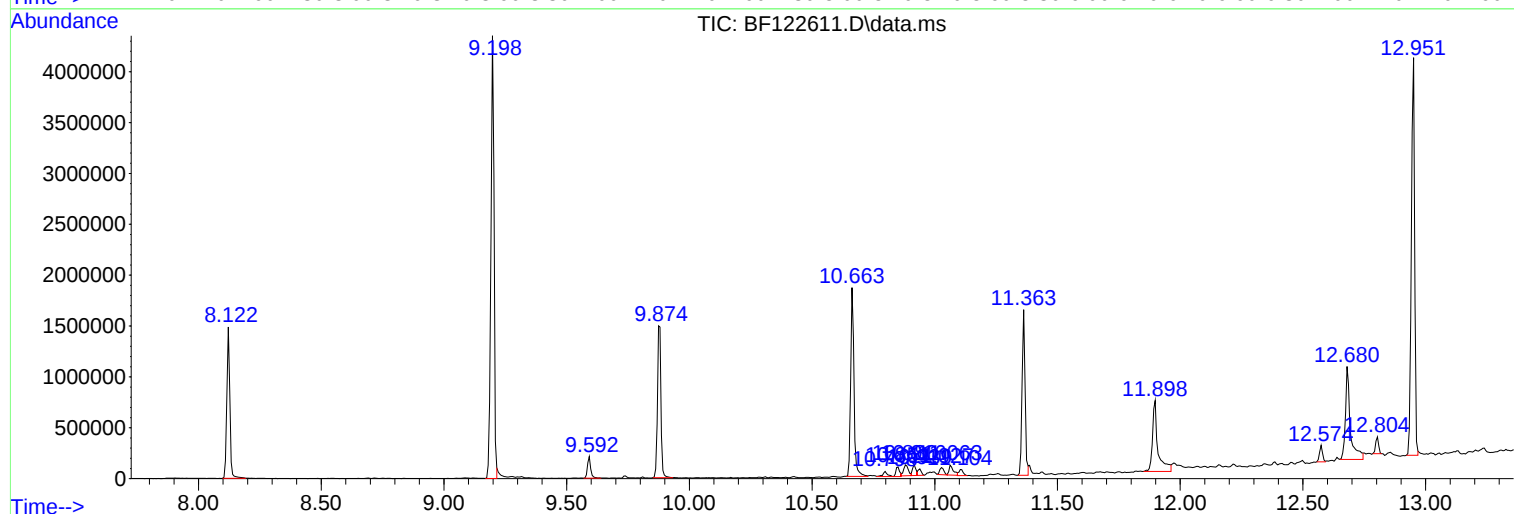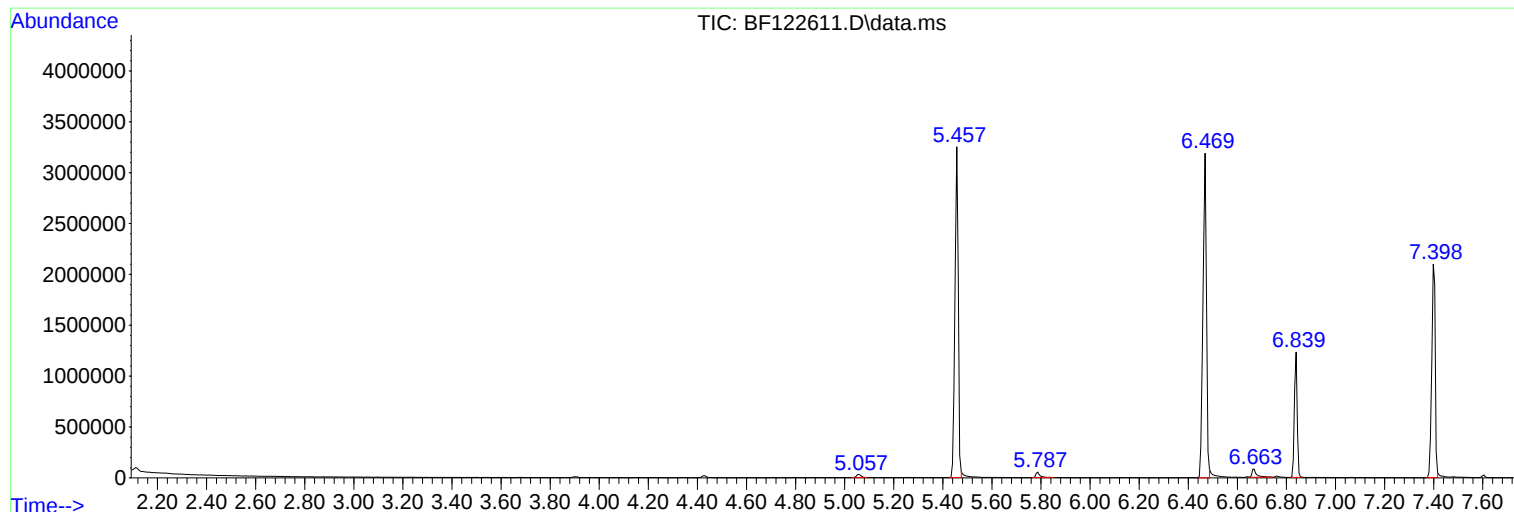

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122611.D
Acq On : 9 Dec 2020 14:05
Operator : JU/CG
Sample : L4969-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122611.D
Acq On : 9 Dec 2020 14:05
Operator : JU/CG
Sample : L4969-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-BRANFORD-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------