

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
 Data File : BF122629.D
 Acq On : 10 Dec 2020 1:03
 Operator : JU/CG
 Sample : L4983-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR1-A-D-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	7	11	16	rVB	44601	59439	1.26%	0.199%
2	2.252	25	28	34	rVB	55437	69059	1.46%	0.231%
3	5.457	569	573	577	rBV	3084249	3233562	68.29%	10.821%
4	6.469	740	745	764	rBV	3314093	3536726	74.69%	11.836%
5	6.840	804	808	811	rBV	1293799	1132507	23.92%	3.790%
6	7.398	898	903	906	rBV	2304302	2254246	47.61%	7.544%
7	8.122	1021	1026	1044	rBV	1718947	1536542	32.45%	5.142%
8	9.198	1204	1209	1212	rBV	4597611	4109795	86.79%	13.754%
9	9.316	1226	1229	1240	rVB	51507	66618	1.41%	0.223%
10	9.592	1272	1276	1285	rBV	262153	307824	6.50%	1.030%
11	9.875	1319	1324	1333	rBV	1917119	1820366	38.44%	6.092%
12	10.663	1454	1458	1469	rBV	1141276	1237682	26.14%	4.142%
13	11.363	1573	1577	1585	rBV	2055573	1931507	40.79%	6.464%
14	12.574	1780	1783	1787	rVB	90635	86004	1.82%	0.288%
15	12.804	1819	1822	1825	rBV	67819	53791	1.14%	0.180%
16	12.951	1842	1847	1850	rBV	4979567	4735242	100.00%	15.847%
17	13.851	1996	2000	2005	rBV4	61879	117168	2.47%	0.392%
18	14.004	2020	2026	2029	rBV	1913128	1886033	39.83%	6.312%
19	14.851	2166	2170	2176	rBV	84974	85904	1.81%	0.287%
20	15.039	2198	2202	2205	rBV	35725	54468	1.15%	0.182%
21	15.462	2268	2274	2285	rBV	1157313	1512904	31.95%	5.063%
22	15.921	2347	2352	2359	rBV2	33127	54220	1.15%	0.181%




Sum of corrected areas: 29881607

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122629.D
Acq On : 10 Dec 2020 1:03
Operator : JU/CG
Sample : L4983-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR1-A-D-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

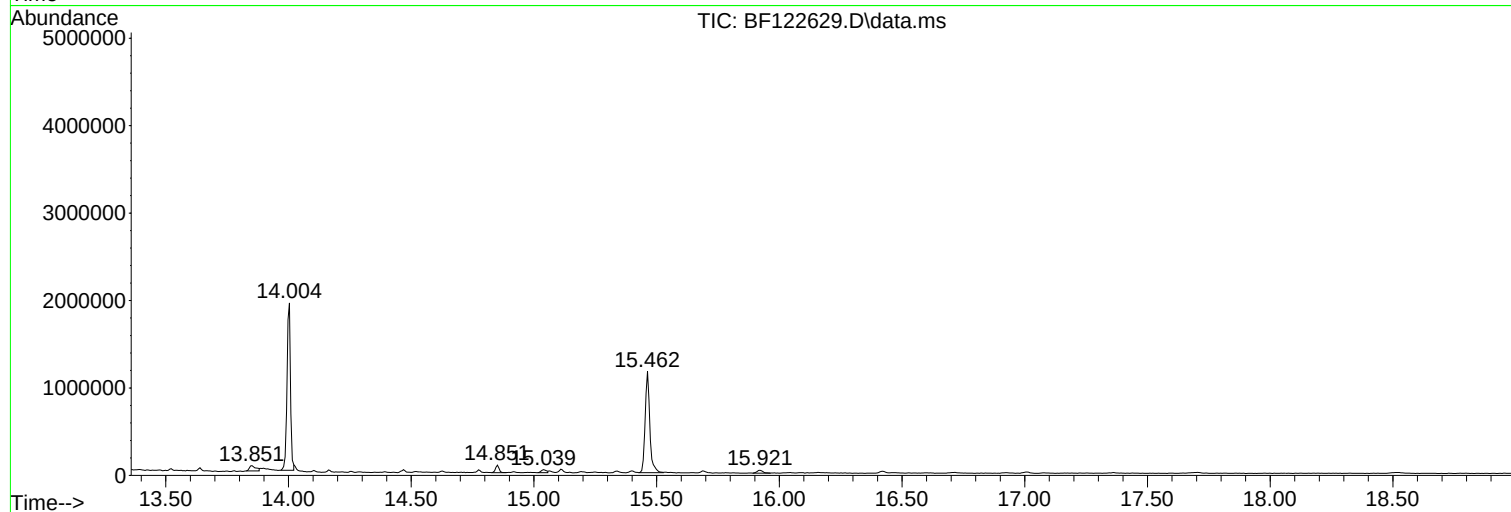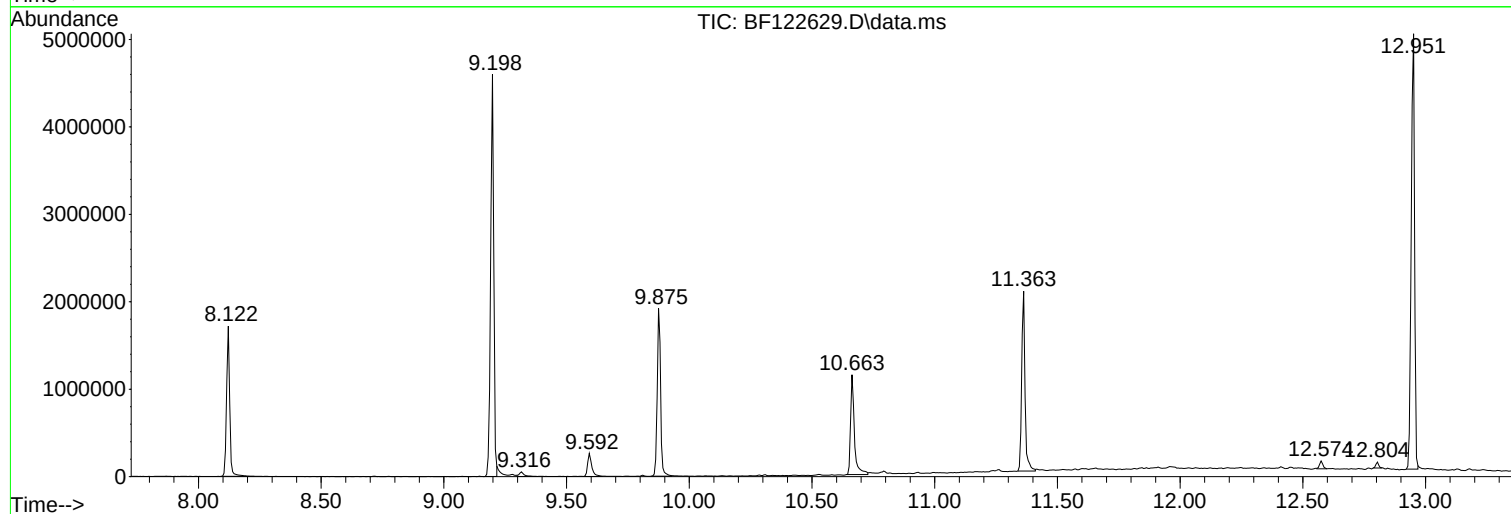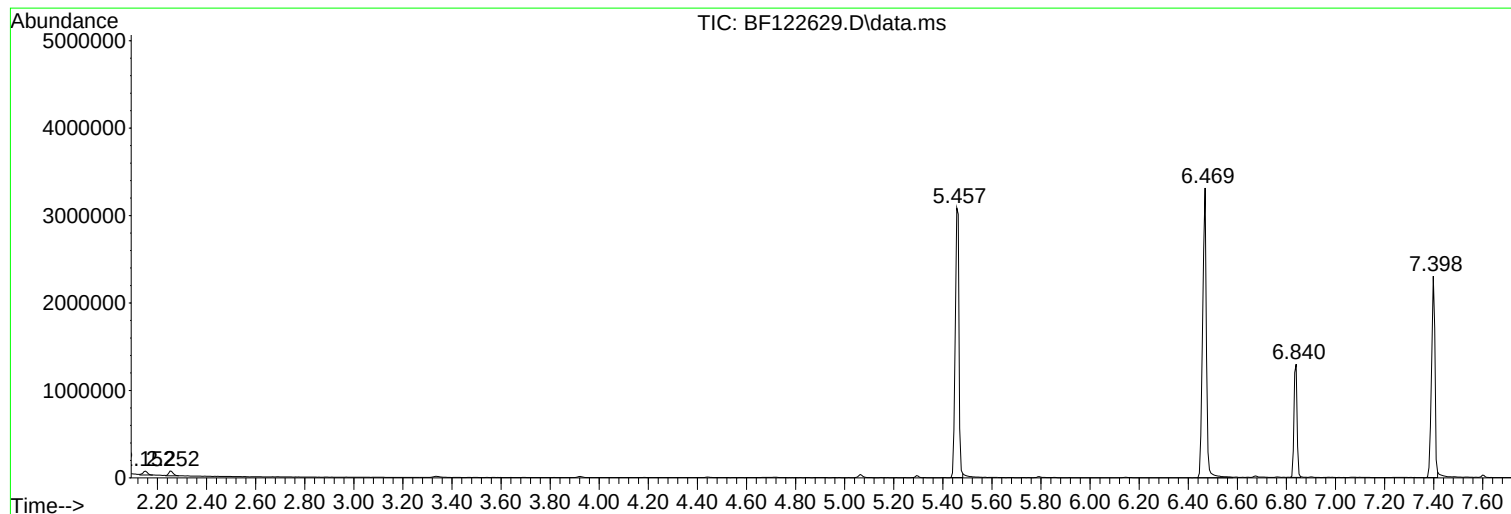

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122629.D
Acq On : 10 Dec 2020 1:03
Operator : JU/CG
Sample : L4983-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR1-A-D-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
Data File : BF122629.D
Acq On : 10 Dec 2020 1:03
Operator : JU/CG
Sample : L4983-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR1-A-D-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------