
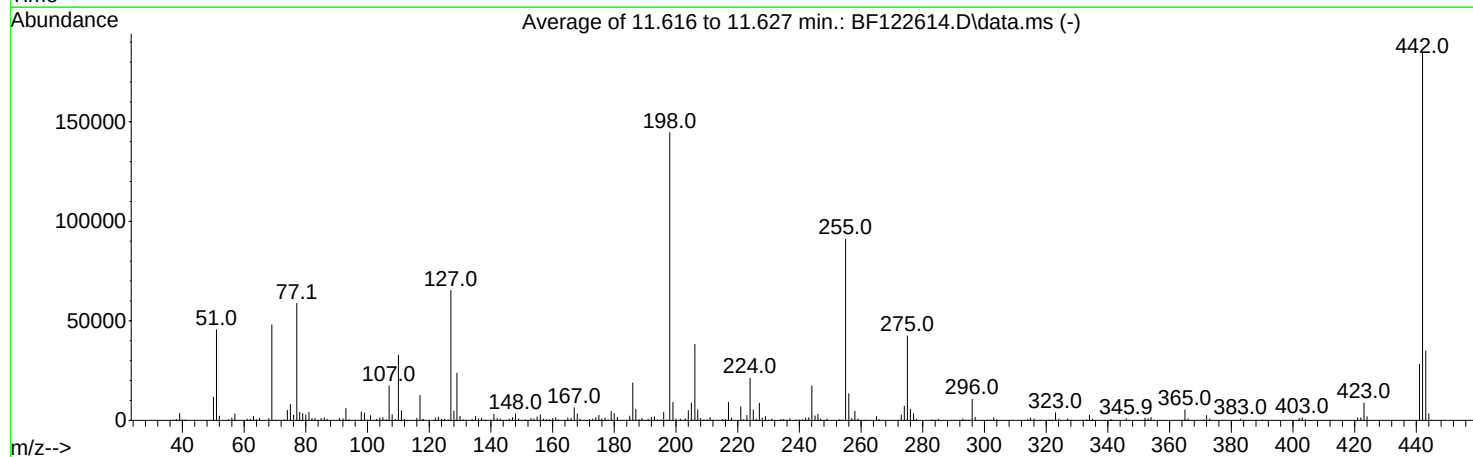


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120920\
 Data File : BF122614.D
 Acq On : 9 Dec 2020 16:51
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 07 12:08:49 2020

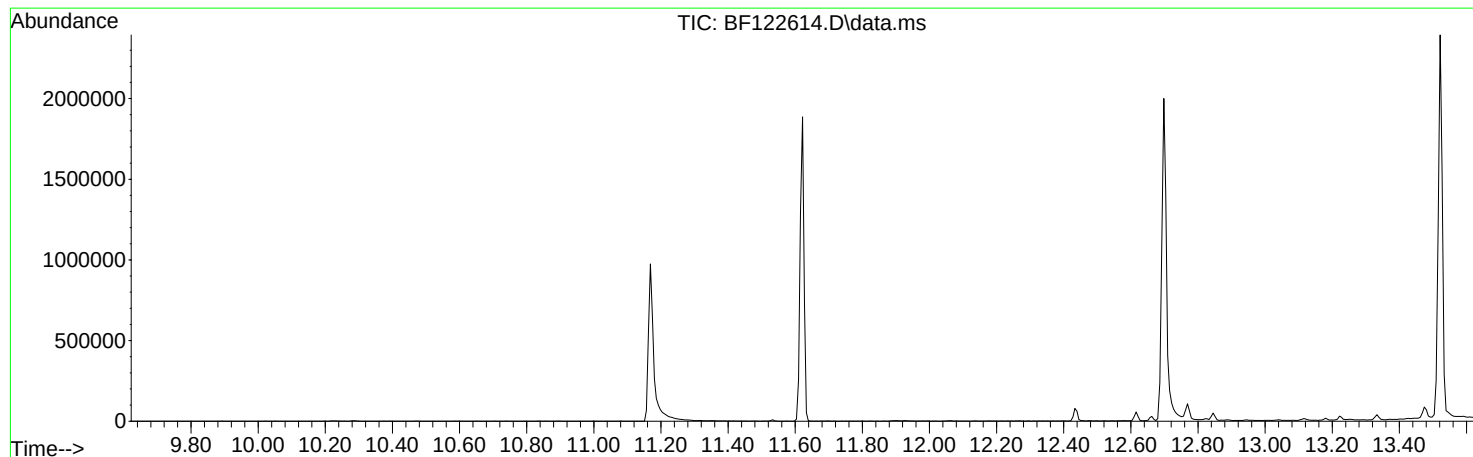

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	45596	PASS
68	69	0.00	2	1.9	906	PASS
69	198	0.00	100	33.2	47962	PASS
70	69	0.00	2	0.2	116	PASS
127	198	10	80	45.1	65216	PASS
197	198	0.00	2	0.1	212	PASS
198	198	100	100	100.0	144605	PASS
199	198	5	9	6.3	9069	PASS
275	198	10	60	29.3	42440	PASS
365	198	1	100	3.7	5295	PASS
441	198	0.01	100	19.5	28127	PASS
442	442	100	100	100.0	184819	PASS
443	442	15	24	18.9	34912	PASS