


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120924\
Data File : BF140782.D
Acq On : 09 Dec 2024 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

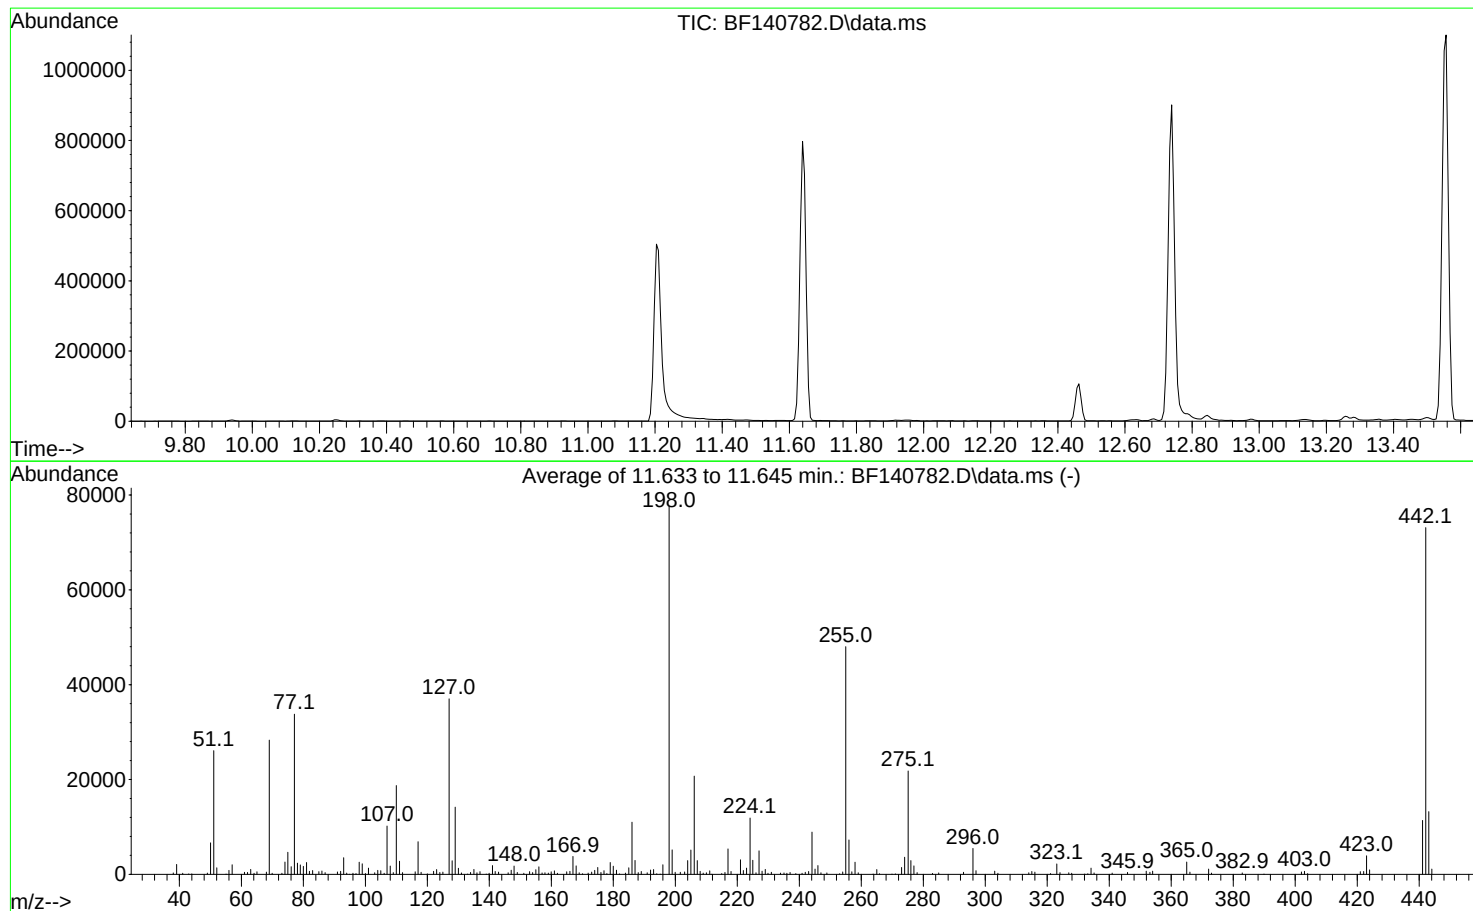

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	26080	PASS
68	69	0.00	2	1.6	463	PASS
69	198	0.00	100	36.5	28325	PASS
70	69	0.00	2	0.8	234	PASS
127	198	10	80	47.7	37035	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77573	PASS
199	198	5	9	6.7	5170	PASS
275	198	10	60	28.1	21805	PASS
365	198	1	100	3.4	2612	PASS
441	198	0.01	100	14.7	11365	PASS
442	442	50	100	100.0	73117	PASS
443	442	15	24	18.1	13240	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/9/2024	BNA_F	<u>BF140782.D</u>
Compound Name	Response	Retention Time
DDT	285973	13.557
DDD	7212	13.257
DDE	366	12.915
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7578	293551	2.58

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120924\
Data File : BF140782.D
Acq On : 09 Dec 2024 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 09 14:07:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

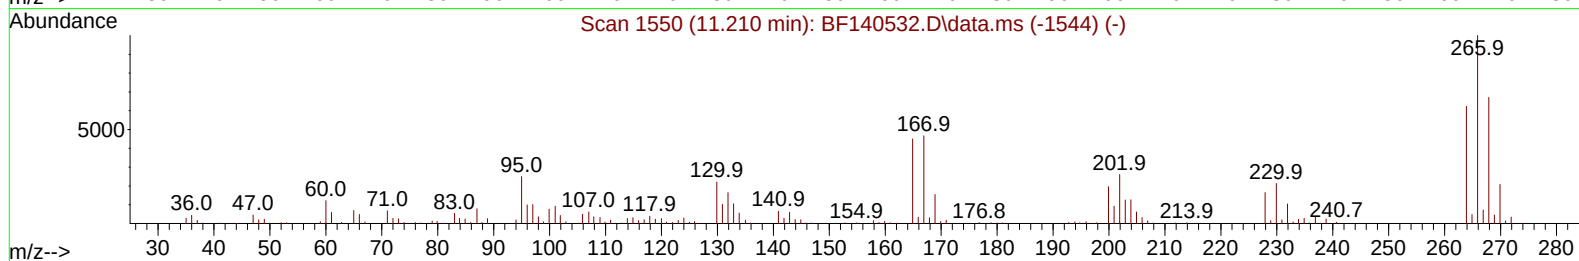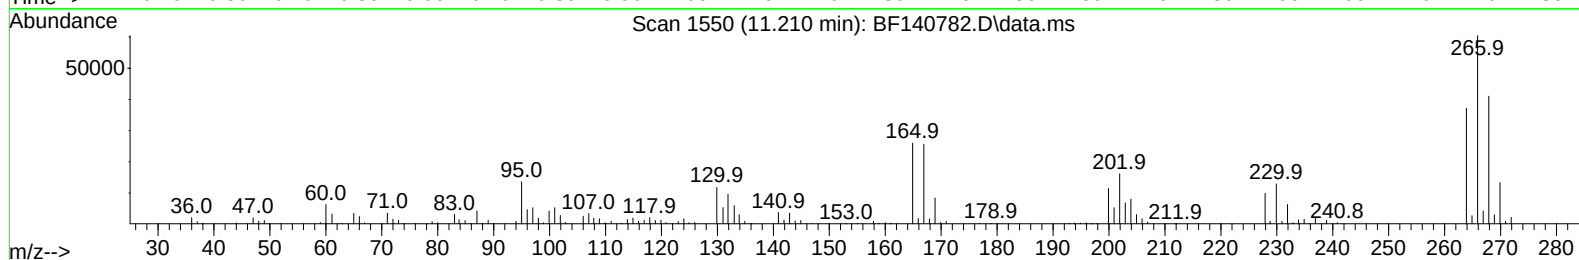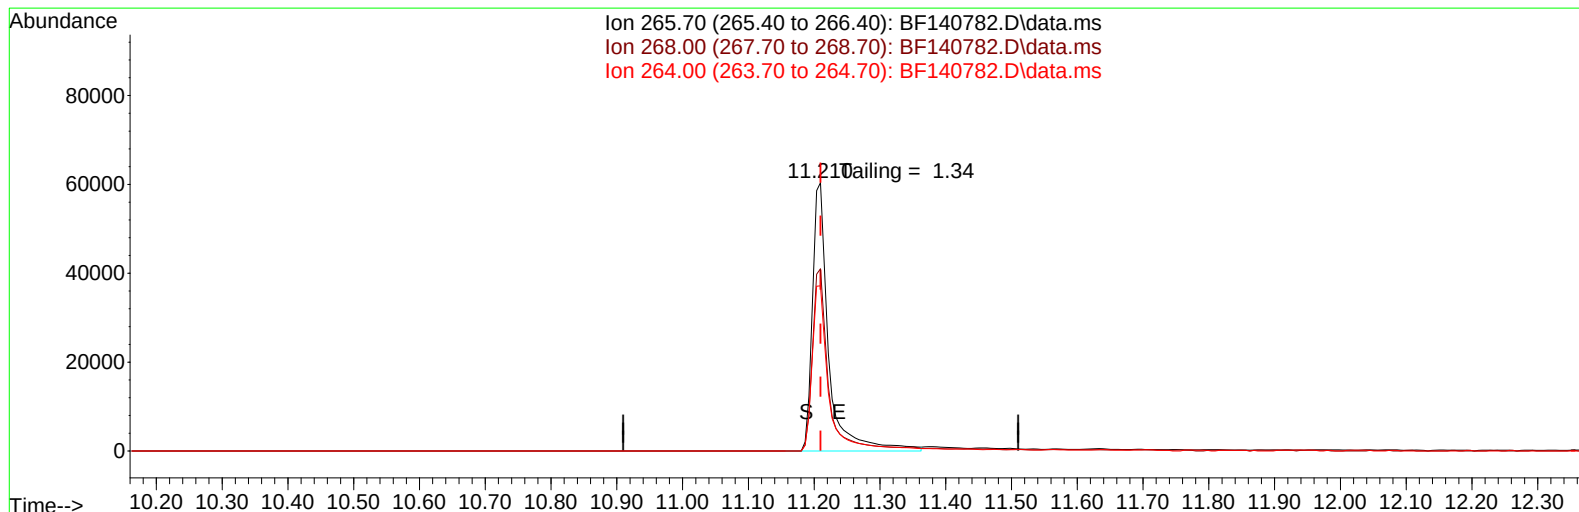

TIC: BF140782.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 21180.55 ng




response 104937

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.92
264.00	62.30	61.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120924\
Data File : BF140782.D
Acq On : 09 Dec 2024 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 09 14:07:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

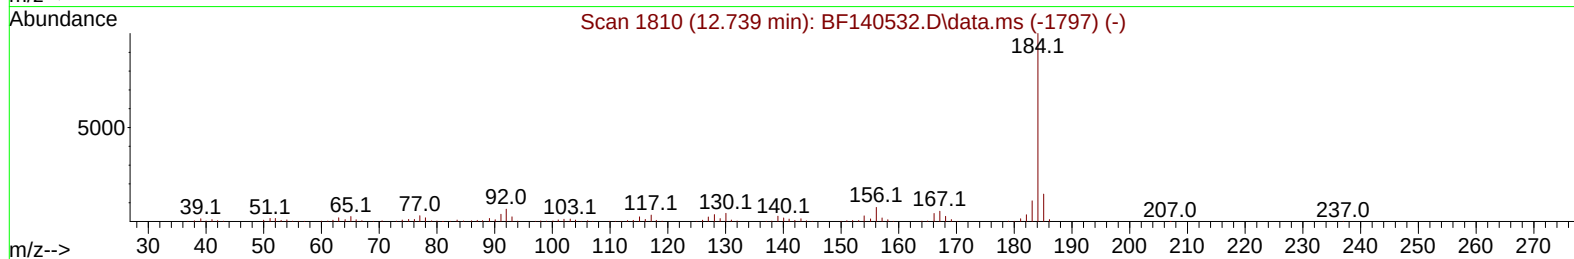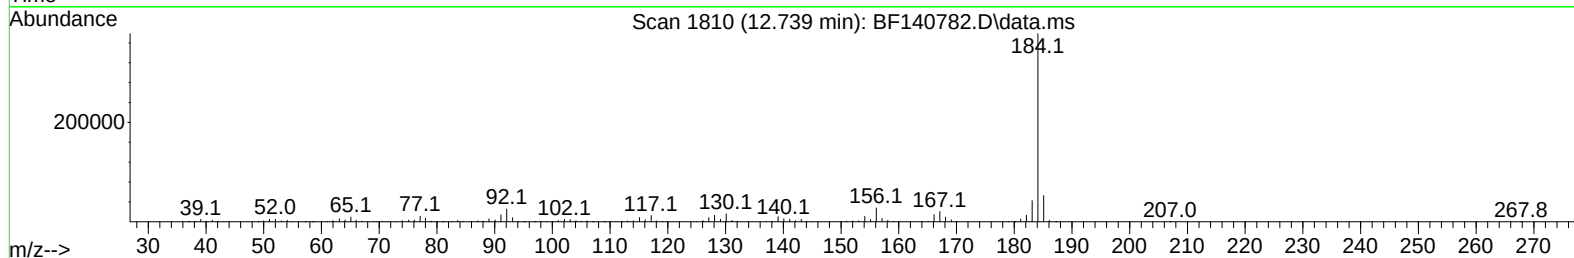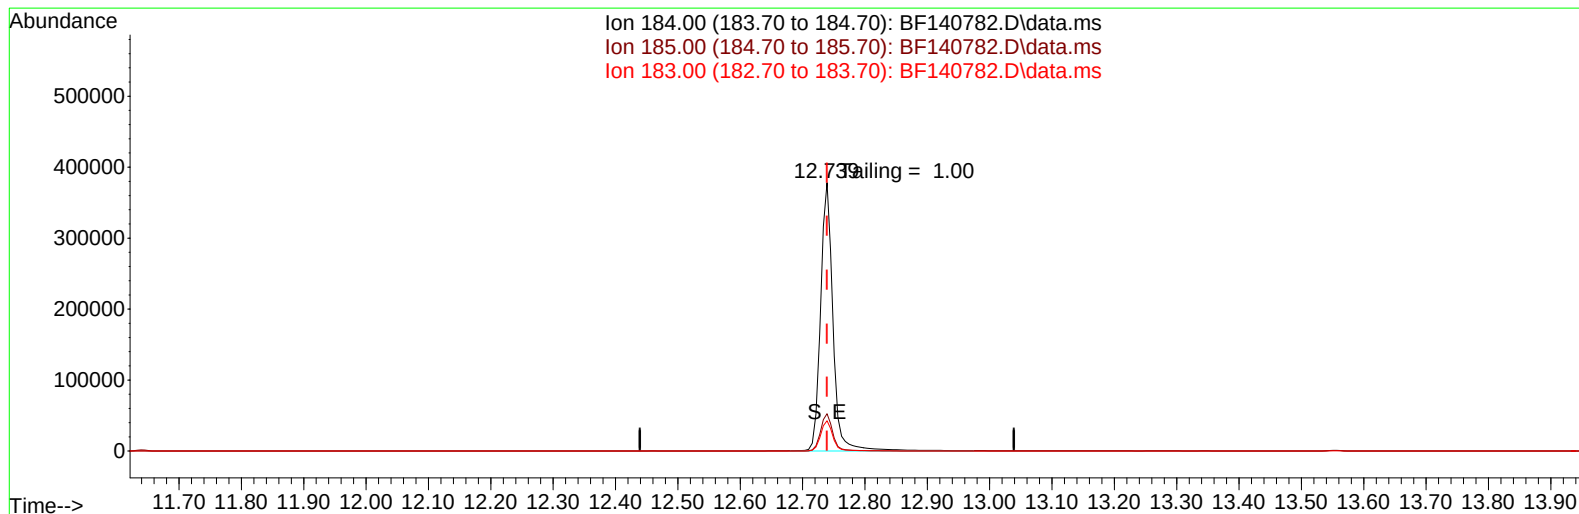

TIC: BF140782.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 20405.35 ng

response 530387

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.90
183.00	11.00	11.26
0.00	0.00	0.00