
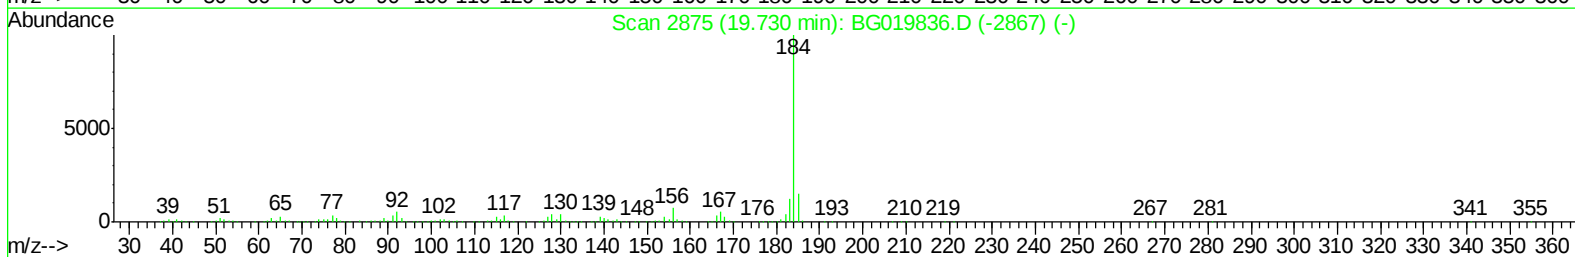
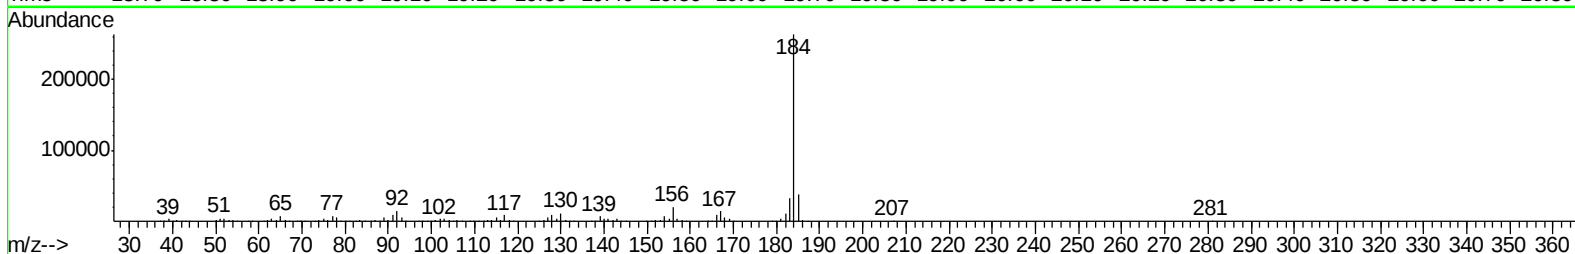


Data Path : Z:\HPCHEM1\BNA_G\Data\BG121115\
Data File : BG020070.D
Acq On : 10 Dec 2015 10:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:30:43 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

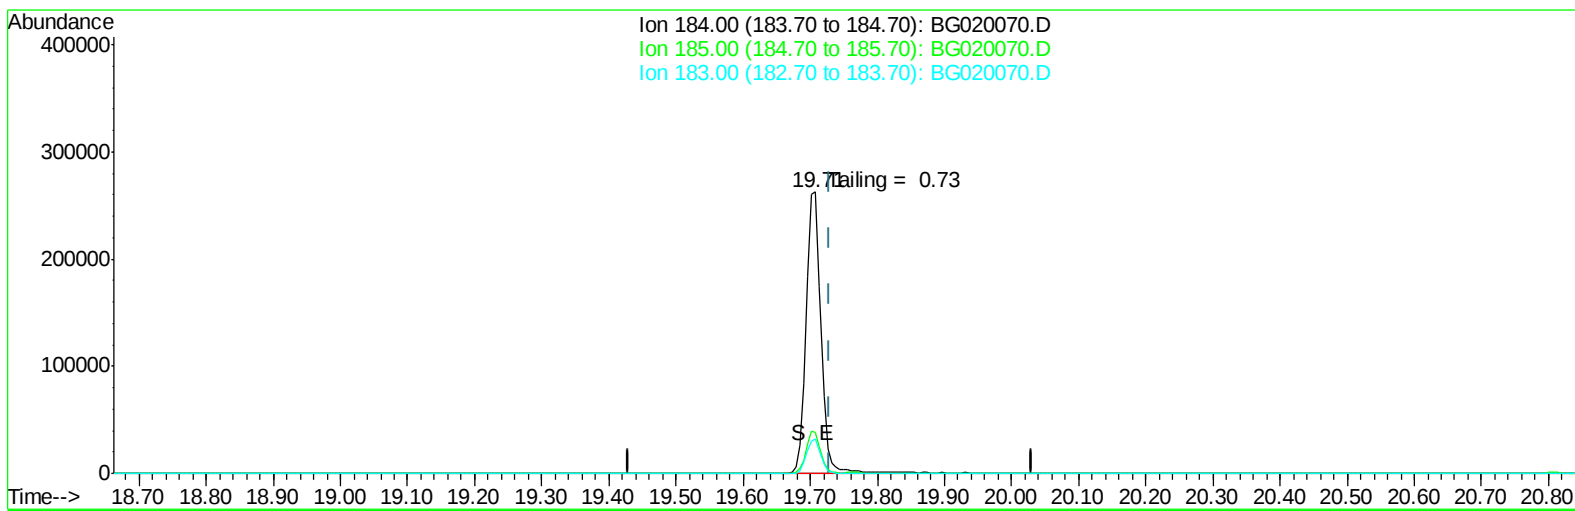

TIC: BG020070.D

(76) Benzidine

19.708min (-0.022) 150906.68ng

response 401512

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.62
183.00	12.60	12.41
0.00	0.00	0.00