
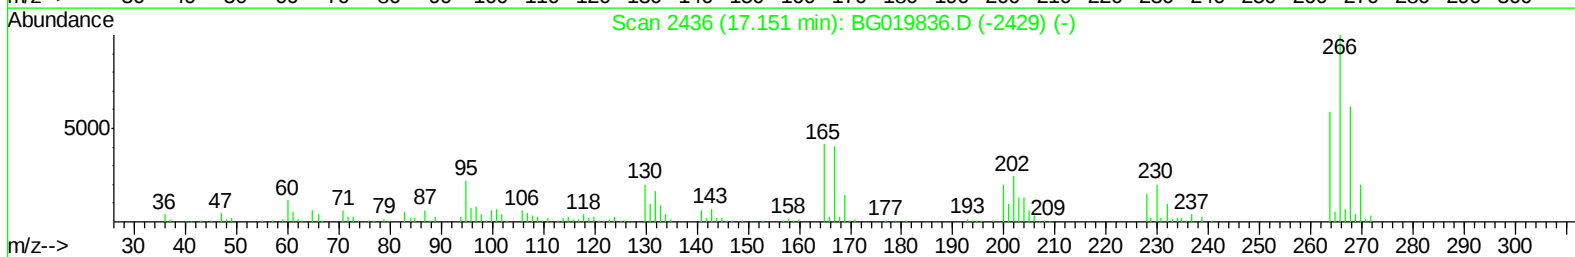
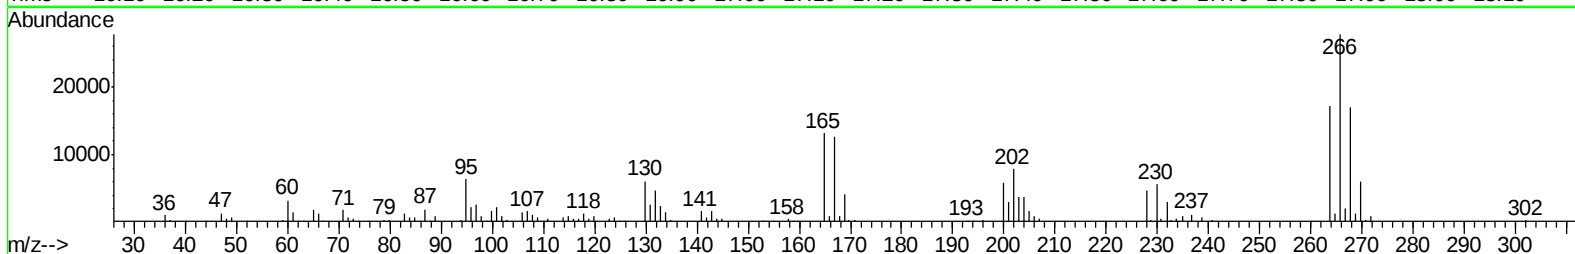


Data Path : Z:\HPCHEM1\BNA_G\Data\BG121115\
Data File : BG020087.D
Acq On : 10 Dec 2015 23:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:31:42 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

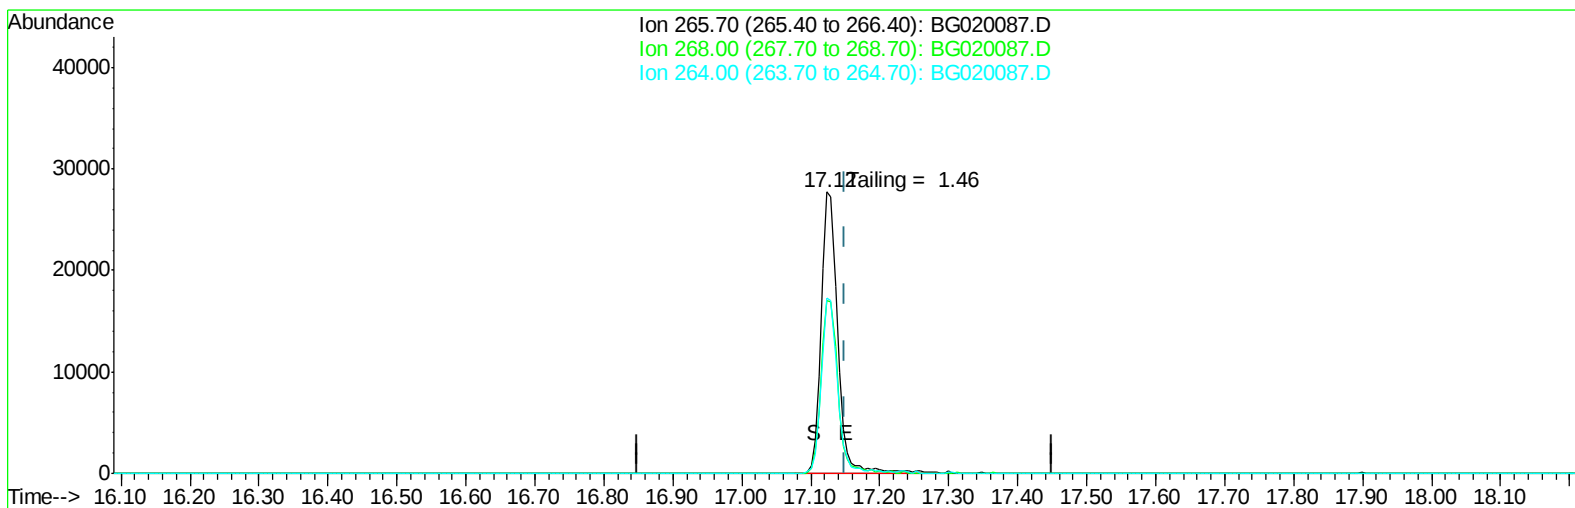

TIC: BG020087.D

(69) Pentachlorophenol (C)

17.124min (-0.026) 0.00ng

response 45372

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	61.29
264.00	60.10	67.00
0.00	0.00	0.00