
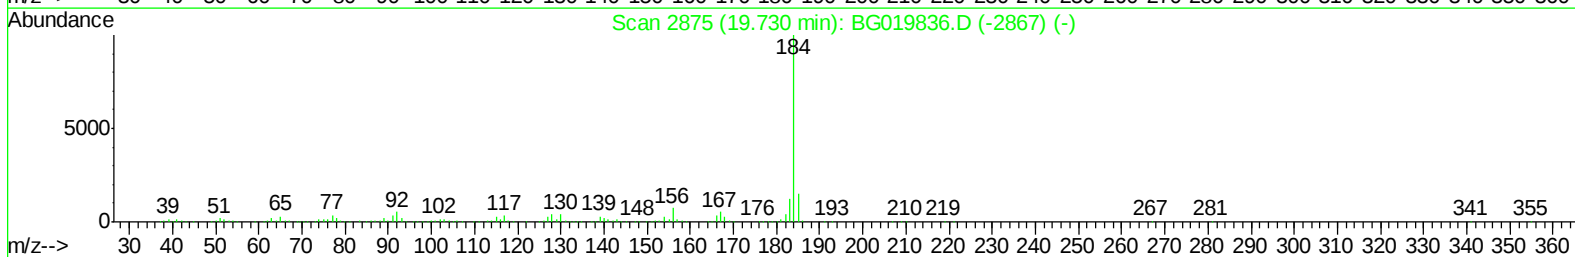
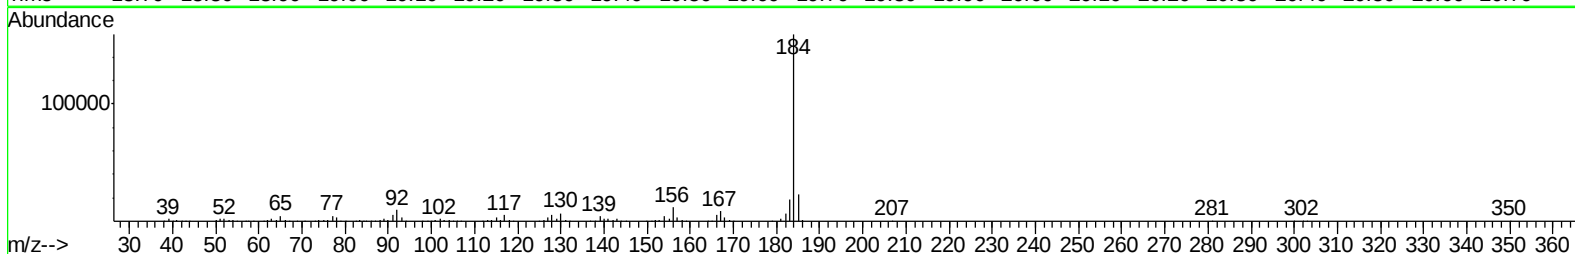


Data Path : Z:\HPCHEM1\BNA\_G\Data\BG121115\  
Data File : BG020087.D  
Acq On : 10 Dec 2015 23:14  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:31:42 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG120215.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 02 18:50:01 2015  
Response via : Initial Calibration

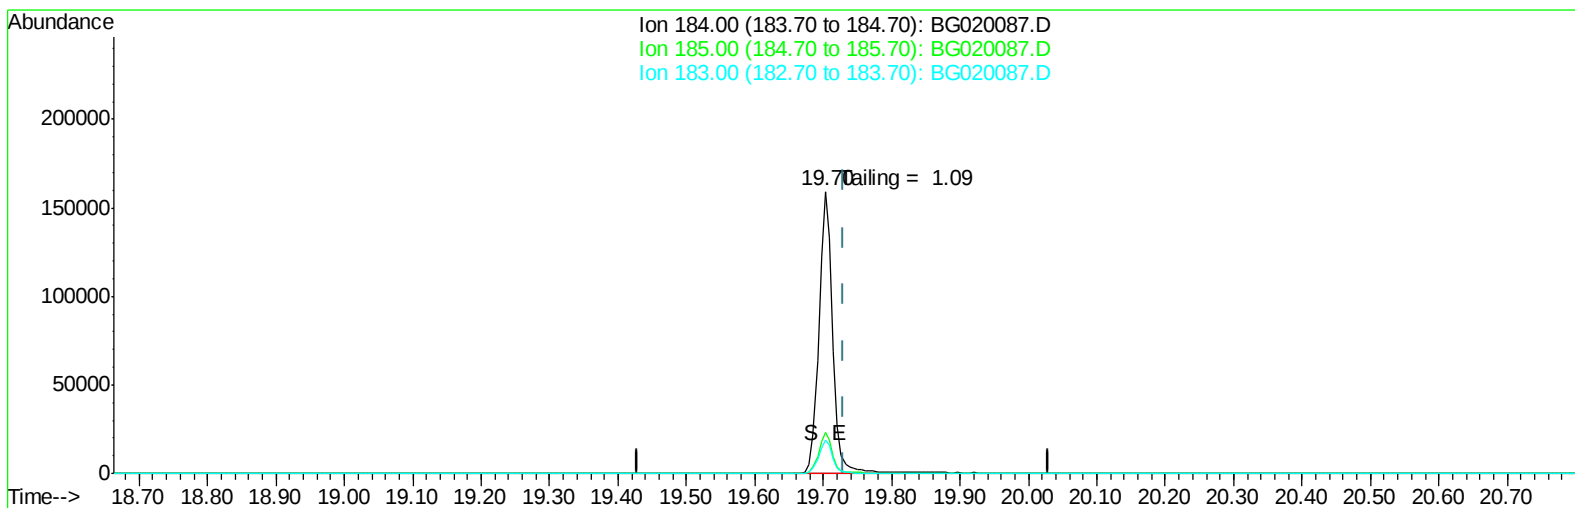

TIC: BG020087.D

(76) Benzidine

19.703min (-0.027) 0.00ng

response 223865

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.80 | 14.73 |
| 183.00 | 12.60 | 11.89 |
| 0.00   | 0.00  | 0.00  |