
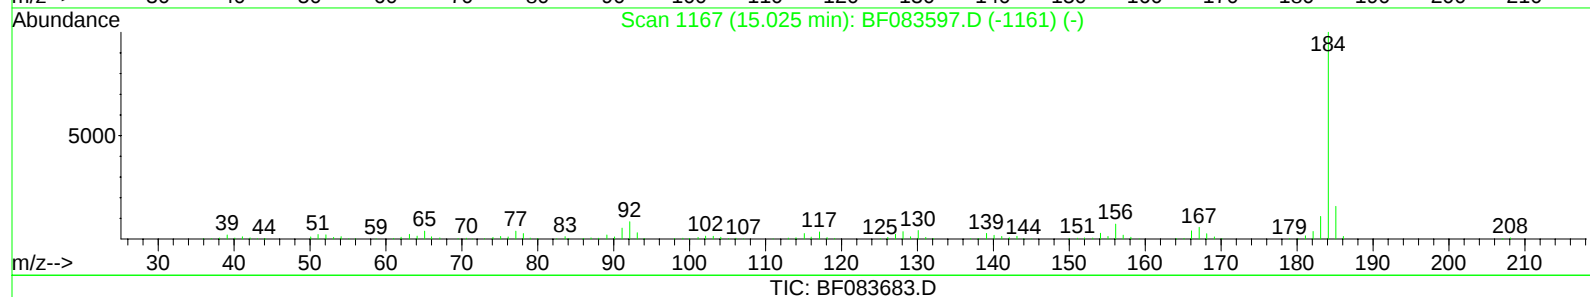
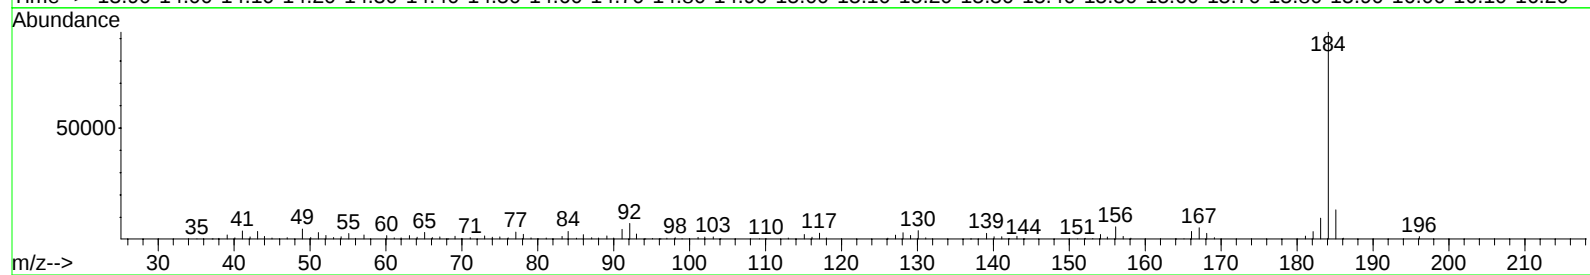


Data Path : Z:\HPCHEM1\BNA F\Data\BF121015\
Data File : BF083683.D
Acq On : 10 Dec 2015 16:56
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:27:57 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

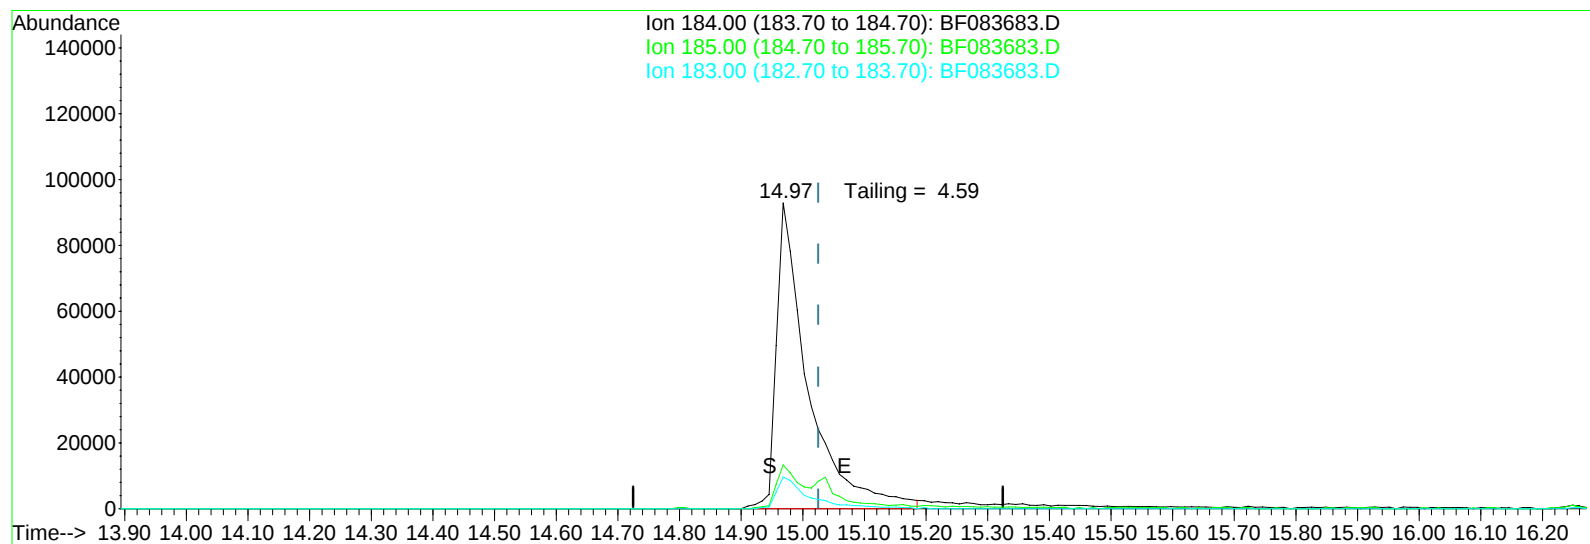

TIC: BF083683.D

(76) Benzidine




14.968min (-0.057) 2226.17ng

response 342136

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.36
183.00	11.20	10.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF121015\
Data File : BF083683.D
Acq On : 10 Dec 2015 16:56
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:27:57 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 00:23:35 2015
Response via : Initial Calibration

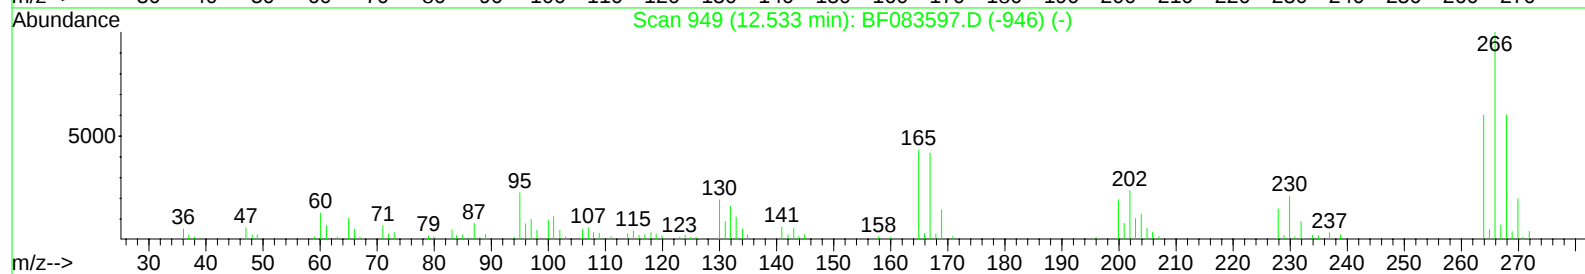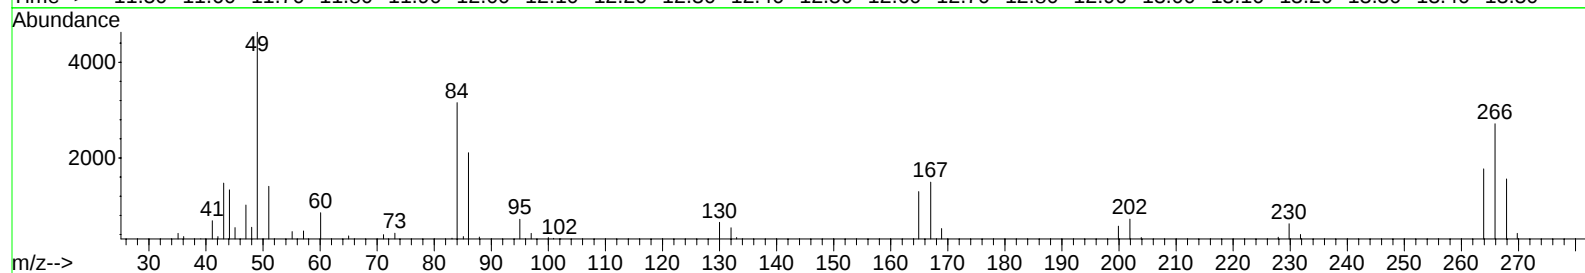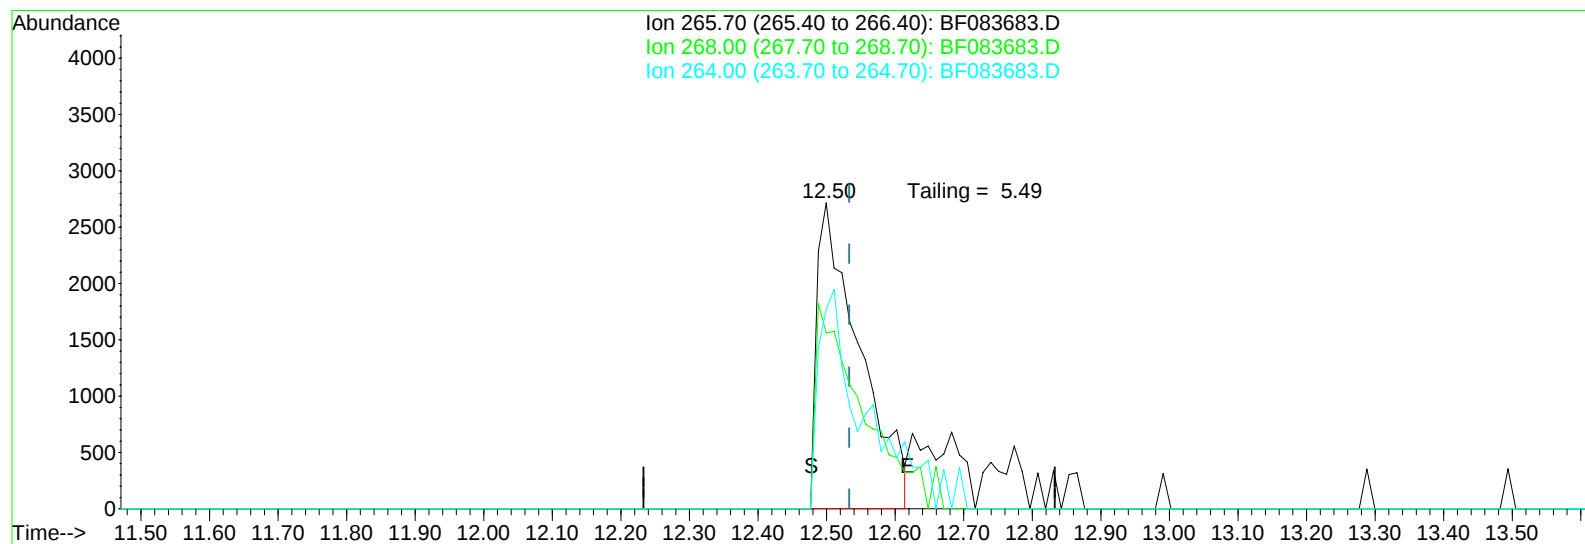

TIC: BF083683.D

(69) Pentachlorophenol (C)

12.499min (-0.034) 14604.71ng

response 11706

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	57.50
264.00	64.30	65.23
0.00	0.00	0.00