


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121015\
 Data File : BF083683.D
 Acq On : 10 Dec 2015 16:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 00:23:35 2015

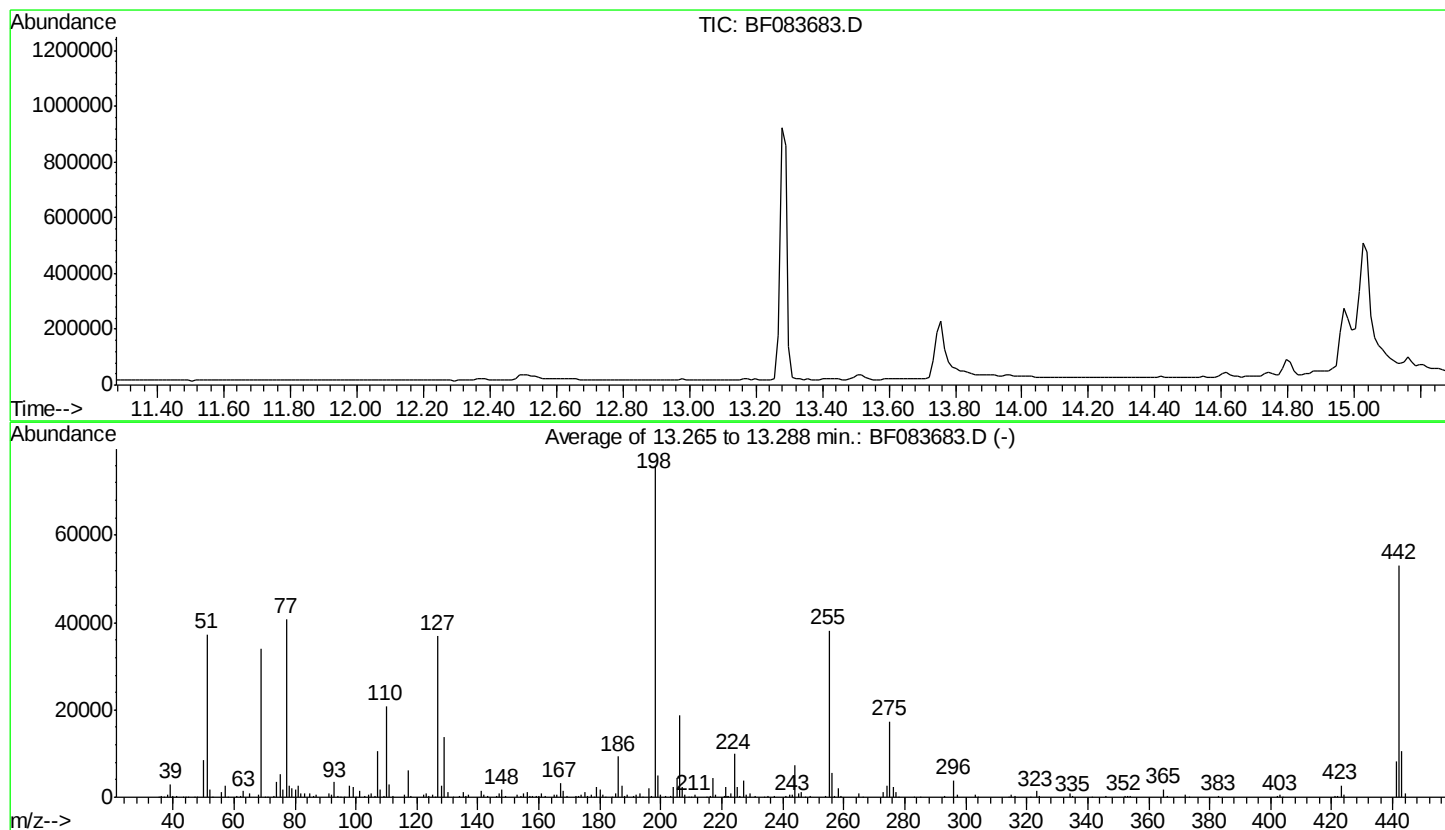

AutoFind: Scans 1013, 1014, 1015; Background Corrected with Scan 1009

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	37237	PASS
68	69	0.00	2	1.5	496	PASS
69	198	0.00	100	44.9	34084	PASS
70	69	0.00	2	0.4	134	PASS
127	198	10	80	48.8	37060	PASS
197	198	0.00	2	0.6	421	PASS
198	198	100	100	100.0	75952	PASS
199	198	5	9	6.7	5091	PASS
275	198	10	60	22.8	17340	PASS
365	198	1	100	2.4	1810	PASS
441	442	0.01	24	15.5	8248	PASS
442	198	50	100	69.9	53106	PASS
443	442	15	24	19.6	10420	PASS