
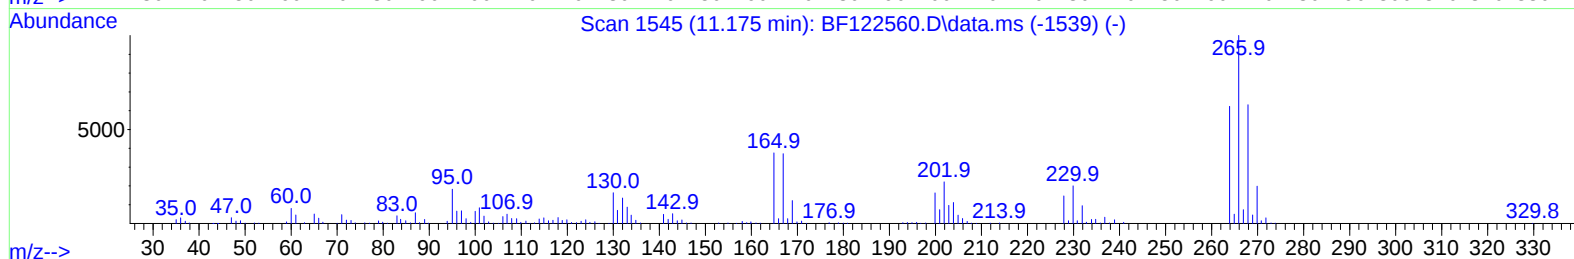
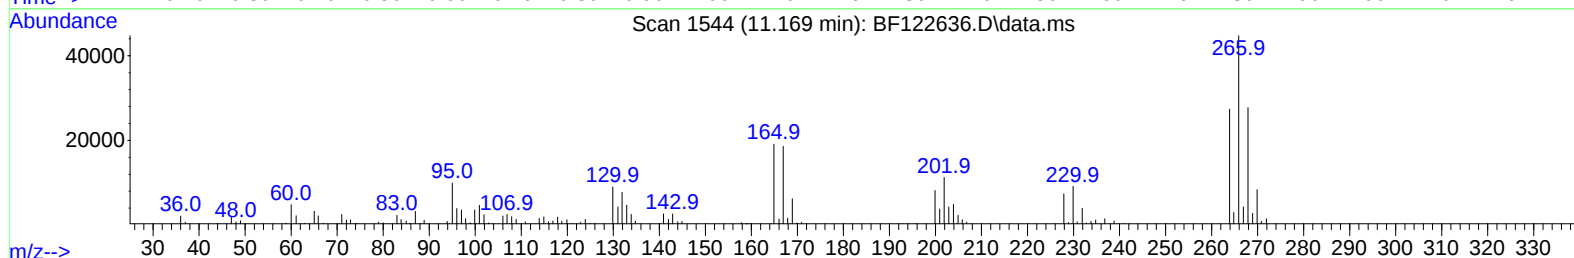


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121020\
Data File : BF122636.D
Acq On : 10 Dec 2020 8:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 04:07:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

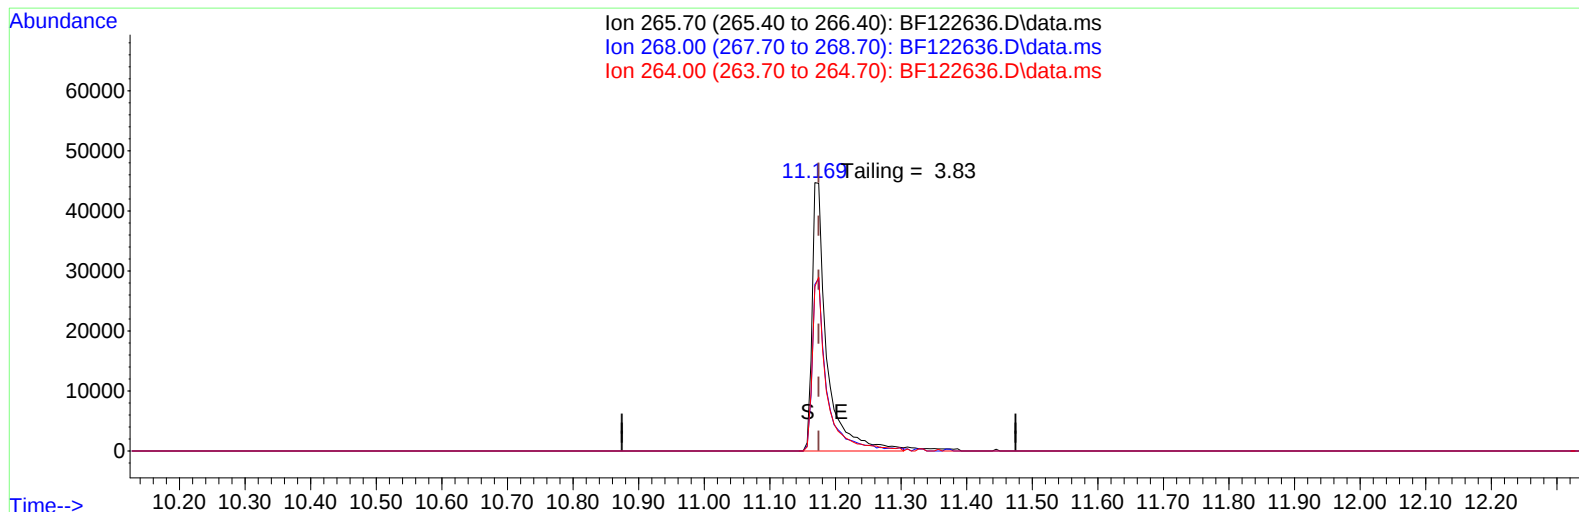

TIC: BF122636.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 30727.17 ng

response 70967

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.09
264.00	62.30	61.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121020\
Data File : BF122636.D
Acq On : 10 Dec 2020 8:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 04:07:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

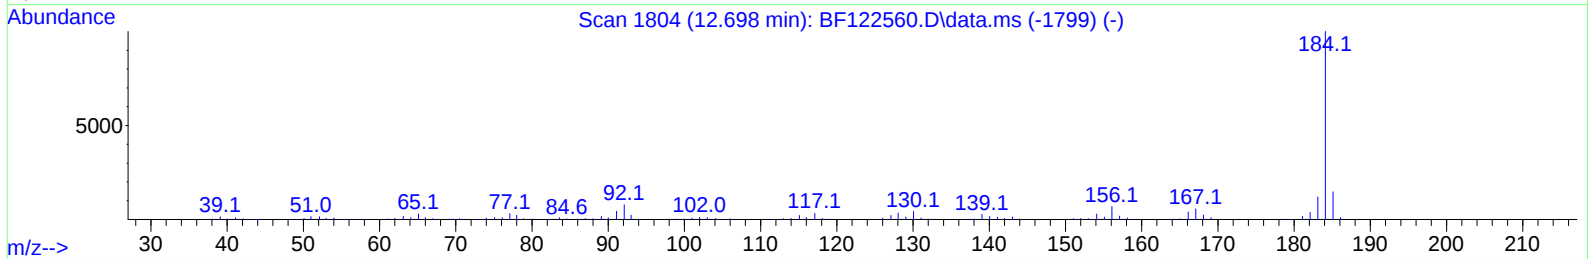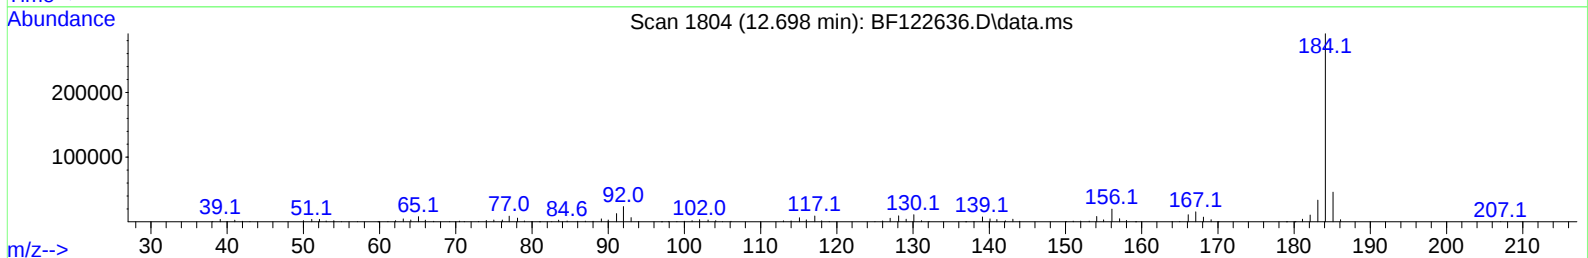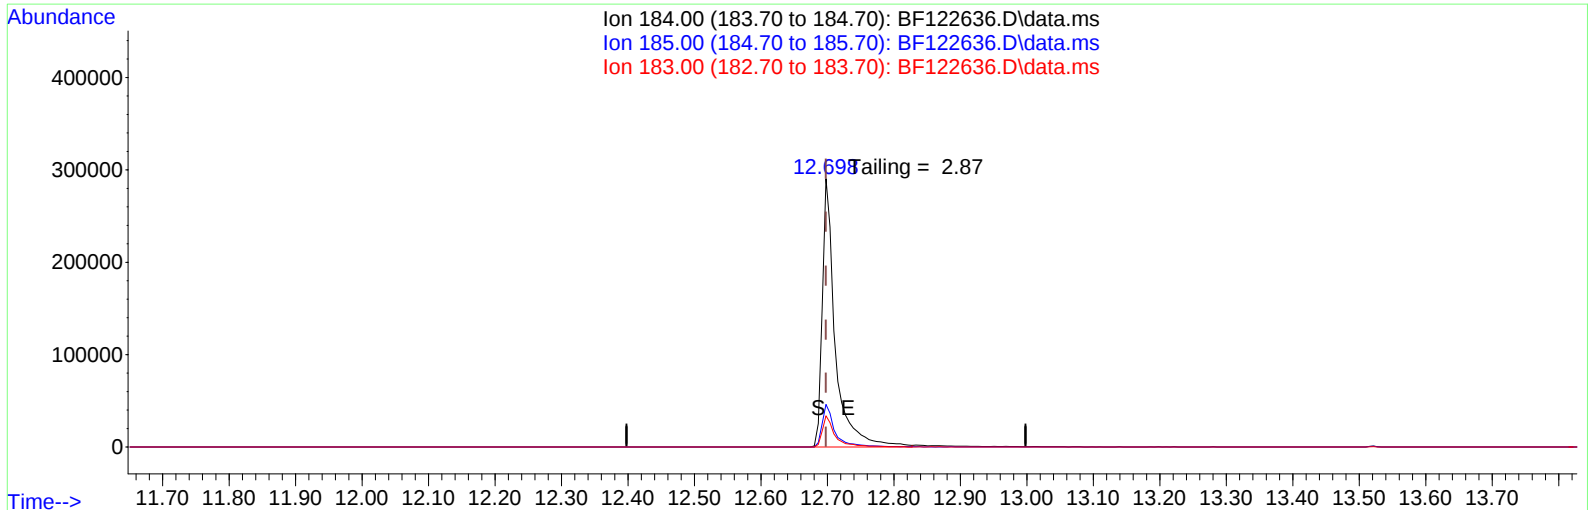

TIC: BF122636.D\data.ms

(77) Benzidine

12.698min (-0.000) 0.00 ng

response 396988

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.86
183.00	12.10	11.61
0.00	0.00	0.00