

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121020\
 Data File : BF122654.D
 Acq On : 10 Dec 2020 19:18
 Operator : JU/CG
 Sample : L4990-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MANHOLE

Manual Integrations
 APPROVED

mohammad
 12/11/2020 1:21:34 PM

Quant Time: Dec 11 00:36:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 12:08:49 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.839	152	162400	20.00	ng	0.00
21) Naphthalene-d8	8.122	136	632381	20.00	ng	0.00
39) Acenaphthene-d10	9.875	164	334227	20.00	ng	0.00
64) Phenanthrene-d10	11.363	188	594032	20.00	ng	0.00
76) Chrysene-d12	14.004	240	451029	20.00	ng	0.00
86) Perylene-d12	15.462	264	436643	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	677884	66.08	ng	0.00
7) Phenol-d6	6.469	99	1092665	80.32	ng	-0.01
23) Nitrobenzene-d5	7.398	82	715803	56.71	ng	-0.01
42) 2,4,6-Tribromophenol	10.663	330	79140	18.09	ng	-0.01
45) 2-Fluorobiphenyl	9.198	172	1386255	56.10	ng	0.00
79) Terphenyl-d14	12.951	244	1410134	54.73	ng	0.00
Target Compounds						Qvalue
10) Phenol	6.481	94	78327	5.56	ng	86
50) Dimethylphthalate	9.592	163	107262	4.02	ng	99
71) Phenanthrene	11.386	178	481088	13.63	ng	98
72) Anthracene	11.439	178	83763	2.39	ng	98
75) Fluoranthene	12.574	202	552236	14.92	ng	99
78) Pyrene	12.804	202	506362	14.52	ng	99
81) Benzo(a)anthracene	13.992	228	220147	7.30	ng	99
83) Chrysene	14.027	228	219958m	7.33	ng	
87) Indeno(1,2,3-cd)pyrene	16.909	276	101991	3.56	ng	96
88) Benzo(b)fluoranthene	15.039	252	226738m	7.40	ng	
89) Benzo(k)fluoranthene	15.062	252	63920m	2.28	ng	
90) Benzo(a)pyrene	15.398	252	163827	6.11	ng	98
92) Benzo(g,h,i)perylene	17.351	276	97718	4.30	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121020\
Data File : BF122654.D
Acq On : 10 Dec 2020 19:18
Operator : JU/CG
Sample : L4990-01
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
MANHOLE

Manual Integrations
APPROVED


mohammad
12/11/2020 1:21:34 PM

Quant Time: Dec 11 00:36:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration



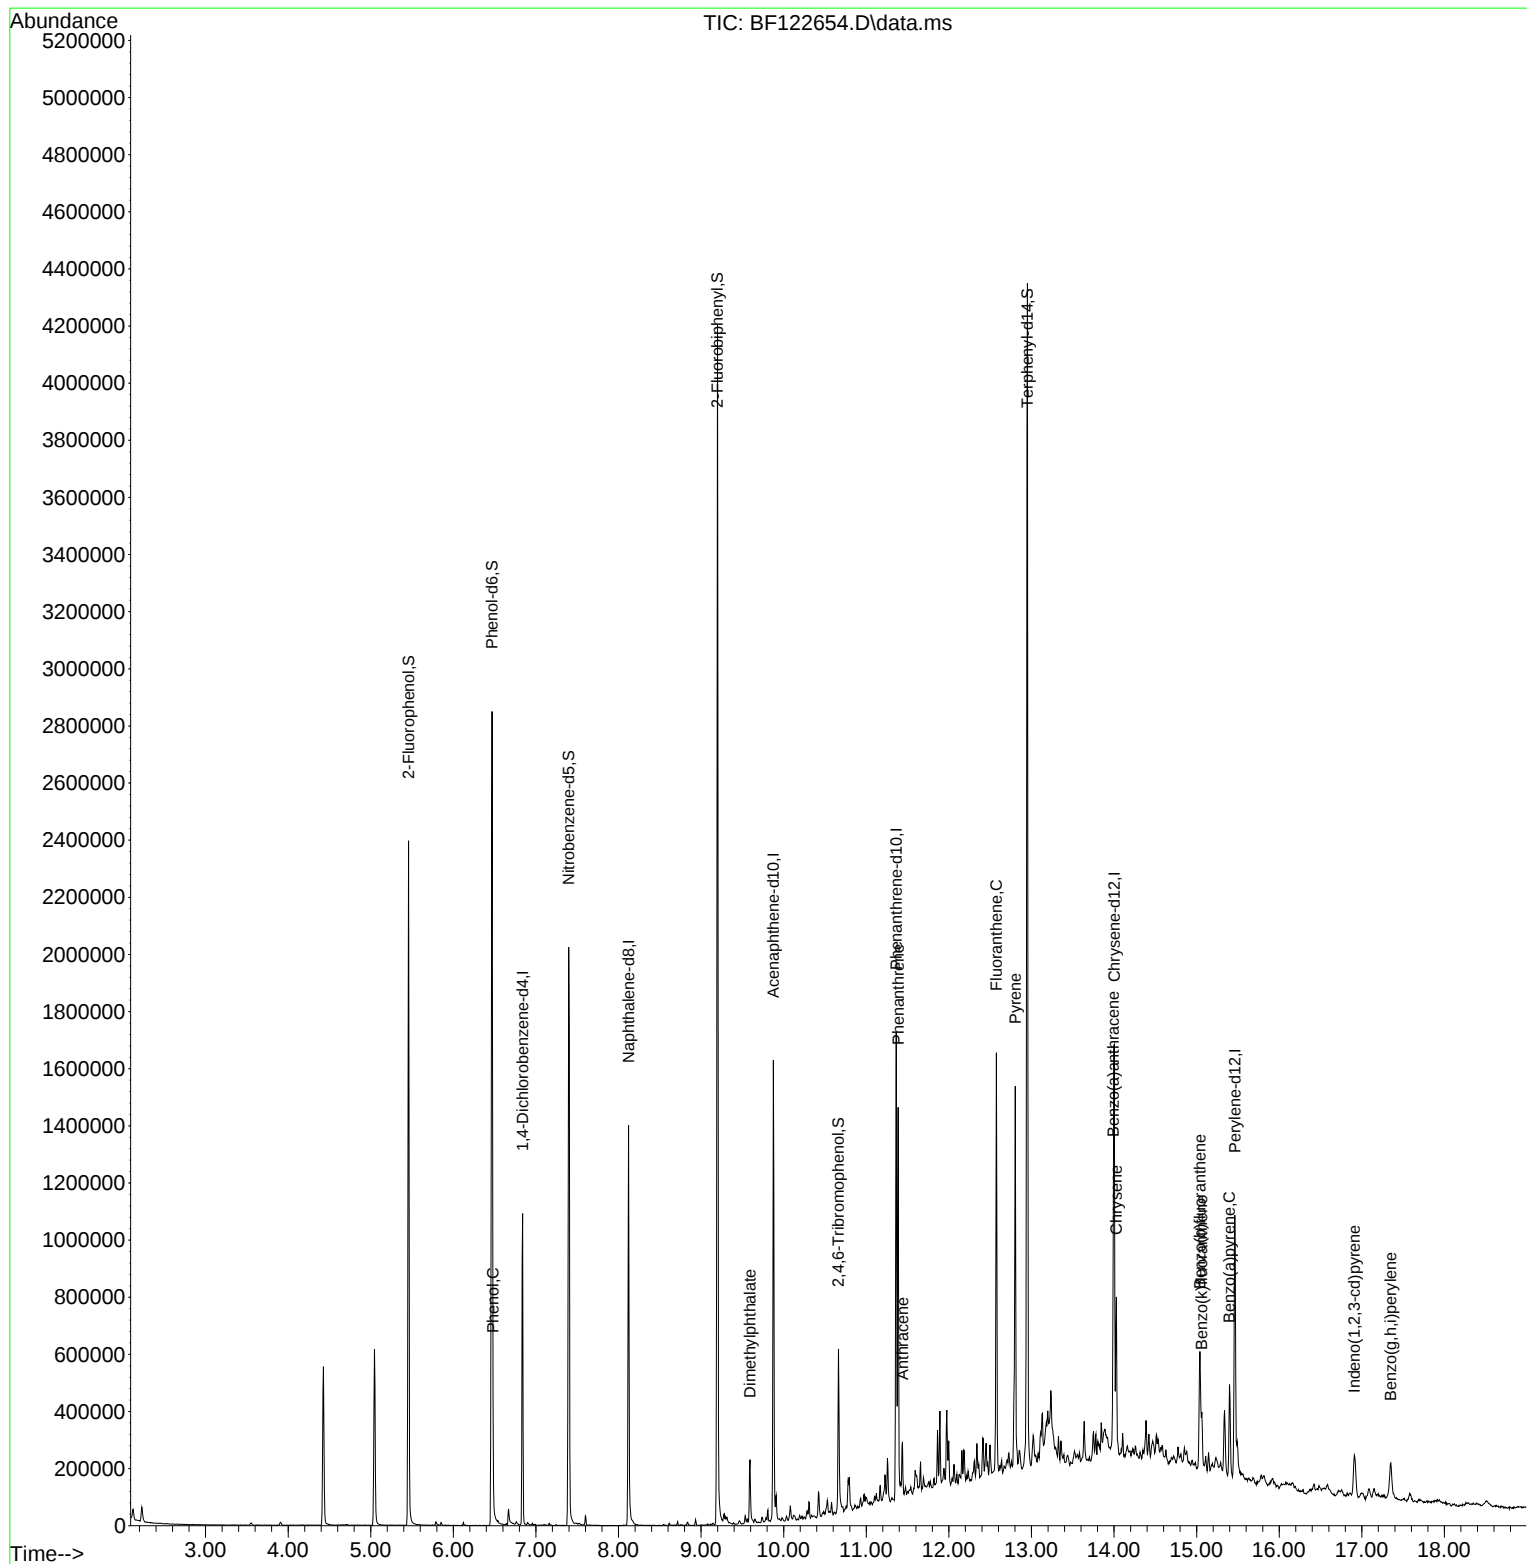


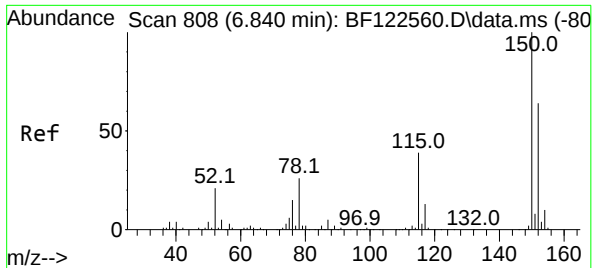


#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.839 min Scan# 808
Delta R.T. -0.001 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

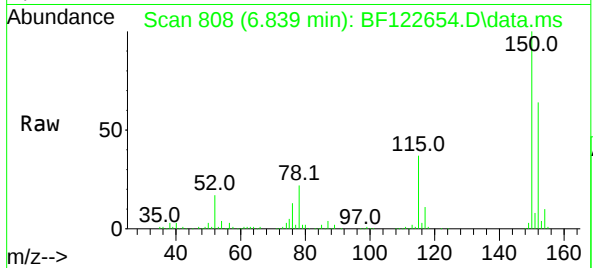



Tgt Ion:152 Resp: 162400
Ion Ratio Lower Upper
152 100
150 156.6 125.8 188.6
115 58.3 49.3 73.9

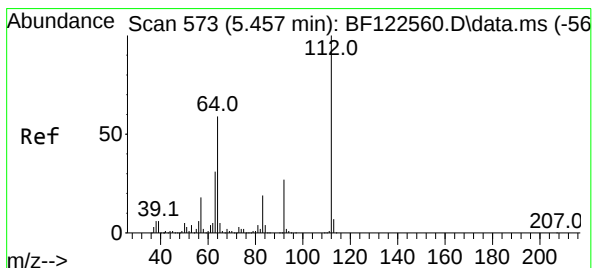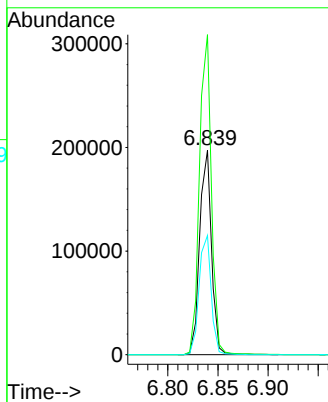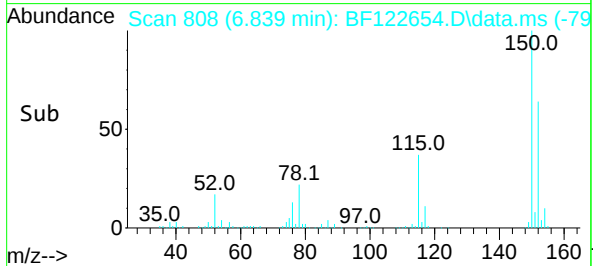

#5
2-Fluorophenol
Concen: 66.08 ng
RT: 5.457 min Scan# 573
Delta R.T. -0.000 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

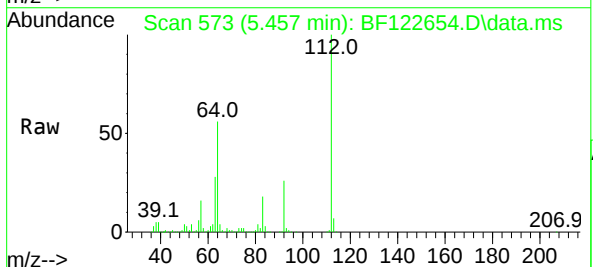

Tgt Ion:112 Resp: 677884
Ion Ratio Lower Upper
112 100
64 56.0 46.9 70.3
63 28.2 24.5 36.7

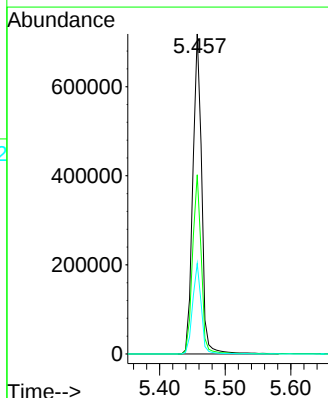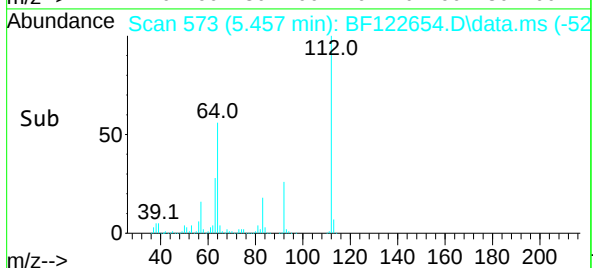


Instrument :
BNA_F
ClientSampleId :
MANHOLE

Manual Integrations
APPROVED

mohammad
12/11/2020 1:21:34 PM






#7
Phenol-d6
Concen: 80.32 ng
RT: 6.469 min Scan# 745
Delta R.T. -0.012 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18




Tgt Ion: 99 Resp: 1092665

Ion	Ratio	Lower	Upper
99	100		
42	16.9	13.8	20.6
71	34.4	26.9	40.3

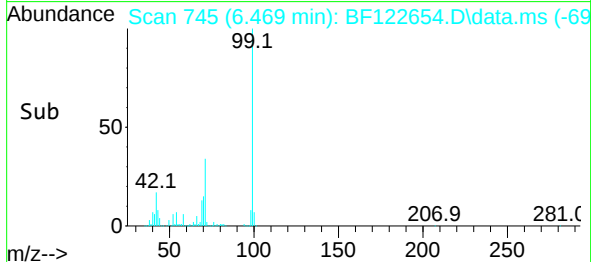
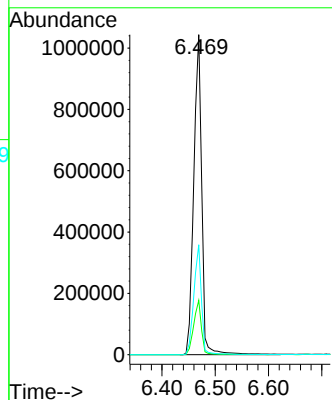


#10
Phenol
Concen: 5.56 ng
RT: 6.481 min Scan# 747
Delta R.T. -0.012 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

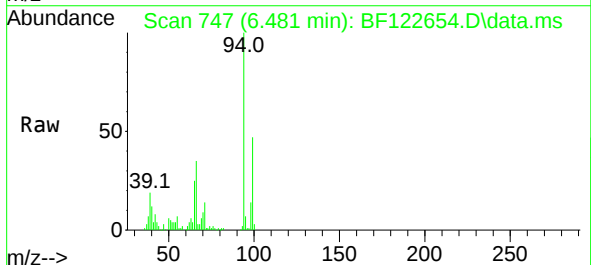

Tgt Ion: 94 Resp: 78327

Ion	Ratio	Lower	Upper
94	100		
65	24.7	11.2	51.2
66	35.3	25.8	65.8

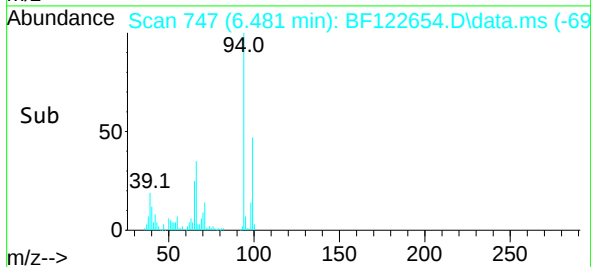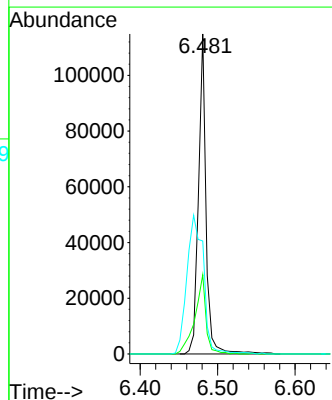

Instrument :
BNA_F
ClientSampleId :
MANHOLE


Manual Integrations
APPROVED

mohammad
12/11/2020 1:21:34 PM



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18




Instrument :
BNA_F
ClientSampleId :
MANHOLE

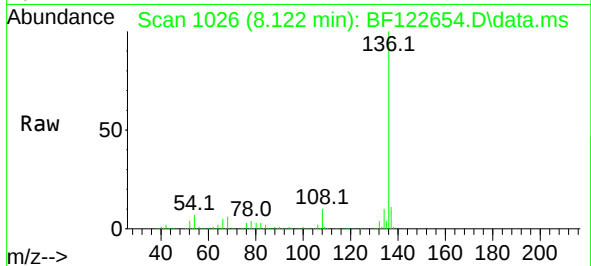


Tgt Ion:136 Resp: 632381
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 7.3 5.5 8.3
68 6.0 4.6 6.8

Manual Integrations
APPROVED



mohammad
12/11/2020 1:21:34 PM

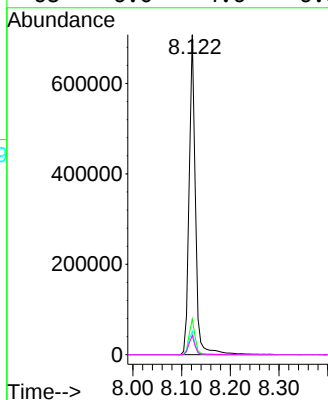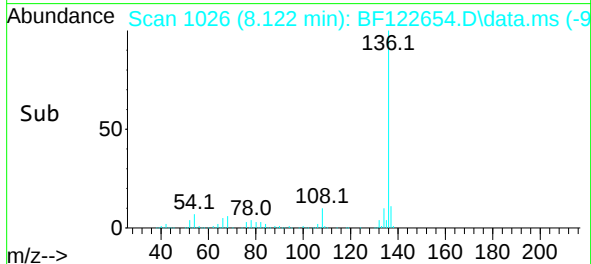


#23
Nitrobenzene-d5
Concen: 56.71 ng
RT: 7.398 min Scan# 903
Delta R.T. -0.012 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

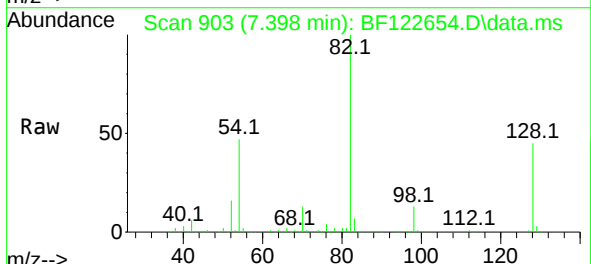


Tgt Ion: 82 Resp: 715803
Ion Ratio Lower Upper
82 100
128 44.6 37.0 55.4
54 47.5 38.4 57.6

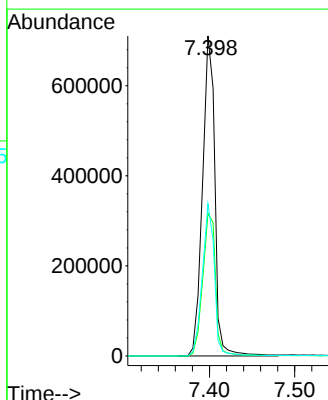



#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.875 min Scan# 1324
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18




Instrument :
BNA_F
ClientSampleId :
MANHOLE




Tgt Ion:164 Resp: 334227
Ion Ratio Lower Upper
164 100
162 102.2 80.8 121.2
160 44.3 35.4 53.0

Manual Integrations
APPROVED



mohammad
12/11/2020 1:21:34 PM

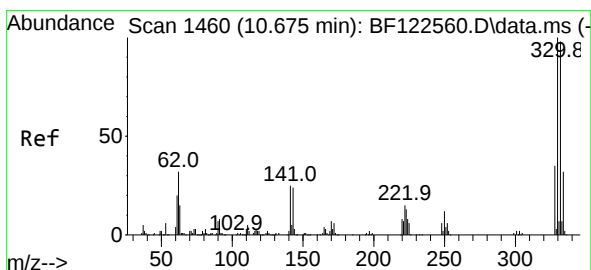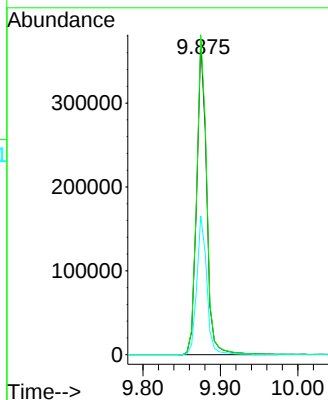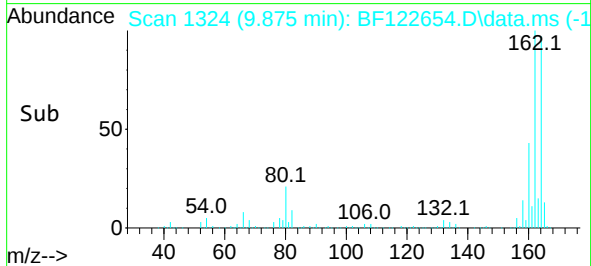


#42
2,4,6-Tribromophenol
Concen: 18.09 ng
RT: 10.663 min Scan# 1458
Delta R.T. -0.012 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

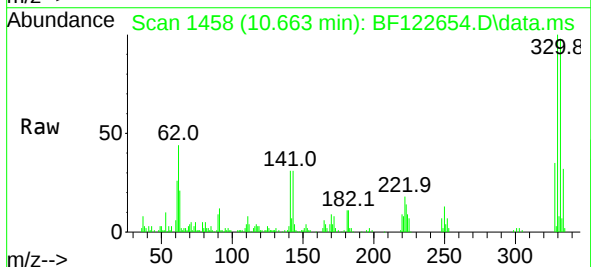

Tgt Ion:330 Resp: 79140
Ion Ratio Lower Upper
330 100
332 98.2 77.5 116.3
141 31.3 23.8 35.8

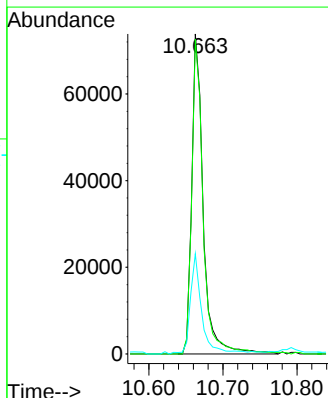







#45
2-Fluorobiphenyl
Concen: 56.10 ng
RT: 9.198 min Scan# 1209
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Instrument :
BNA_F
ClientSampleId :
MANHOLE

Tgt Ion:172 Resp: 1386255
Ion Ratio Lower Upper
172 100
171 36.0 29.6 44.4
170 23.5 19.5 29.3




Manual Integrations
APPROVED


mohammad
12/11/2020 1:21:34 PM

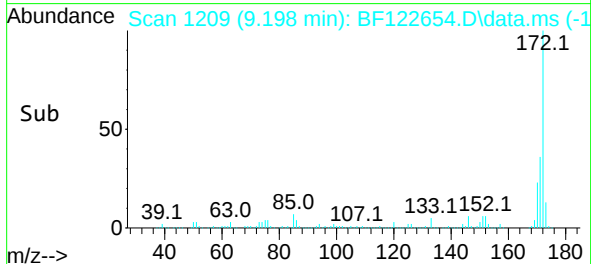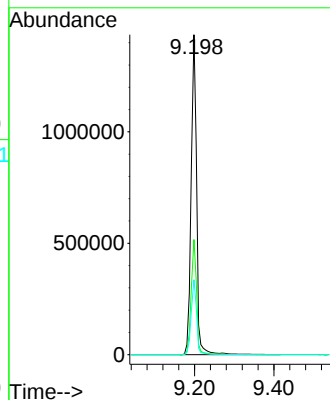


#50
Dimethylphthalate
Concen: 4.02 ng
RT: 9.592 min Scan# 1276
Delta R.T. -0.018 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Tgt Ion:163 Resp: 107262
Ion Ratio Lower Upper
163 100
194 3.9 3.4 5.0
164 9.6 8.1 12.1

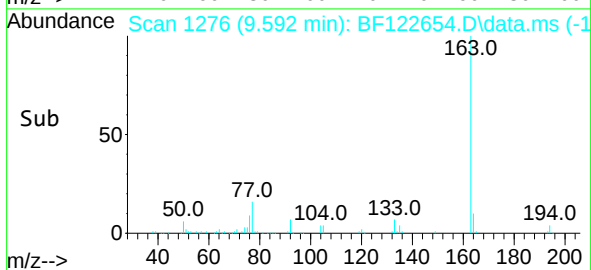
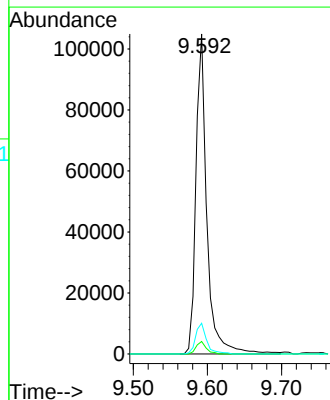
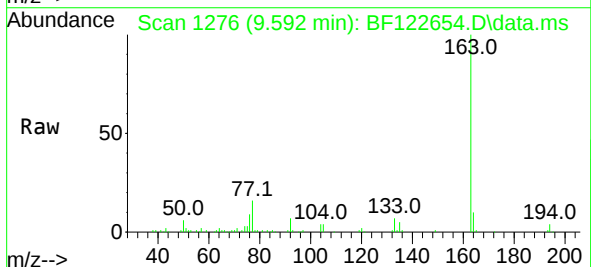


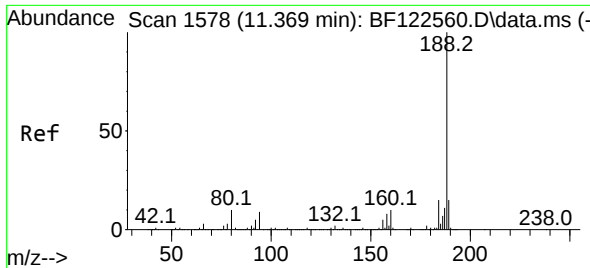


#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.363 min Scan# 1577
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

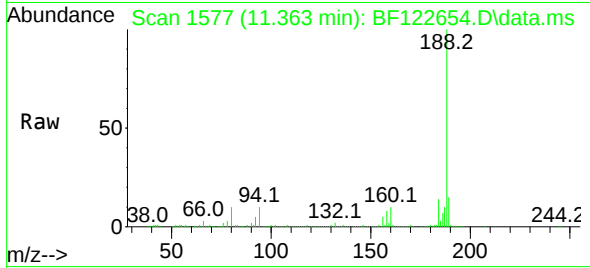



Tgt Ion:188 Resp: 594032
Ion Ratio Lower Upper
188 100
94 9.8 7.4 11.2
80 10.0 8.2 12.4

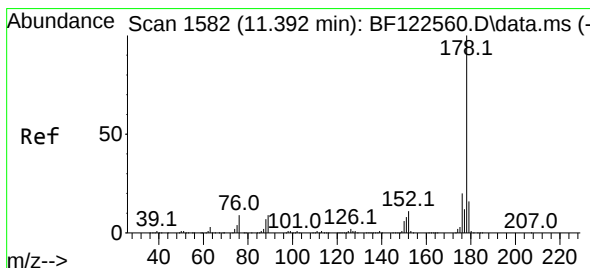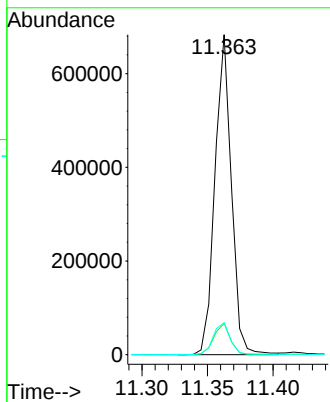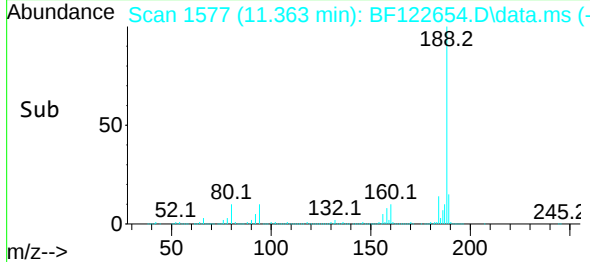

#71
Phenanthrene
Concen: 13.63 ng
RT: 11.386 min Scan# 1581
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

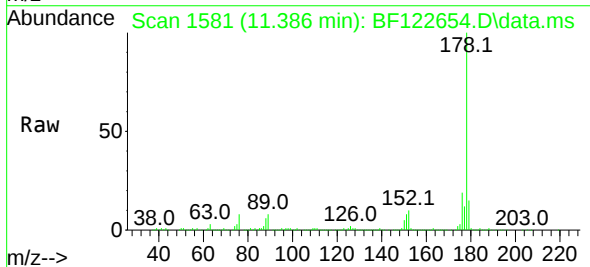


Tgt Ion:178 Resp: 481088
Ion Ratio Lower Upper
178 100
176 19.3 16.2 24.2
179 15.4 12.7 19.1

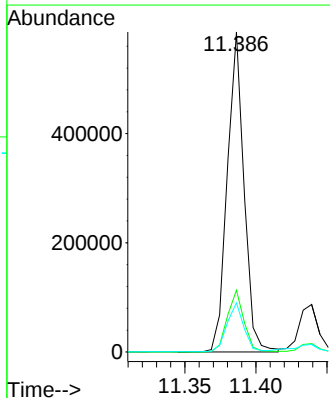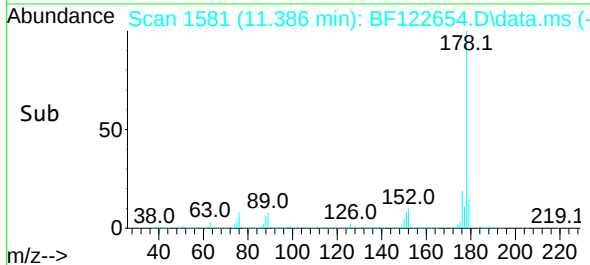

Instrument :
BNA_F
ClientSampleId :
MANHOLE

Manual Integrations
APPROVED

mohammad
12/11/2020 1:21:34 PM

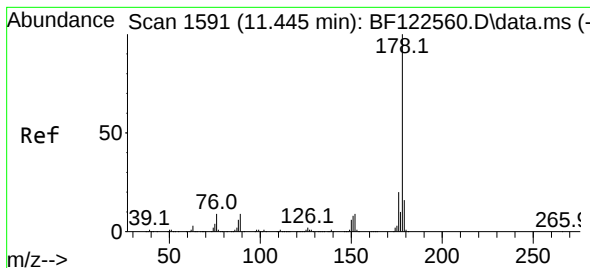

#72

Anthracene

Concen: 2.39 ng

RT: 11.439 min Scan# 1590

Delta R.T. -0.006 min

Lab File: BF122654.D

Acq: 10 Dec 2020 19:18

Tgt Ion:	178	Resp:	83763
Ion Ratio	Lower	Upper	
178	100		
176	17.6	15.6	23.4
179	15.8	12.8	19.2

Instrument :





BNA_F

ClientSampleId :

MANHOLE

Manual Integrations
APPROVED

mohammad
12/11/2020 1:21:34 PM

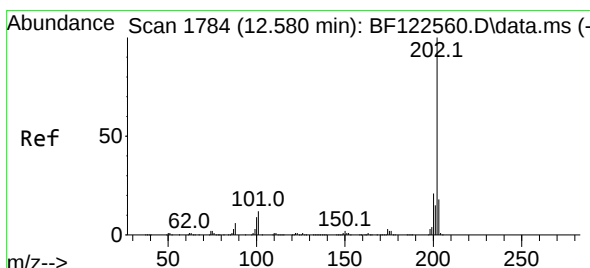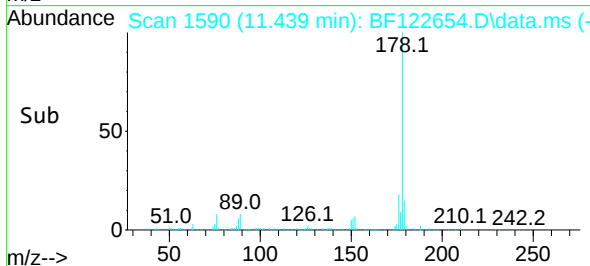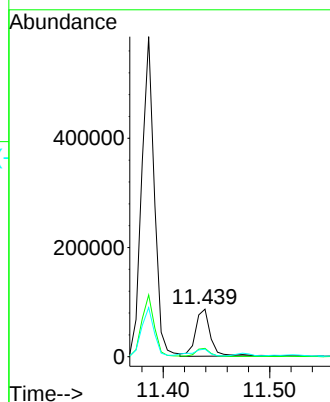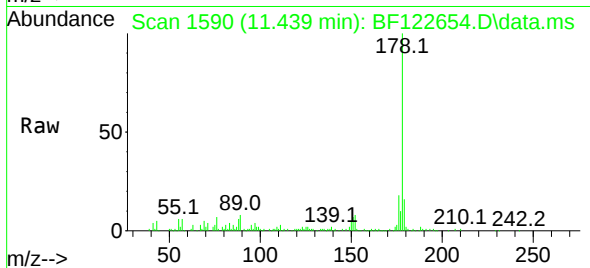

#75

Fluoranthene

Concen: 14.92 ng




RT: 12.574 min Scan# 1783


Delta R.T. -0.006 min

Lab File: BF122654.D


Acq: 10 Dec 2020 19:18

Tgt Ion:	202	Resp:	552236
Ion Ratio	Lower	Upper	
202	100		
101	11.7	0.0	32.2
203	18.3	0.0	38.1

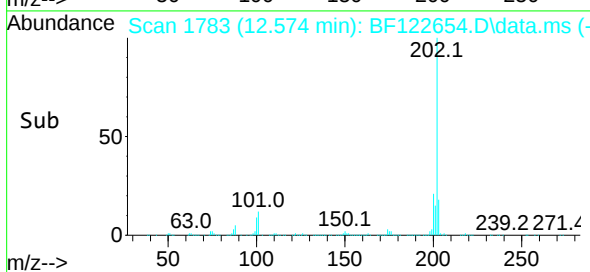
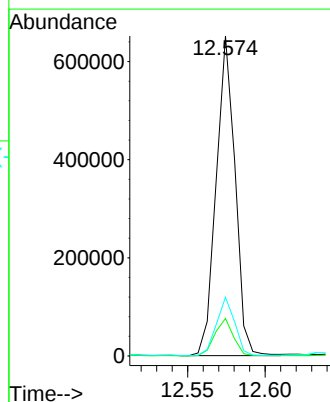
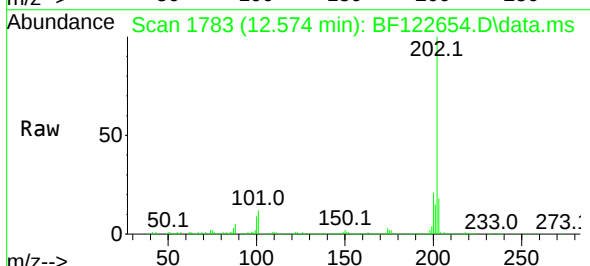





#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.004 min Scan# 2026
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

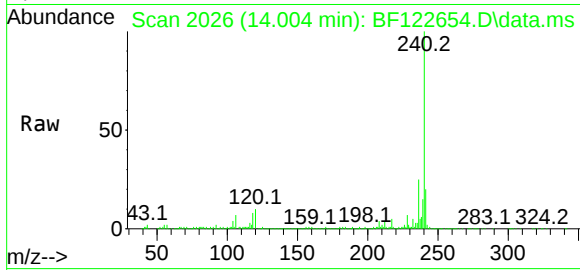



Tgt Ion:240 Resp: 451029
Ion Ratio Lower Upper
240 100
120 10.0 8.6 12.8
236 25.4 20.3 30.5

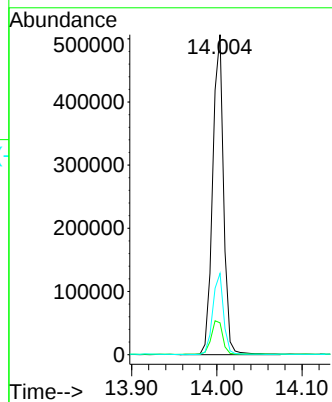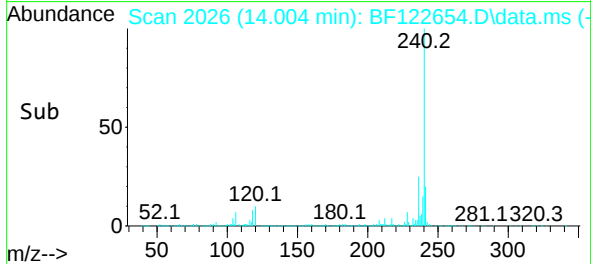

#78
Pyrene
Concen: 14.52 ng
RT: 12.804 min Scan# 1822
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

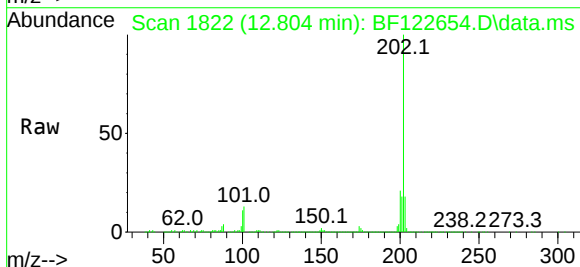


Tgt Ion:202 Resp: 506362
Ion Ratio Lower Upper
202 100
200 21.0 17.6 26.4
203 18.0 14.6 21.8

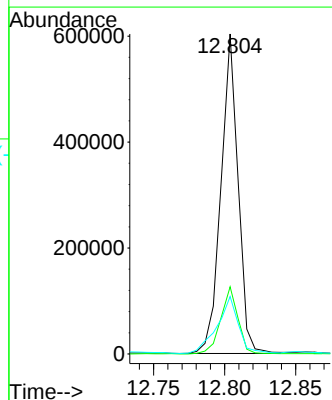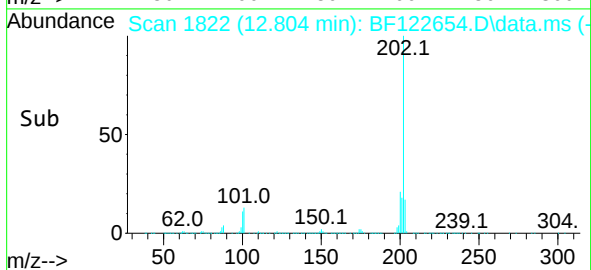

Instrument :
BNA_F
ClientSampleId :
MANHOLE


Manual Integrations
APPROVED

mohammad
12/11/2020 1:21:34 PM

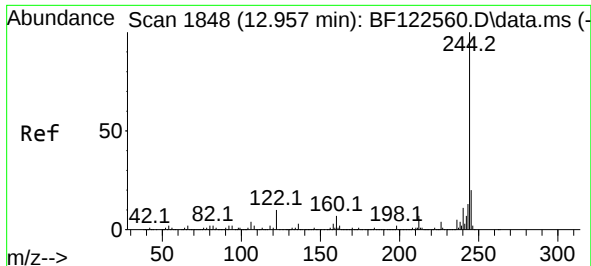

#79
Terphenyl-d14
Concen: 54.73 ng
RT: 12.951 min Scan# 1847
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18




Instrument :
BNA_F
ClientSampleId :
MANHOLE




Tgt Ion:244 Resp: 1410134
Ion Ratio Lower Upper
244 100
212 7.1 5.7 8.5
122 10.3 8.3 12.5

Manual Integrations
APPROVED



mohammad
12/11/2020 1:21:34 PM

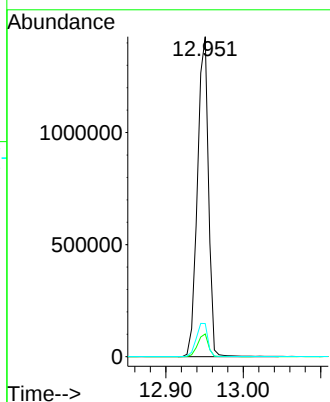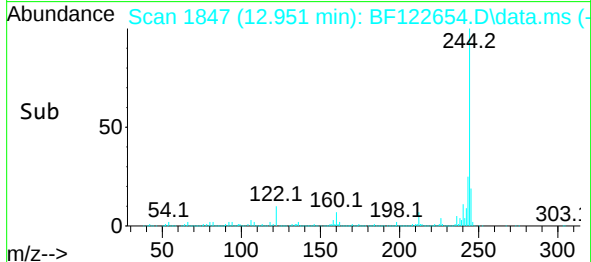


#81
Benzo(a)anthracene
Concen: 7.30 ng
RT: 13.992 min Scan# 2024
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

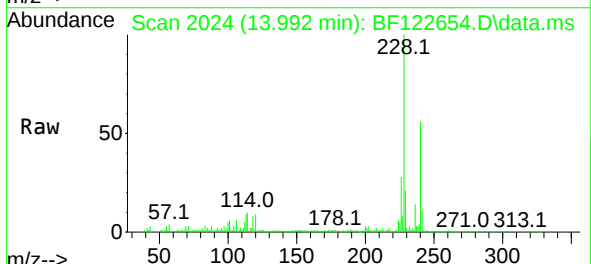

Tgt Ion:228 Resp: 220147
Ion Ratio Lower Upper
228 100
226 28.0 23.0 34.4
229 20.9 16.6 24.8

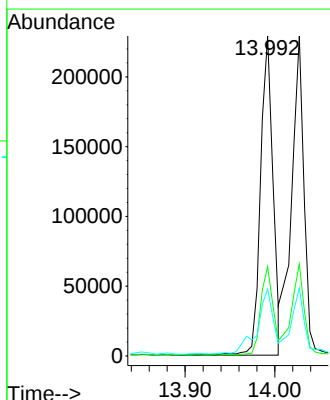

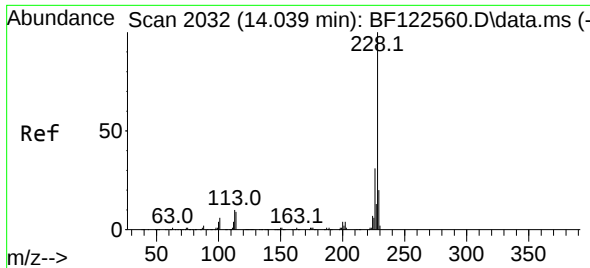





#83
Chrysene
Concen: 7.33 ng m
RT: 14.027 min Scan# 2030
Delta R.T. -0.012 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Tgt Ion:228 Resp: 219958
Ion Ratio Lower Upper
228 100
226 28.8 24.6 36.8
229 21.3 15.8 23.6

Instrument :
BNA_F
ClientSampleId :
MANHOLE




Manual Integrations
APPROVED


mohammad
12/11/2020 1:21:34 PM

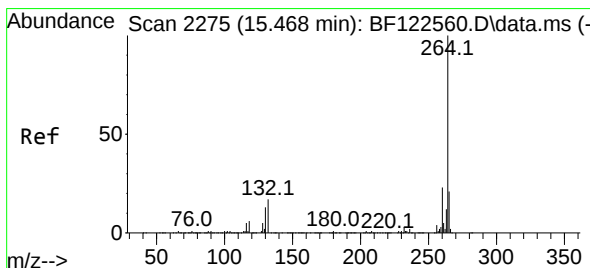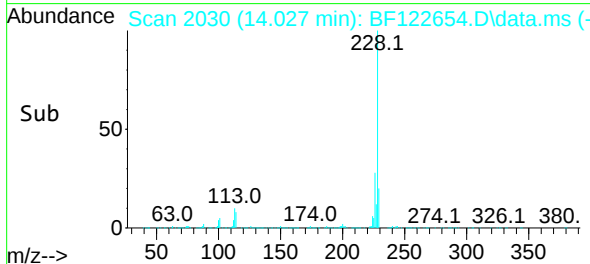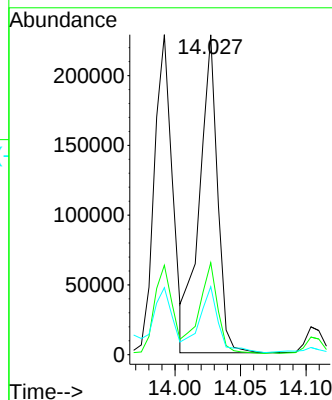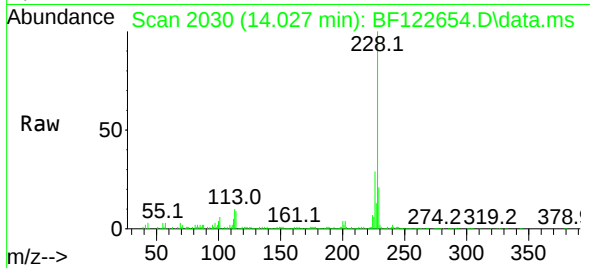

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.462 min Scan# 2274
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Tgt Ion:264 Resp: 436643
Ion Ratio Lower Upper
264 100
260 23.7 18.6 28.0
265 22.4 17.0 25.6

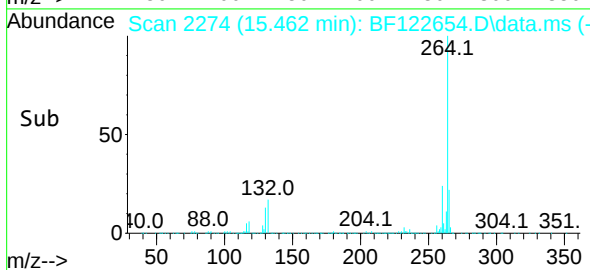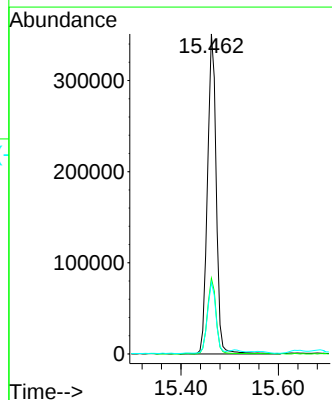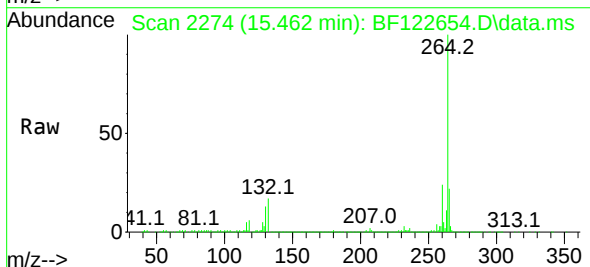







#87
Indeno(1,2,3-cd)pyrene
Concen: 3.56 ng
RT: 16.909 min Scan# 2520
Delta R.T. -0.024 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Tgt Ion: 276 Resp: 101991
Ion Ratio Lower Upper
276 100
138 20.5 18.7 28.1
277 24.3 20.2 30.4

Instrument :
BNA_F
ClientSampleId :
MANHOLE




Manual Integrations
APPROVED


mohammad
12/11/2020 1:21:34 PM

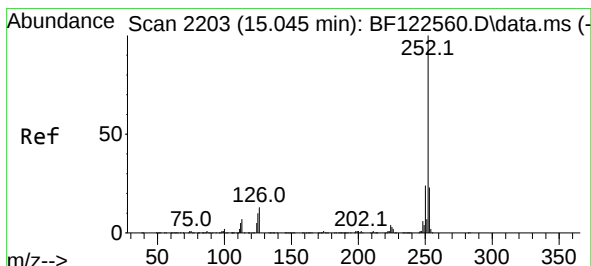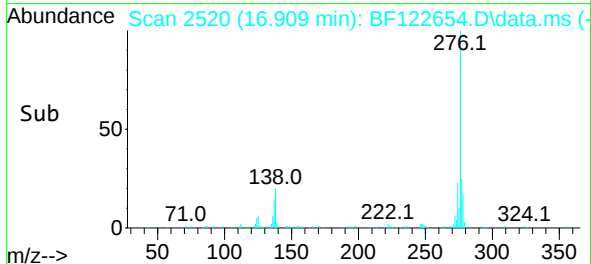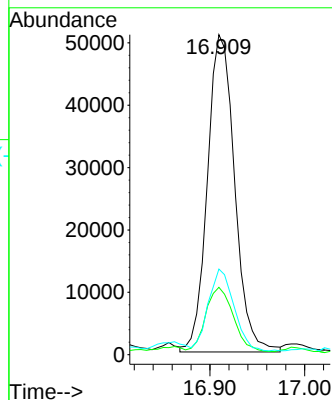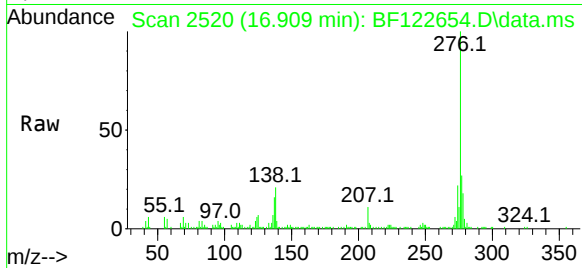

#88
Benzo(b)fluoranthene
Concen: 7.40 ng m
RT: 15.039 min Scan# 2202
Delta R.T. -0.006 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Tgt Ion: 252 Resp: 226738
Ion Ratio Lower Upper
252 100
253 21.6 18.3 27.5
125 10.7 8.1 12.1

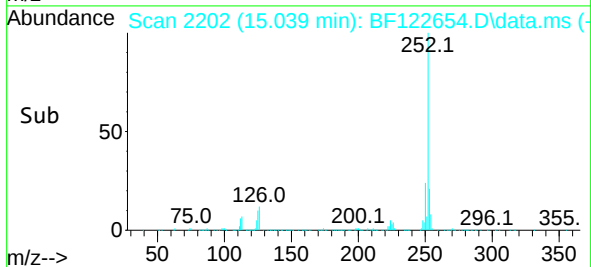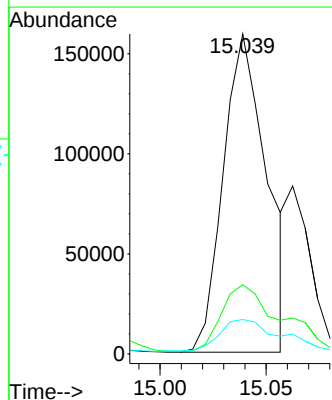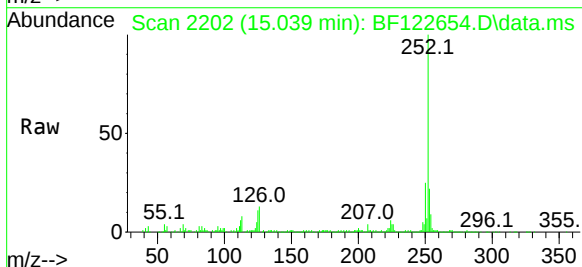







#89
Benzo(k)fluoranthene
Concen: 2.28 ng m
RT: 15.062 min Scan# 2206
Delta R.T. -0.012 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Tgt Ion:252 Resp: 63920
Ion Ratio Lower Upper
252 100
253 21.4 17.8 26.8
125 11.8 8.4 12.6

Instrument :
BNA_F
ClientSampleId :
MANHOLE




Manual Integrations
APPROVED


mohammad
12/11/2020 1:21:34 PM

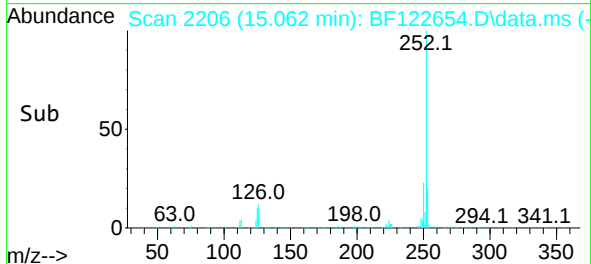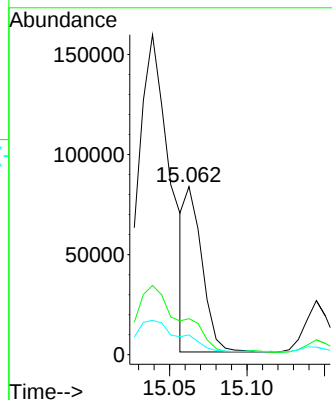

#90
Benzo(a)pyrene
Concen: 6.11 ng
RT: 15.398 min Scan# 2263
Delta R.T. -0.012 min
Lab File: BF122654.D
Acq: 10 Dec 2020 19:18

Tgt Ion:252 Resp: 163827
Ion Ratio Lower Upper
252 100
253 22.3 17.5 26.3
125 12.0 8.6 12.8

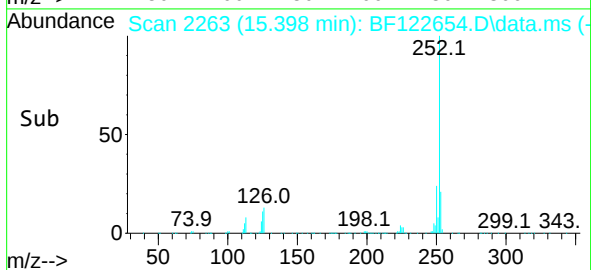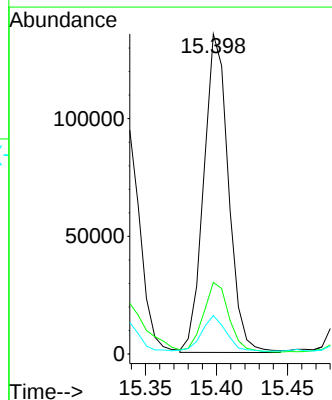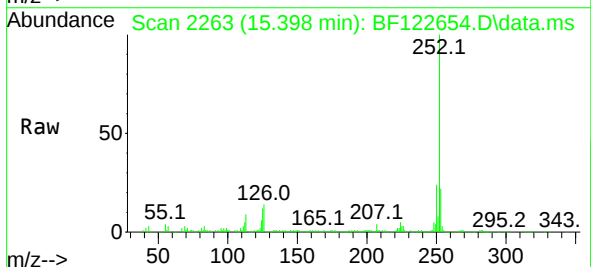

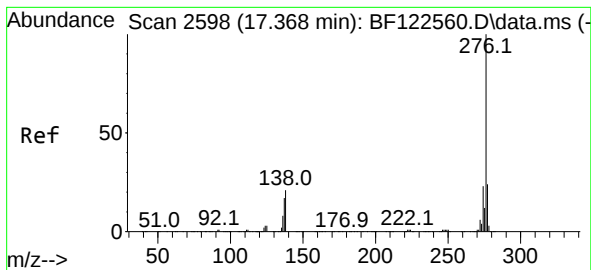

#92
 Benzo(g,h,i)perylene
 Concen: 4.30 ng
 RT: 17.351 min Scan# 2595
 Delta R.T. -0.018 min
 Lab File: BF122654.D
 Acq: 10 Dec 2020 19:18

Tgt Ion:	276	Resp:	97718
Ion Ratio	Lower	Upper	
276	100		
277	23.5	19.3	28.9
138	20.8	16.6	24.8

Instrument :
 BNA_F
 ClientSampleId :
 MANHOLE

Manual Integrations
 APPROVED

mohammad
 12/11/2020 1:21:34 PM

