

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF121020\  
 Data File : BF122638.D  
 Acq On : 10 Dec 2020 9:44  
 Operator : JU/CG  
 Sample : PB133474BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB133474BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122638.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.469       | 570           | 575         | 578          | rBV      | 4201790        | 4307116       | 64.54%          | 11.396%       |
| 2         | 6.475       | 740           | 746         | 749          | rBV      | 3873038        | 4306243       | 64.53%          | 11.393%       |
| 3         | 6.839       | 804           | 808         | 811          | rBV      | 1342523        | 1059862       | 15.88%          | 2.804%        |
| 4         | 7.404       | 898           | 904         | 907          | rBV      | 2794141        | 2902864       | 43.50%          | 7.680%        |
| 5         | 8.122       | 1021          | 1026        | 1040         | rBV      | 1562320        | 1463546       | 21.93%          | 3.872%        |
| 6         | 9.198       | 1203          | 1209        | 1213         | rBV      | 4975101        | 5560065       | 83.32%          | 14.711%       |
| 7         | 9.875       | 1319          | 1324        | 1339         | rBV      | 1787893        | 1812524       | 27.16%          | 4.795%        |
| 8         | 10.669      | 1454          | 1459        | 1484         | rBV      | 3715875        | 3981180       | 59.66%          | 10.533%       |
| 9         | 11.363      | 1573          | 1577        | 1585         | rBV      | 2106497        | 1921928       | 28.80%          | 5.085%        |
| 10        | 12.957      | 1842          | 1848        | 1851         | rBV      | 6135770        | 6673520       | 100.00%         | 17.656%       |
| 11        | 14.004      | 2021          | 2026        | 2041         | rVB      | 1977023        | 1876531       | 28.12%          | 4.965%        |
| 12        | 14.374      | 2076          | 2089        | 2092         | rBV7     | 27948          | 83560         | 1.25%           | 0.221%        |
| 13        | 14.604      | 2119          | 2128        | 2143         | rBV3     | 52075          | 185873        | 2.79%           | 0.492%        |
| 14        | 15.468      | 2269          | 2275        | 2292         | rVB      | 1129076        | 1661665       | 24.90%          | 4.396%        |




Sum of corrected areas: 37796477

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF121020\  
Data File : BF122638.D  
Acq On : 10 Dec 2020 9:44  
Operator : JU/CG  
Sample : PB133474BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB133474BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF120520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

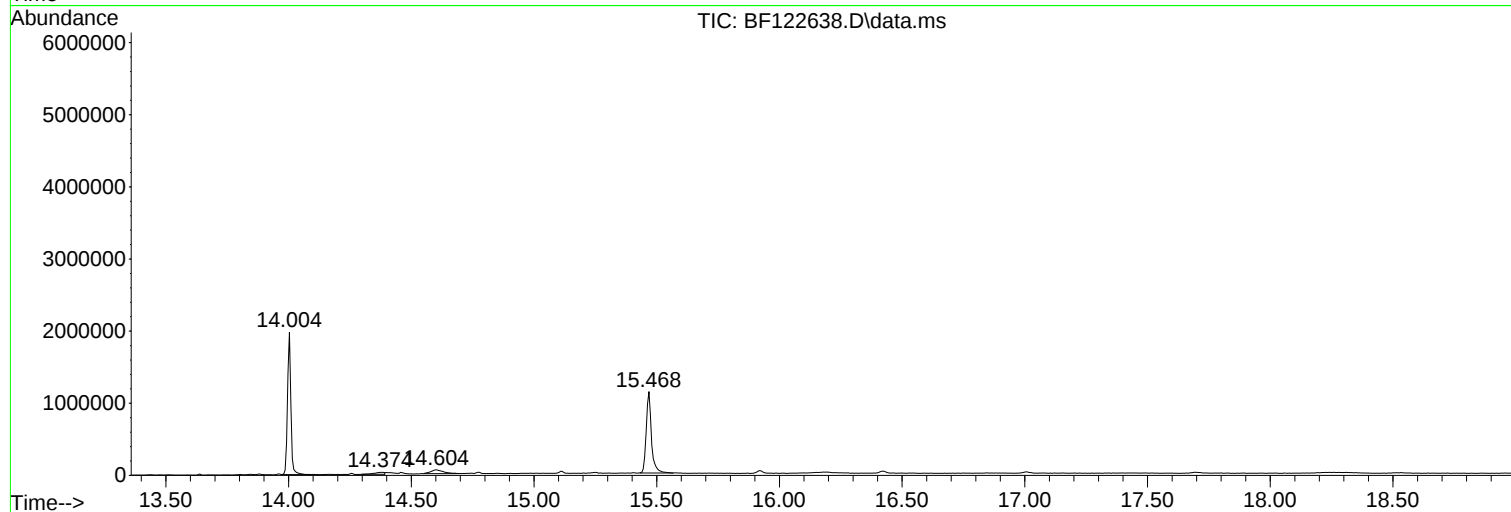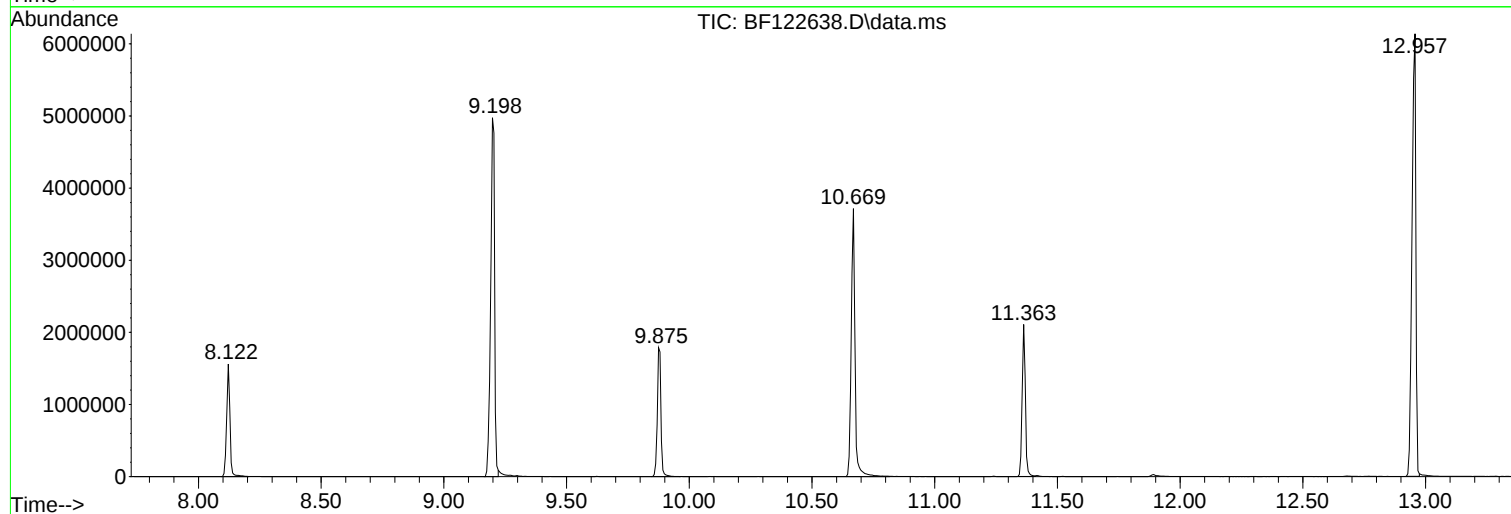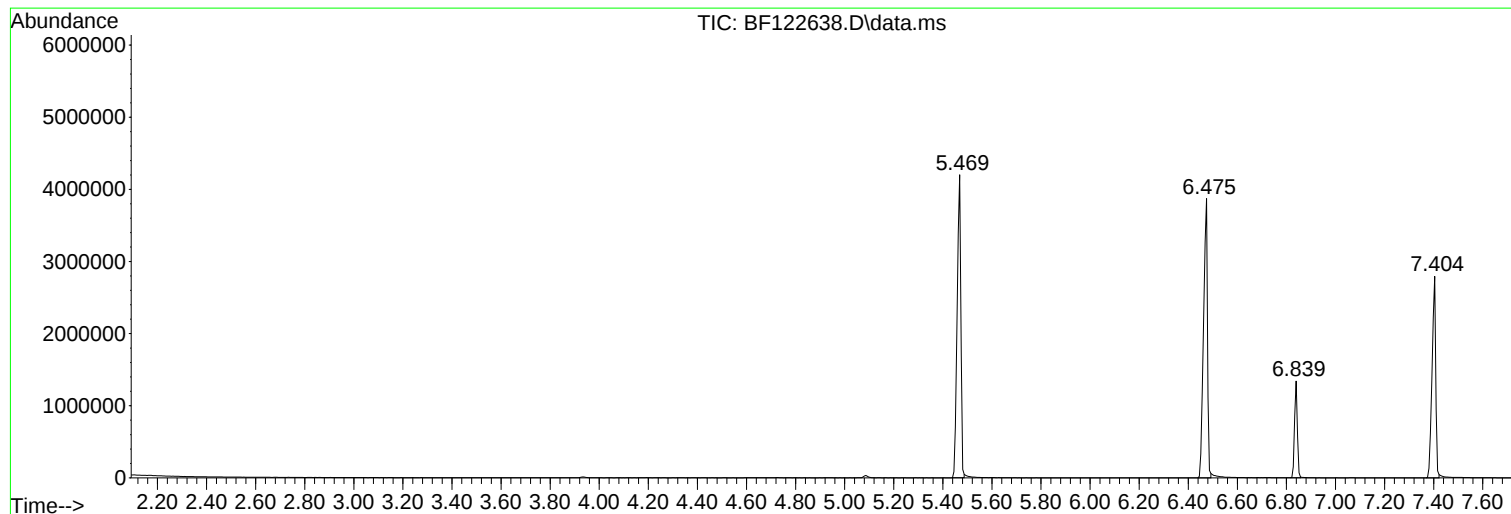

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF121020\  
Data File : BF122638.D  
Acq On : 10 Dec 2020 9:44  
Operator : JU/CG  
Sample : PB133474BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB133474BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF120520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF121020\  
Data File : BF122638.D  
Acq On : 10 Dec 2020 9:44  
Operator : JU/CG  
Sample : PB133474BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB133474BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF120520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|