
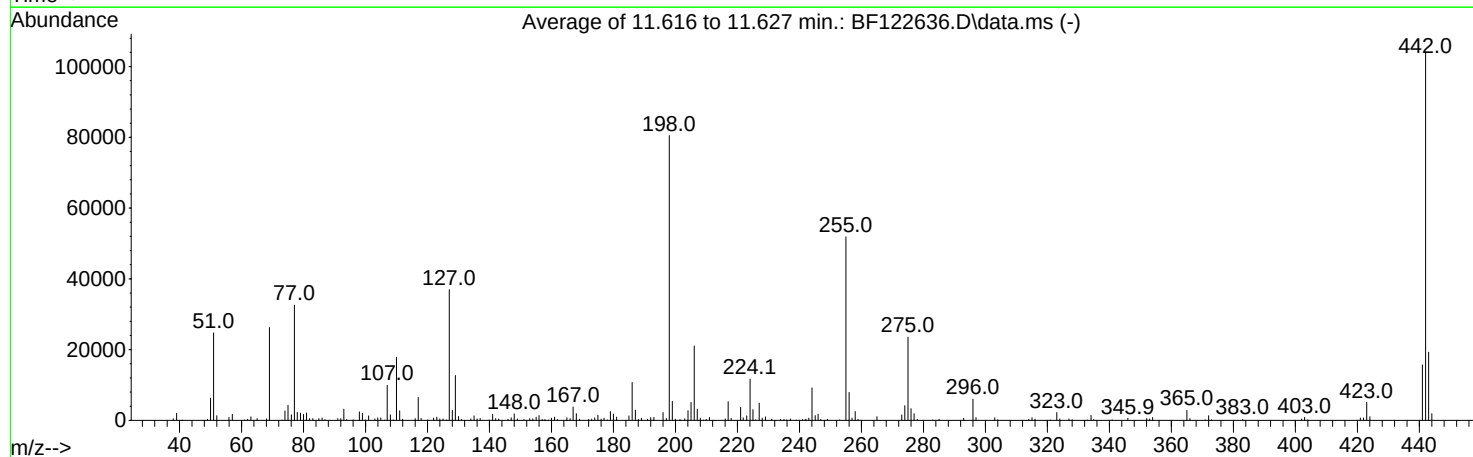


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121020\
Data File : BF122636.D
Acq On : 10 Dec 2020 8:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 07 12:08:49 2020

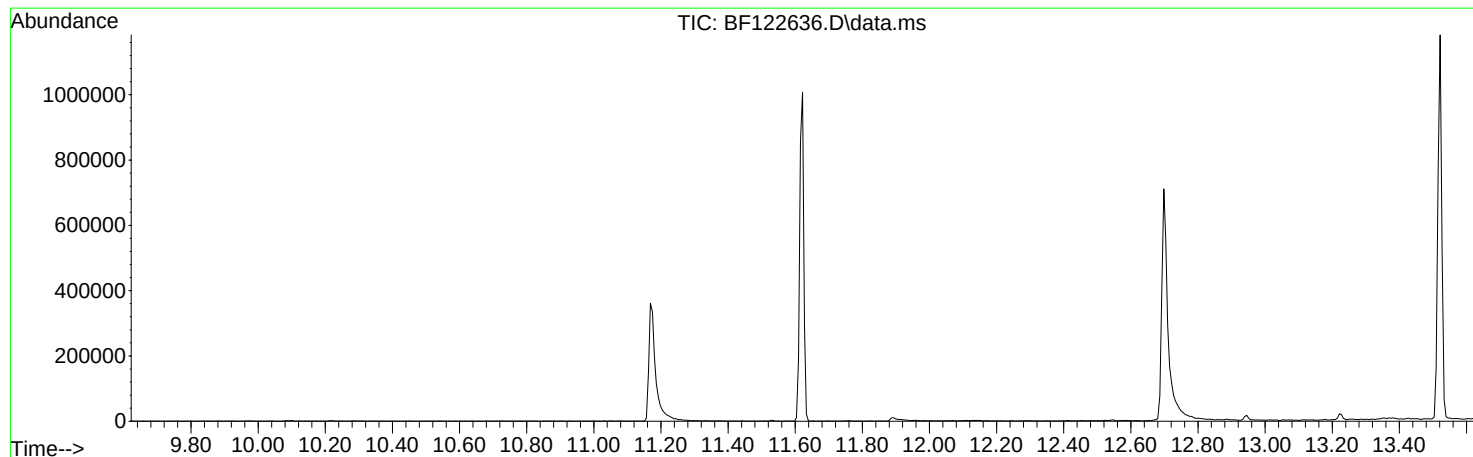

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	24746	PASS
68	69	0.00	2	1.5	398	PASS
69	198	0.00	100	32.6	26237	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	36928	PASS
197	198	0.00	2	0.6	518	PASS
198	198	100	100	100.0	80512	PASS
199	198	5	9	6.7	5394	PASS
275	198	10	60	29.2	23508	PASS
365	198	1	100	3.5	2814	PASS
441	198	0.01	100	19.5	15697	PASS
442	442	100	100	100.0	103971	PASS
443	442	15	24	18.5	19248	PASS