


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121022\
 Data File : BF131582.D
 Acq On : 10 Dec 2022 10:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 06:08:27 2022

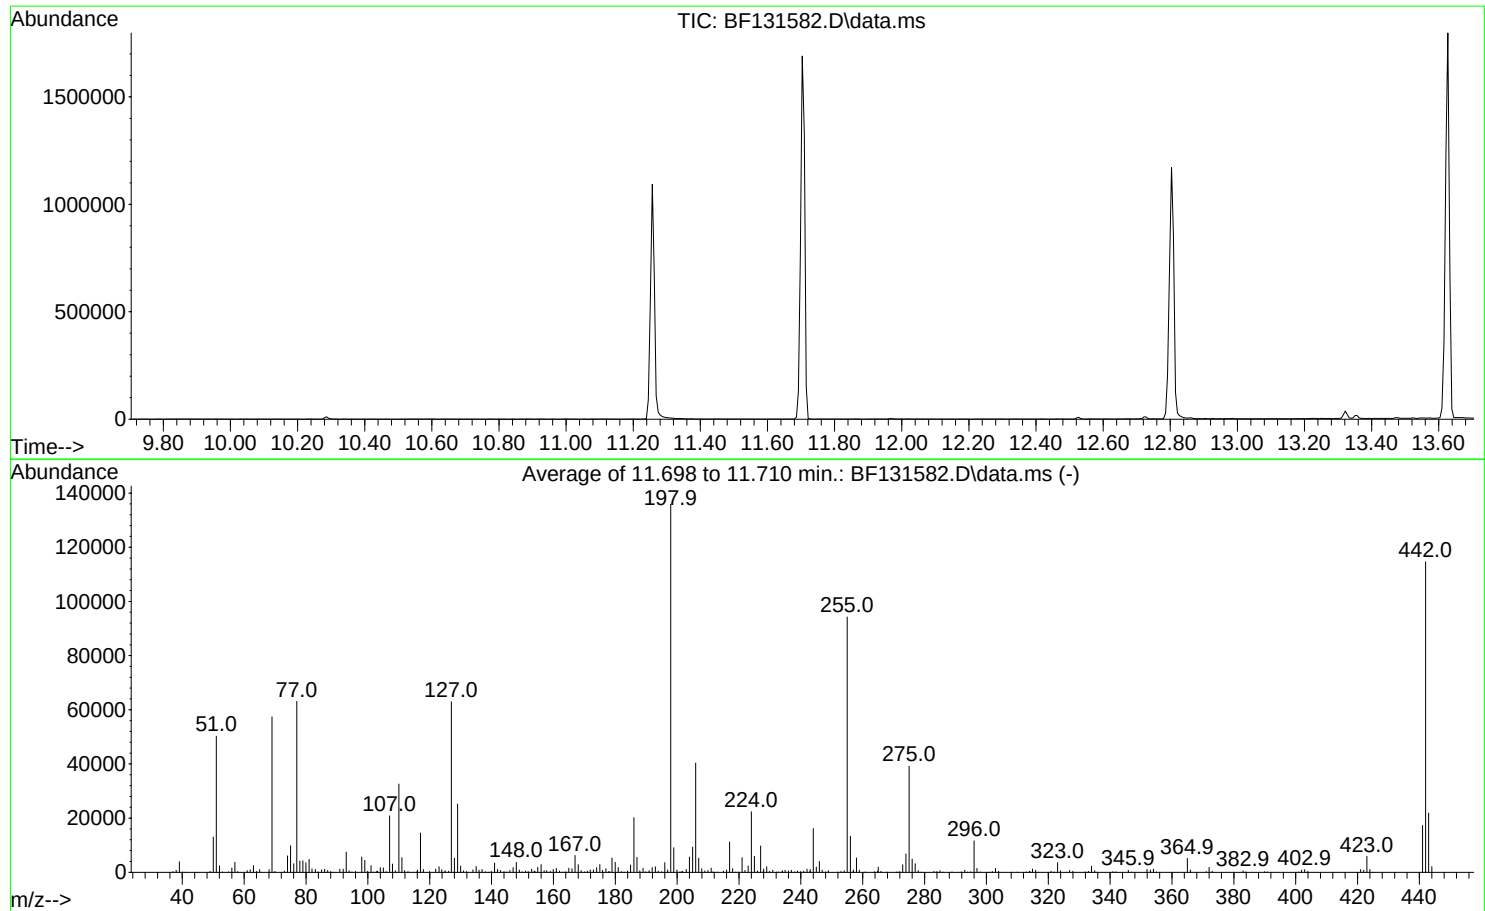




AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	50256	PASS
68	69	0.00	2	1.7	1001	PASS
69	198	0.00	100	42.3	57400	PASS
70	69	0.00	2	0.5	305	PASS
127	198	10	80	46.3	62920	PASS
197	198	0.00	2	0.6	845	PASS
198	198	100	100	100.0	135816	PASS
199	198	5	9	6.7	9076	PASS
275	198	10	60	28.8	39141	PASS
365	198	1	100	3.8	5128	PASS
441	198	0.01	100	12.7	17277	PASS
442	442	50	100	100.0	114624	PASS
443	442	15	24	19.1	21917	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121022\
Data File : BF131582.D
Acq On : 10 Dec 2022 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 12 07:30:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 06:08:27 2022
Response via : Initial Calibration

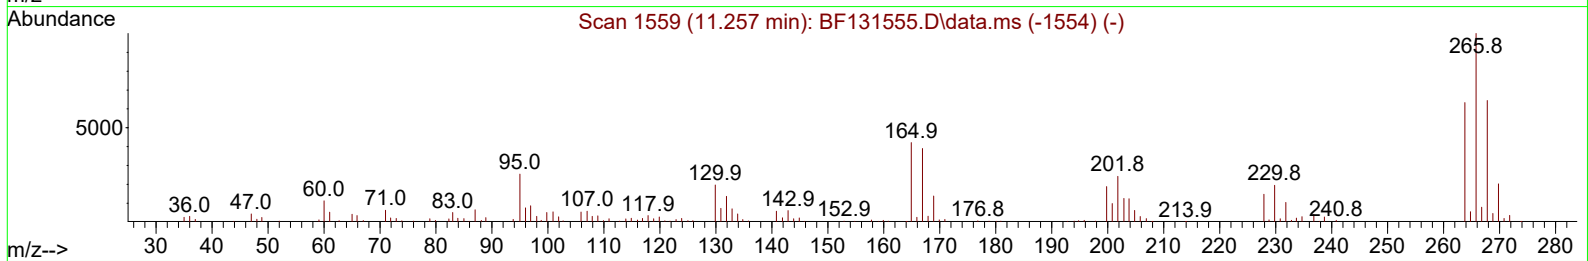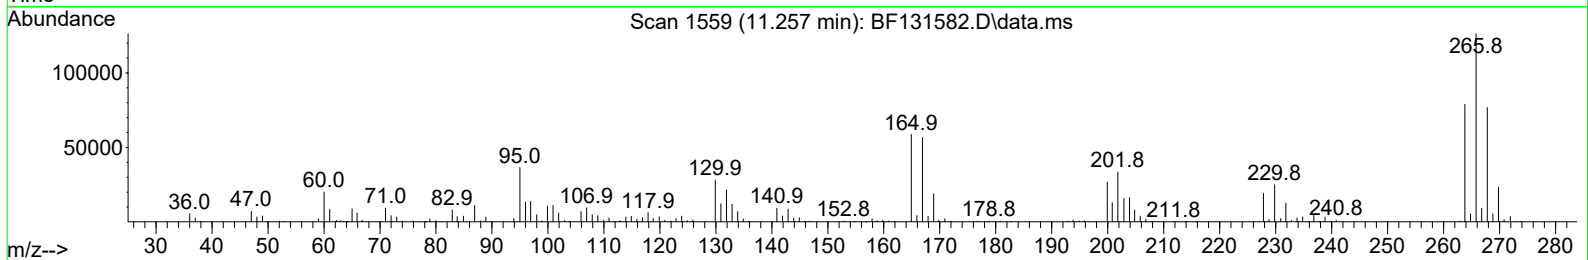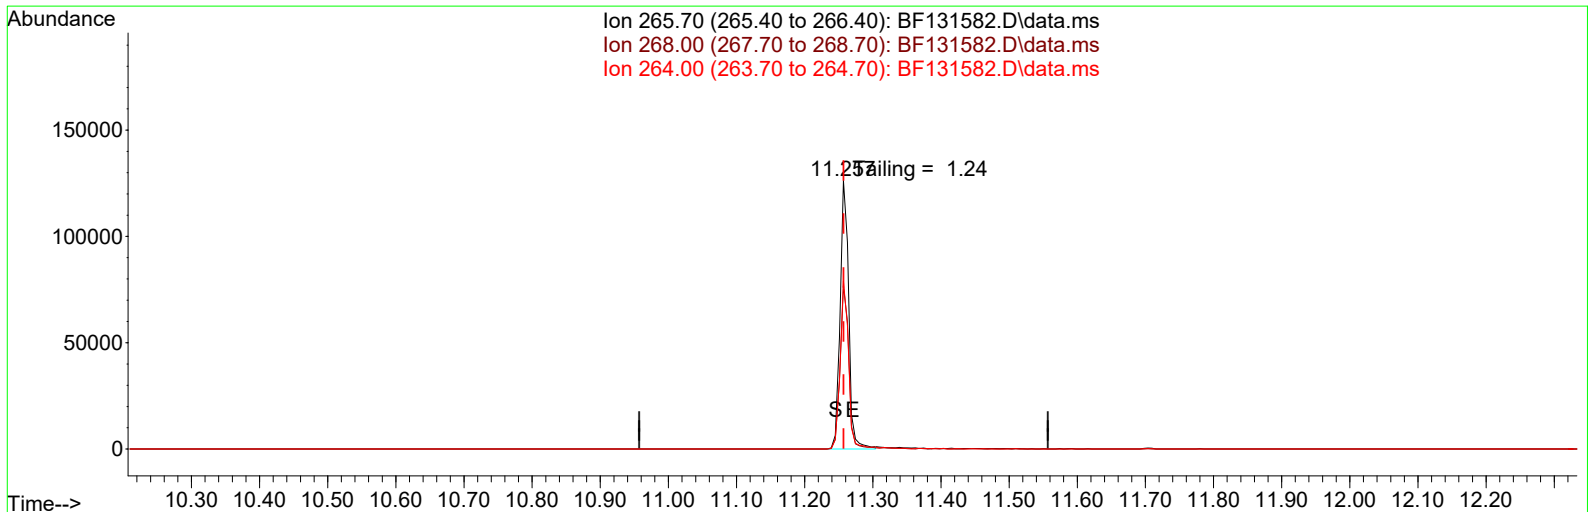

TIC: BF131582.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 26625.18 ng




response 111195

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	60.83
264.00	63.40	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121022\
Data File : BF131582.D
Acq On : 10 Dec 2022 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 12 07:30:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 06:08:27 2022
Response via : Initial Calibration

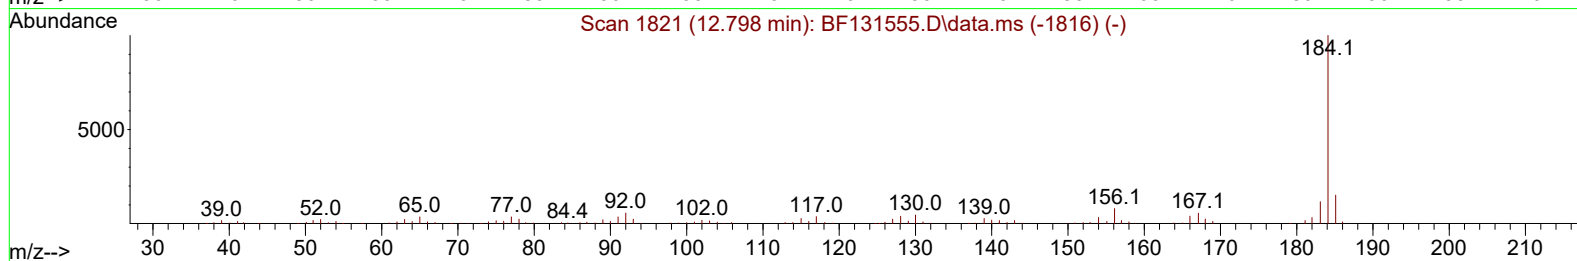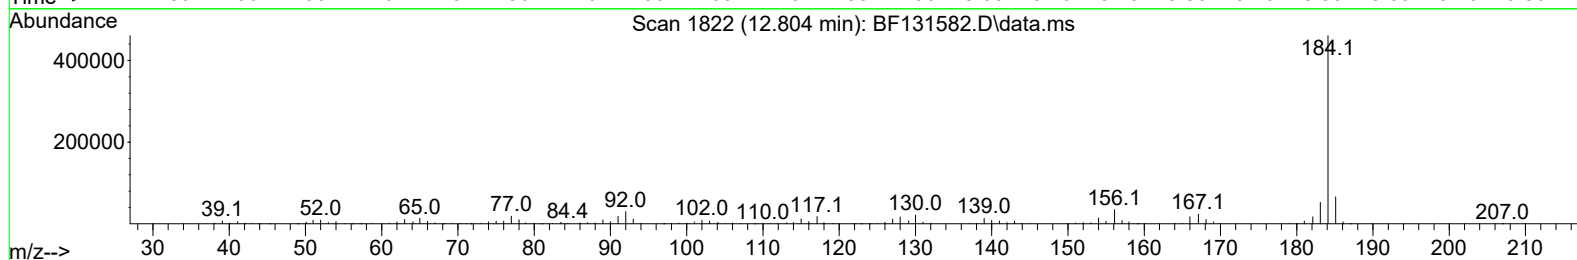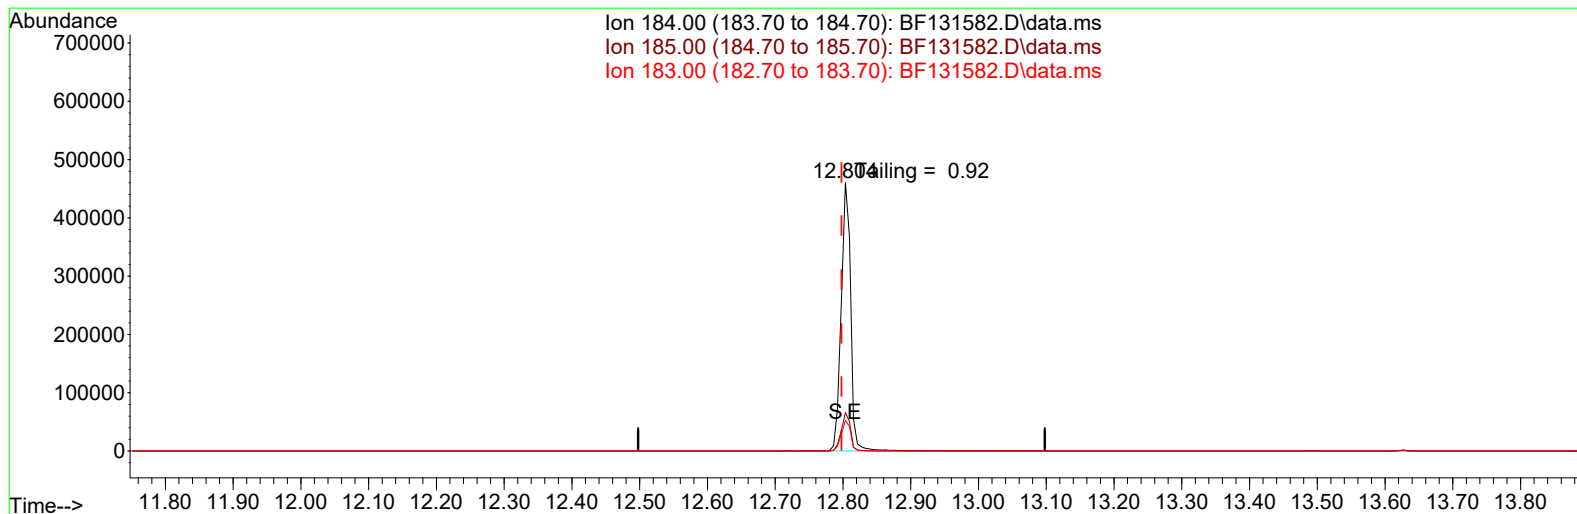

TIC: BF131582.D\data.ms

(77) Benzidine

12.804min (+ 0.006) 0.00 ng

response 447083

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.35
183.00	11.60	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/10/2022	BNA_F	<u>BF131582.D</u>
Compound Name	Response	Retention Time
DDT	285113	13.627
DDD	7737	13.321
DDE	331	12.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8068	293181	2.75

Instrument :
BNA_F
ClientSampleId :
DFTPP