

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
 Data File : BF140806.D
 Acq On : 10 Dec 2024 15:23
 Operator : RC/JU
 Sample : P5174-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROLL-OFF-COMP

Quant Time: Dec 10 16:46:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 15:23:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	88201	20.000	ng	-0.01
21) Naphthalene-d8	8.145	136	332013	20.000	ng	-0.01
39) Acenaphthene-d10	9.898	164	184172	20.000	ng	-0.02
64) Phenanthrene-d10	11.392	188	322964	20.000	ng	-0.01
76) Chrysene-d12	14.045	240	158184	20.000	ng	0.00
86) Perylene-d12	15.557	264	104862	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.522	112	654532	126.616	ng	0.02
7) Phenol-d6	6.522	99	795505	116.403	ng	0.00
23) Nitrobenzene-d5	7.428	82	594478	91.586	ng	-0.01
42) 2,4,6-Tribromophenol	10.698	330	259517	131.752	ng	0.00
45) 2-Fluorobiphenyl	9.216	172	1155029	93.441	ng	-0.02
79) Terphenyl-d14	12.980	244	937602	92.296	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
Data File : BF140806.D
Acq On : 10 Dec 2024 15:23
Operator : RC/JU
Sample : P5174-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP

Quant Time: Dec 10 16:46:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration



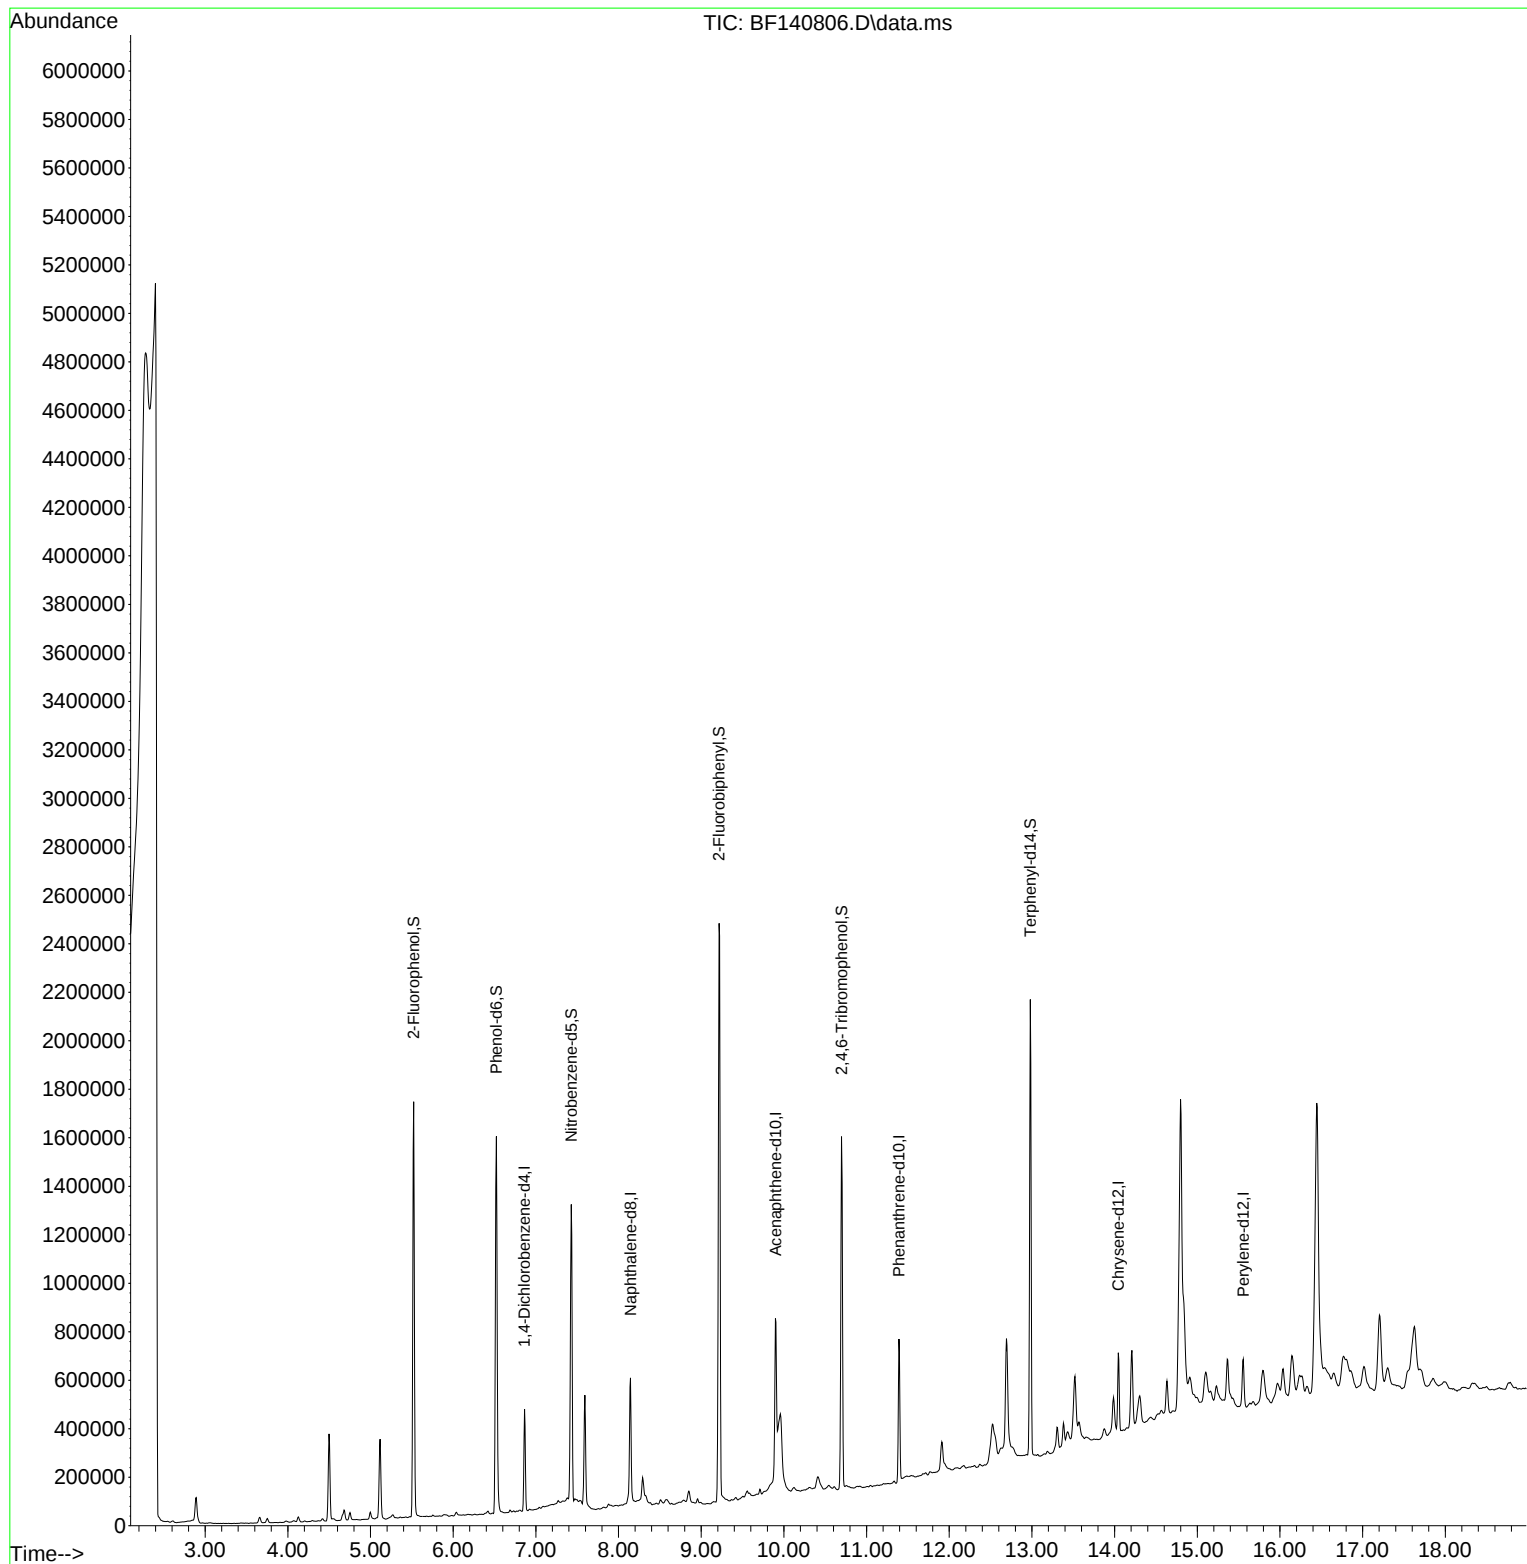




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.863 min Scan# 813
Delta R.T. -0.012 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23




Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP


Tgt Ion:152 Resp: 88201
Ion Ratio Lower Upper
152 100
150 158.6 128.5 192.7
115 61.5 50.2 75.4

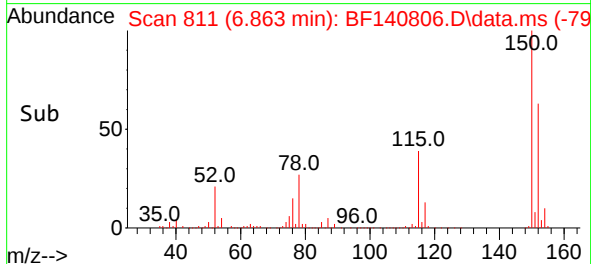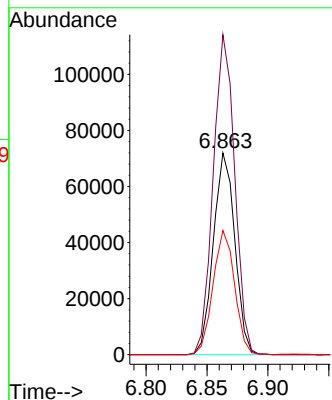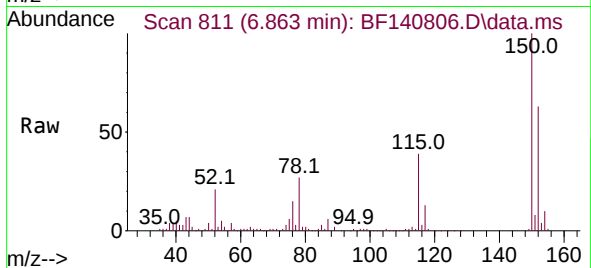

#5
2-Fluorophenol
Concen: 126.616 ng
RT: 5.522 min Scan# 583
Delta R.T. 0.024 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23

Tgt Ion:112 Resp: 654532
Ion Ratio Lower Upper
112 100
64 58.3 49.2 73.8
63 30.5 27.0 40.4


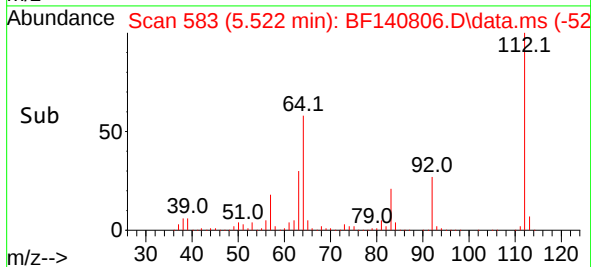
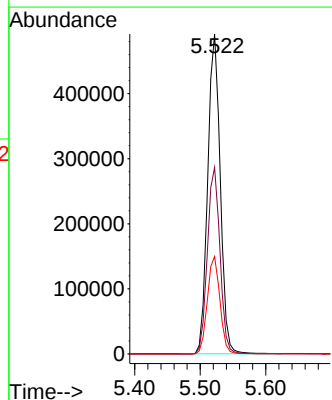
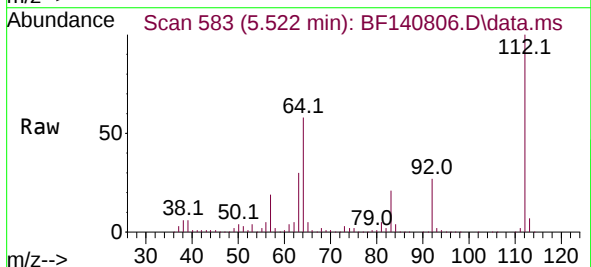


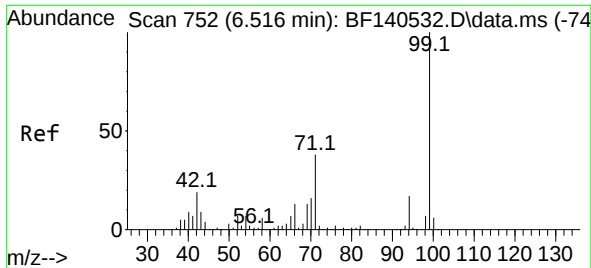

#7
Phenol-d6
Concen: 116.403 ng
RT: 6.522 min Scan# 71
Delta R.T. 0.006 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23




Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP


Tgt Ion: 99 Resp: 795505
Ion Ratio Lower Upper
99 100
42 18.0 15.4 23.0
71 35.9 30.6 46.0

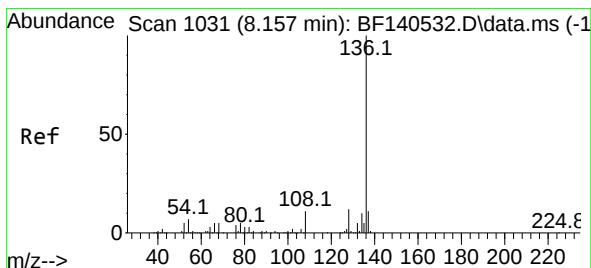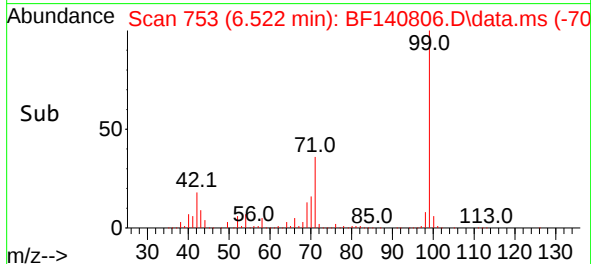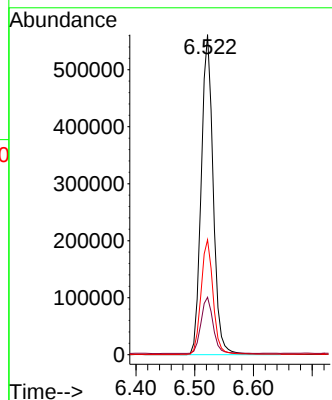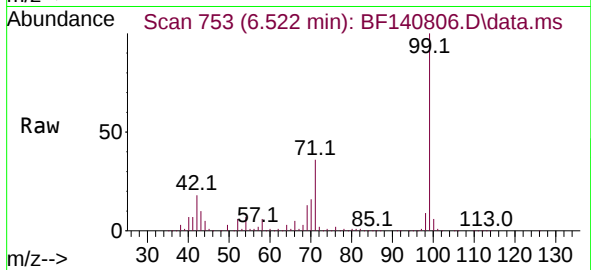

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.145 min Scan# 1029
Delta R.T. -0.012 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23

Tgt Ion: 136 Resp: 332013
Ion Ratio Lower Upper
136 100
137 10.5 8.6 13.0
54 7.3 5.8 8.8
68 5.5 4.1 6.1


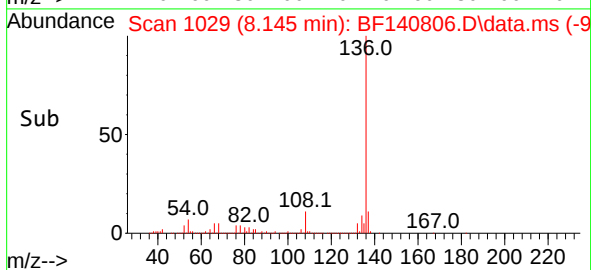
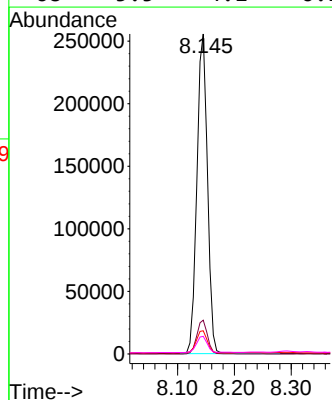
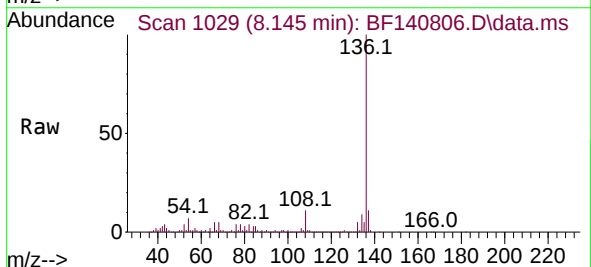


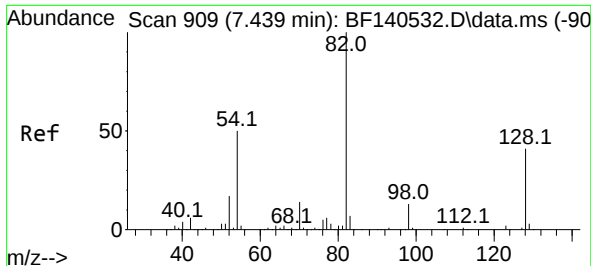

#23
Nitrobenzene-d5
Concen: 91.586 ng
RT: 7.428 min Scan# 909
Delta R.T. -0.012 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23




Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP


Tgt Ion: 82 Resp: 594478
Ion Ratio Lower Upper
82 100
128 43.6 33.0 49.4
54 47.9 39.5 59.3

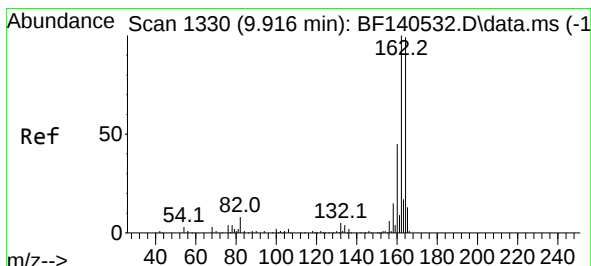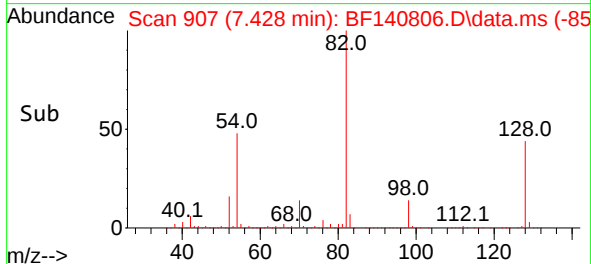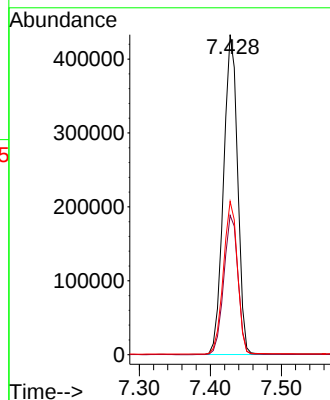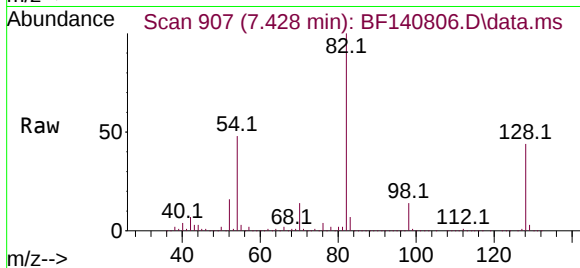

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.898 min Scan# 1327
Delta R.T. -0.018 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23

Tgt Ion:164 Resp: 184172
Ion Ratio Lower Upper
164 100
162 99.9 80.6 120.8
160 43.1 36.2 54.4


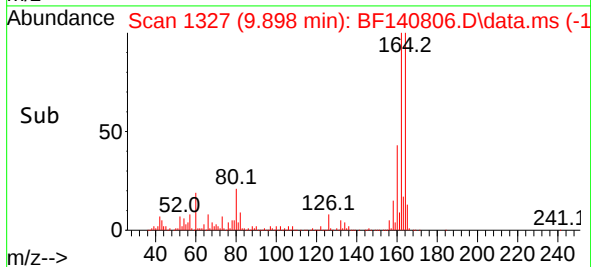
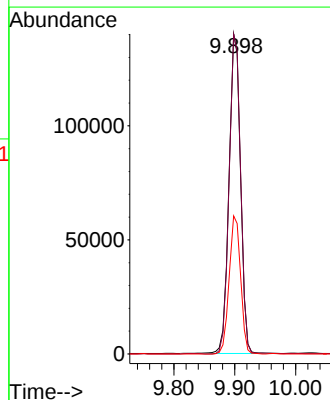
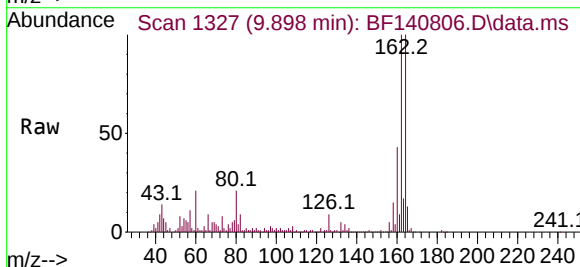


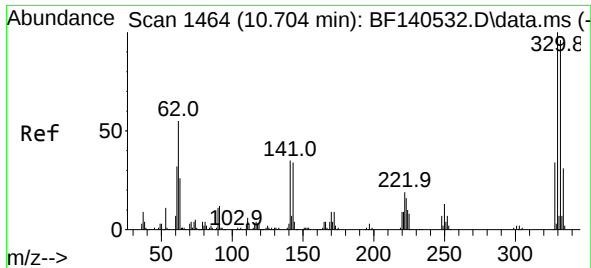

#42
2,4,6-Tribromophenol
Concen: 131.752 ng
RT: 10.698 min Scan# 1463
Delta R.T. -0.006 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23




Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP


Tgt Ion:330 Resp: 259517
Ion Ratio Lower Upper
330 100
332 97.3 76.9 115.3
141 31.8 26.7 40.1

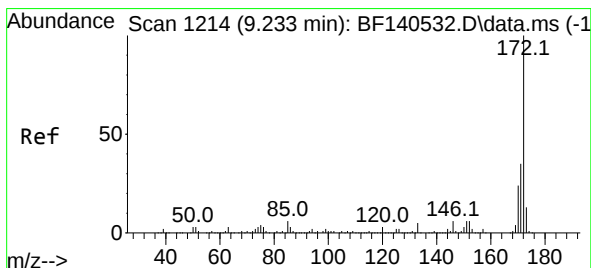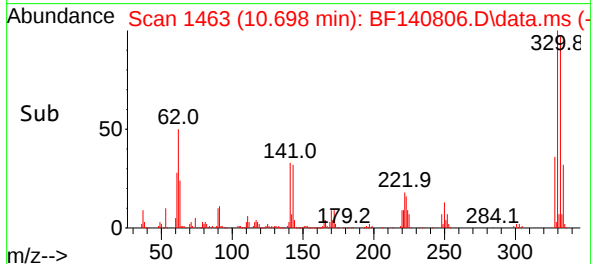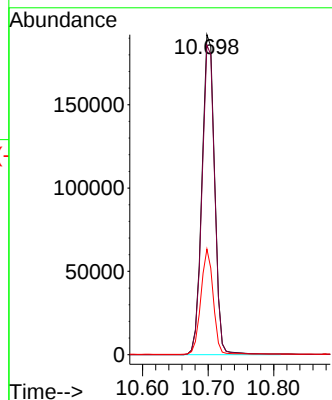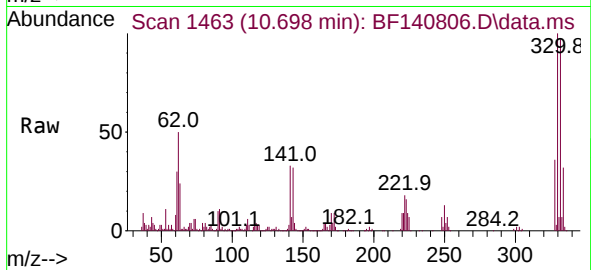

#45
2-Fluorobiphenyl
Concen: 93.441 ng
RT: 9.216 min Scan# 1211
Delta R.T. -0.018 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23

Tgt Ion:172 Resp: 1155029
Ion Ratio Lower Upper
172 100
171 35.3 28.4 42.6
170 23.6 19.0 28.6


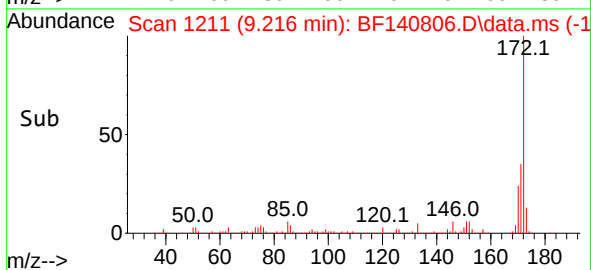
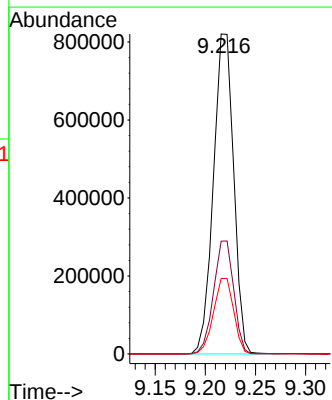
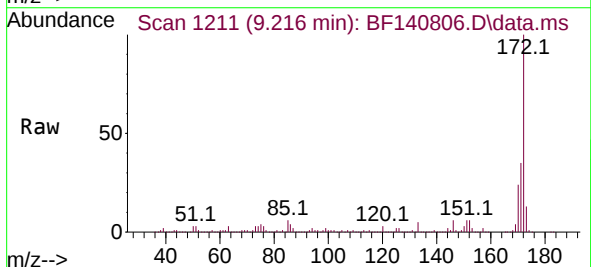


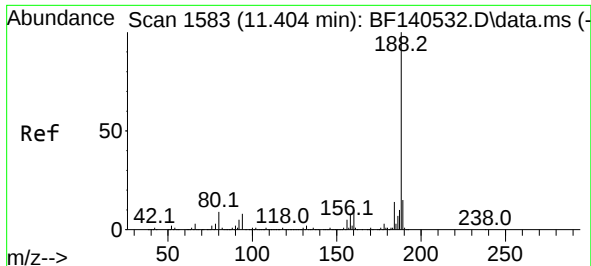

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.392 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23




Instrument :
BNA_F
ClientSampleId :
ROLL-OFF-COMP


Tgt Ion:188 Resp: 322964
Ion Ratio Lower Upper
188 100
94 8.5 6.4 9.6
80 9.4 6.9 10.3

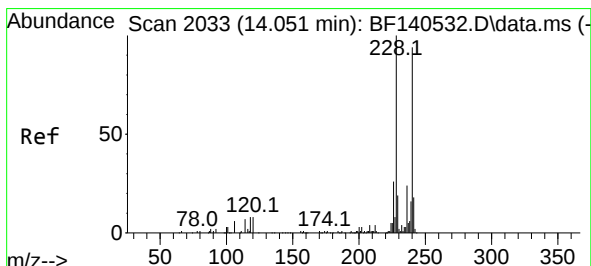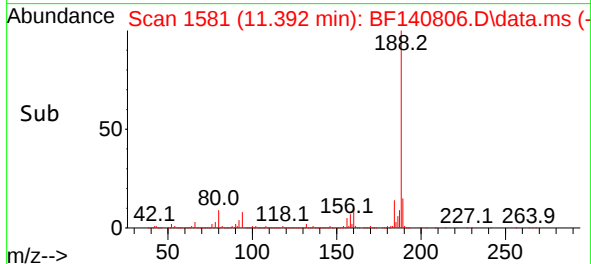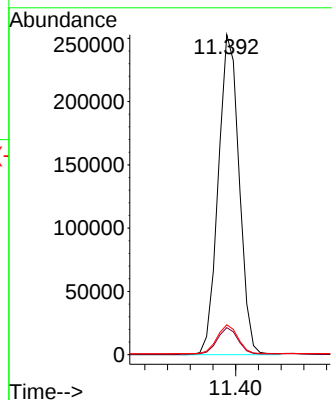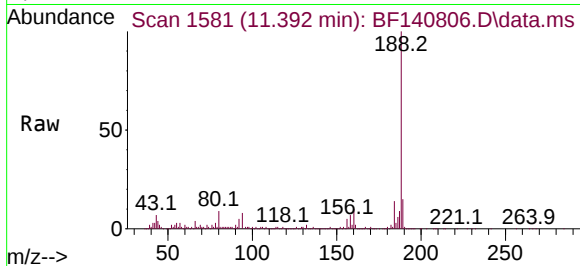

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF140806.D
Acq: 10 Dec 2024 15:23

Tgt Ion:240 Resp: 158184
Ion Ratio Lower Upper
240 100
120 9.7 7.3 10.9
236 25.3 20.6 31.0


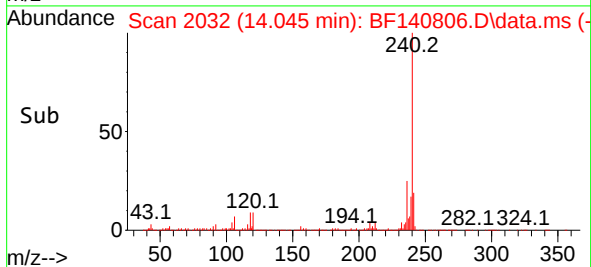
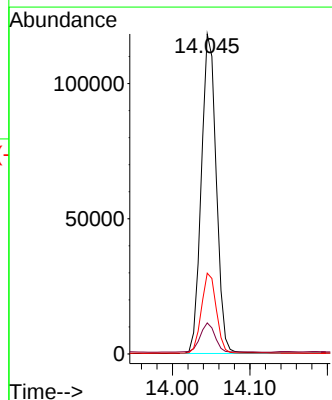
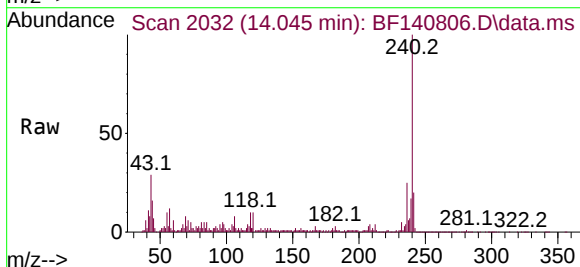


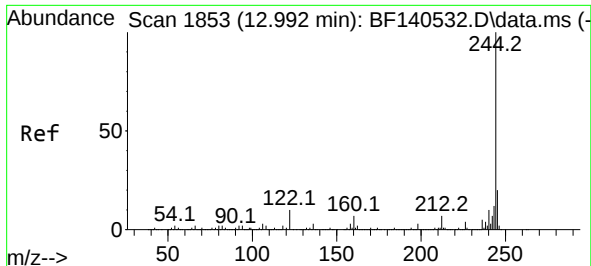

#79
 Terphenyl-d14
 Concen: 92.296 ng
 RT: 12.980 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BF140806.D
 Acq: 10 Dec 2024 15:23

Instrument :
 BNA_F
 ClientSampleId :
 ROLL-OFF-COMP

Tgt Ion:244 Resp: 937602
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.8 8.8
 122 10.4 8.0 12.0

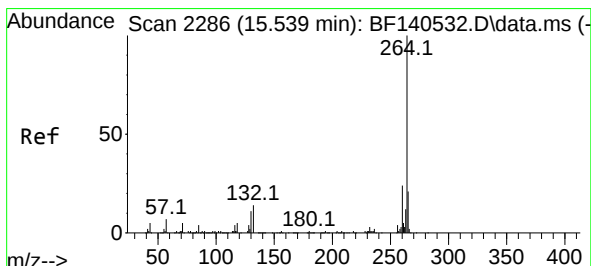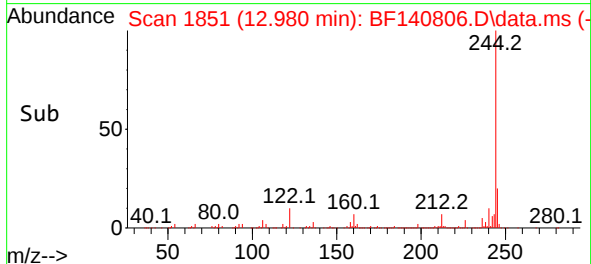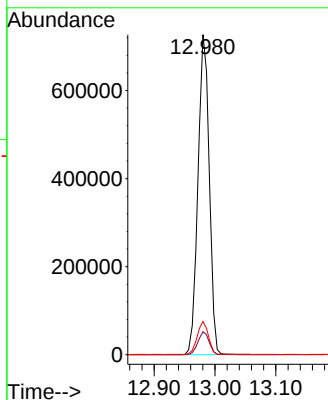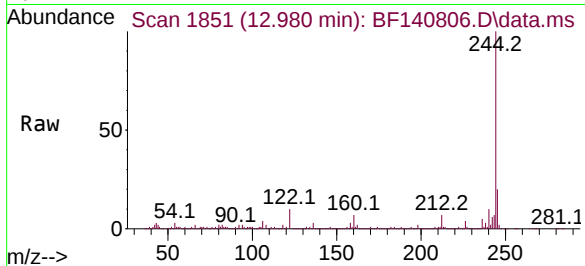

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.557 min Scan# 2289
 Delta R.T. 0.018 min
 Lab File: BF140806.D
 Acq: 10 Dec 2024 15:23

Tgt Ion:264 Resp: 104862
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.0 28.6
 265 21.2 16.6 25.0

