

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
 Data File : BF140796.D
 Acq On : 10 Dec 2024 10:31
 Operator : RC/JU
 Sample : PB165477BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB165477BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	14	20	34	rVB	42367	77494	2.17%	0.409%
2	5.504	575	580	613	rBV	1738841	2351077	65.98%	12.421%
3	6.510	745	751	779	rVB	1633769	2391784	67.12%	12.636%
4	6.863	806	811	823	rVB	376555	472171	13.25%	2.495%
5	7.428	900	907	925	rBV	1118178	1580555	44.36%	8.350%
6	8.145	1023	1029	1045	rBV	443516	621706	17.45%	3.285%
7	9.216	1204	1211	1235	rBV	2324940	3204597	89.93%	16.930%
8	9.898	1321	1327	1342	rVB	567135	743782	20.87%	3.930%
9	10.698	1457	1463	1495	rBV	1378383	1959586	54.99%	10.353%
10	11.392	1575	1581	1605	rBV	615159	831011	23.32%	4.390%
11	12.980	1845	1851	1856	rBV	2683040	3563365	100.00%	18.826%
12	14.045	2027	2032	2046	rVB	449539	640322	17.97%	3.383%
13	15.539	2280	2286	2301	rBV	279485	490518	13.77%	2.591%




Sum of corrected areas: 18927968

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
Data File : BF140796.D
Acq On : 10 Dec 2024 10:31
Operator : RC/JU
Sample : PB165477BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165477BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

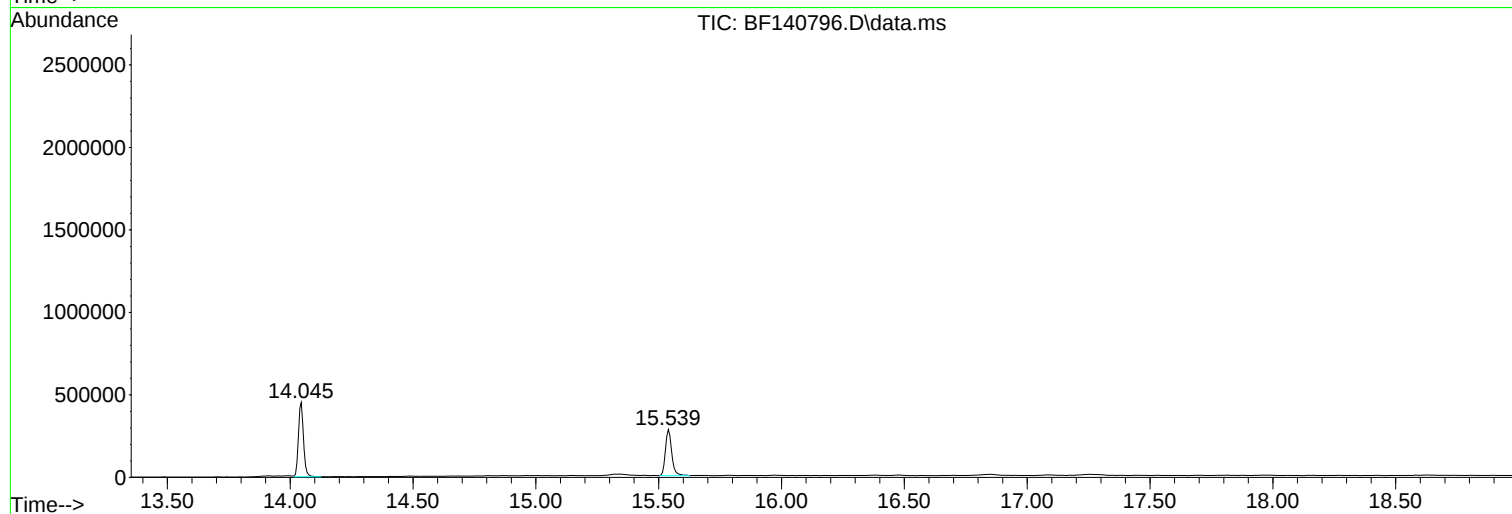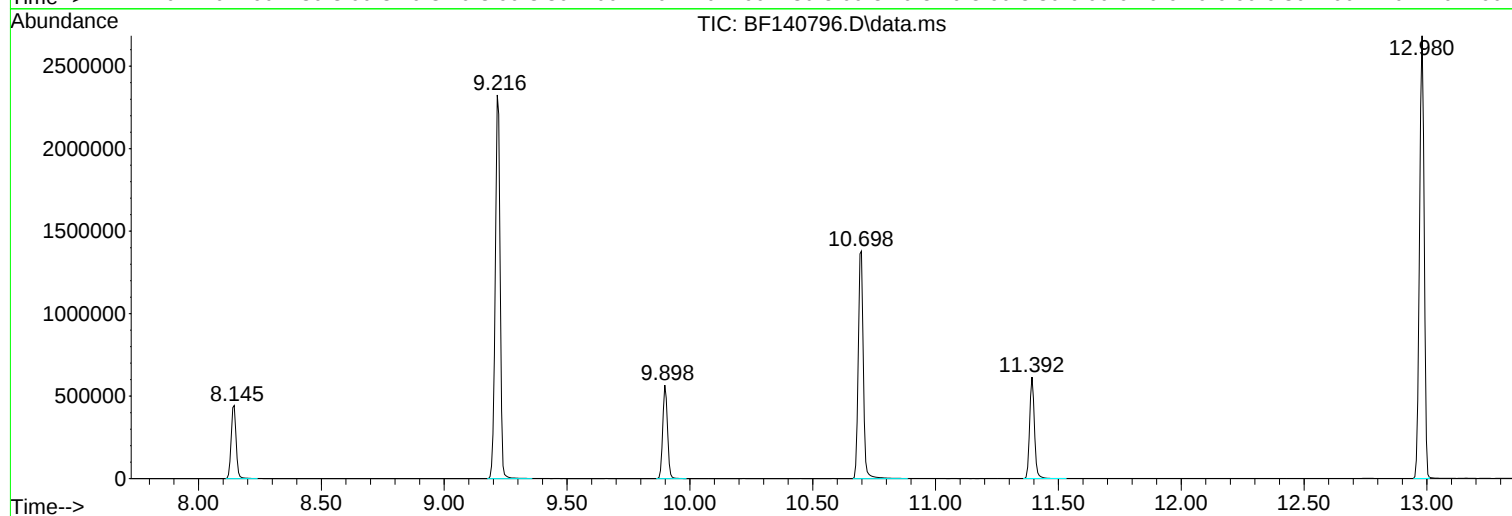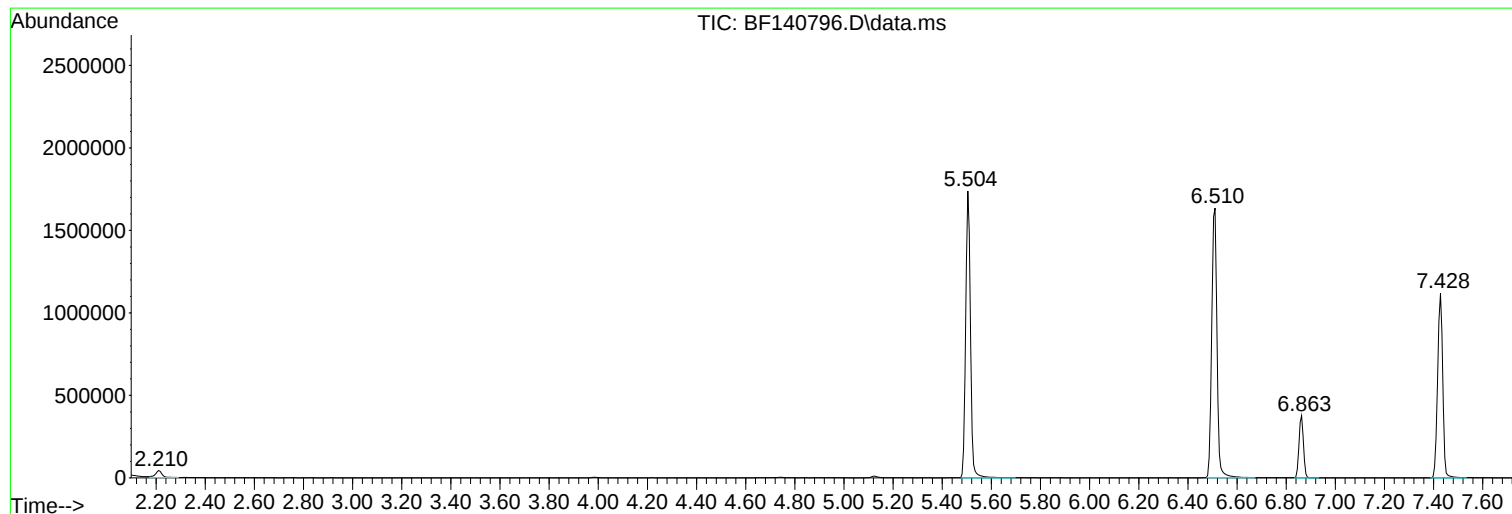

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
Data File : BF140796.D
Acq On : 10 Dec 2024 10:31
Operator : RC/JU
Sample : PB165477BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165477BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.210	3.28 ng	77494	1,4-Dichlorobenzene-d4	6.863

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17

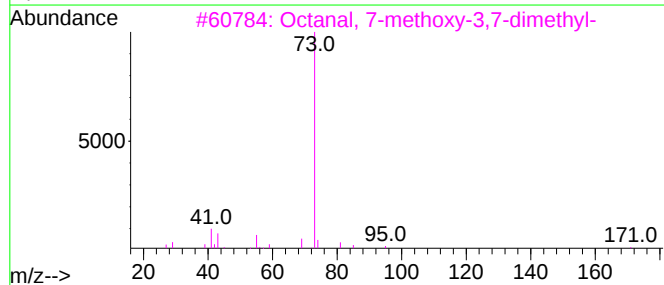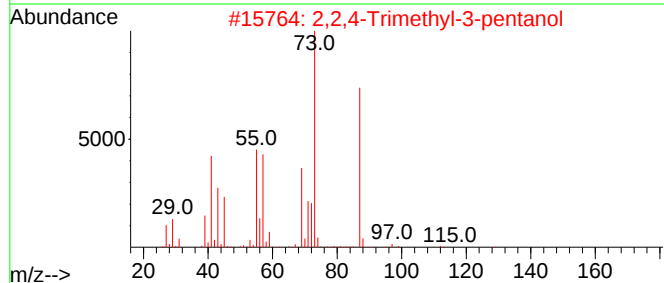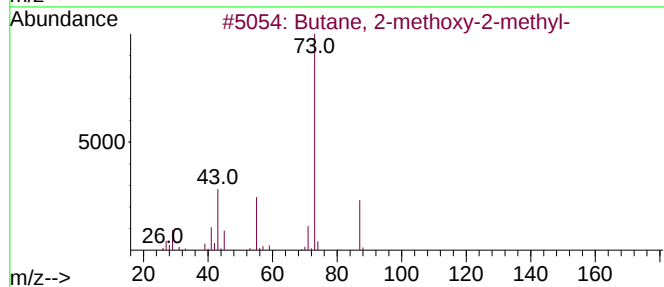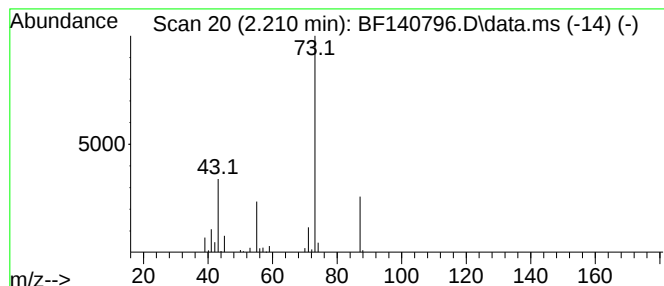

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
Data File : BF140796.D
Acq On : 10 Dec 2024 10:31
Operator : RC/JU
Sample : PB165477BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165477BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.210	3.3	ng	77494	1	6.863	472171	20.0