


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
Data File : BF140794.D
Acq On : 10 Dec 2024 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

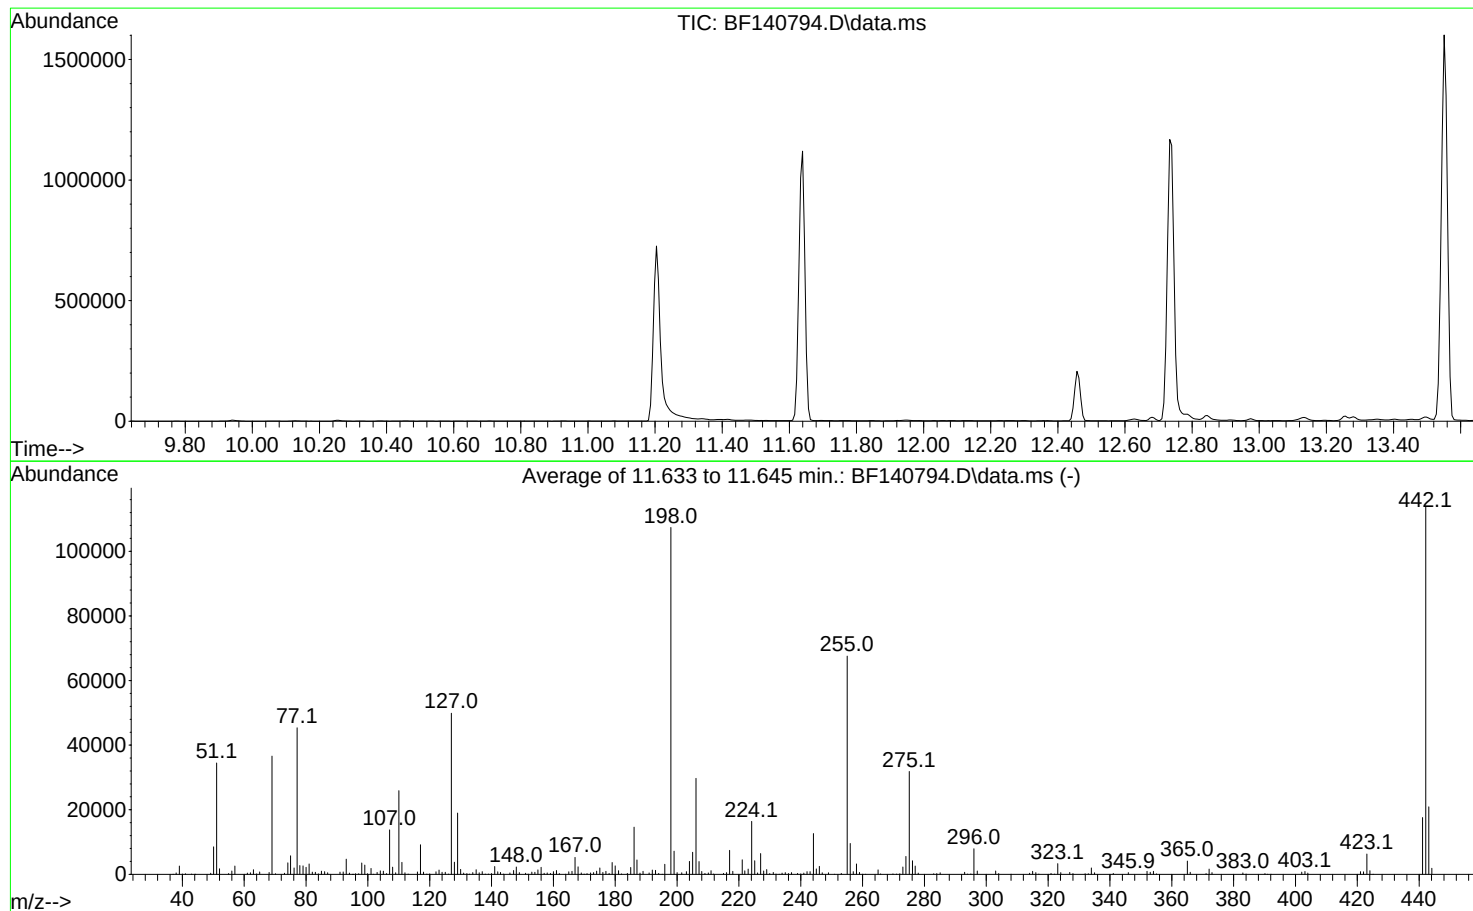

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	34491	PASS
68	69	0.00	2	1.7	612	PASS
69	198	0.00	100	34.1	36603	PASS
70	69	0.00	2	0.6	224	PASS
127	198	10	80	46.4	49859	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	107384	PASS
199	198	5	9	6.7	7204	PASS
275	198	10	60	29.7	31861	PASS
365	198	1	100	3.8	4092	PASS
441	198	0.01	100	16.4	17566	PASS
442	442	50	100	100.0	113861	PASS
443	442	15	24	18.4	20920	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/10/2024	BNA_F	<u>BF140794.D</u>
Compound Name	Response	Retention Time
DDT	411486	13.557
DDD	11786	13.257
DDE	692	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12478	423964	2.94

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
Data File : BF140794.D
Acq On : 10 Dec 2024 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 10 13:02:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

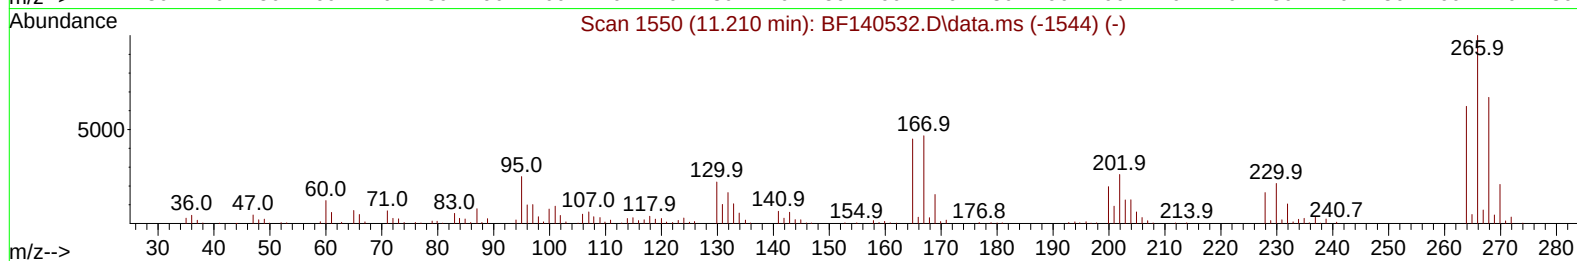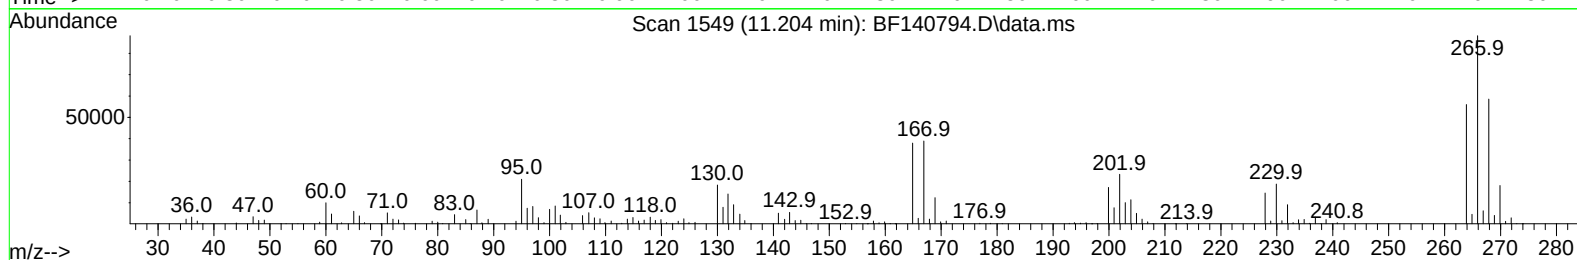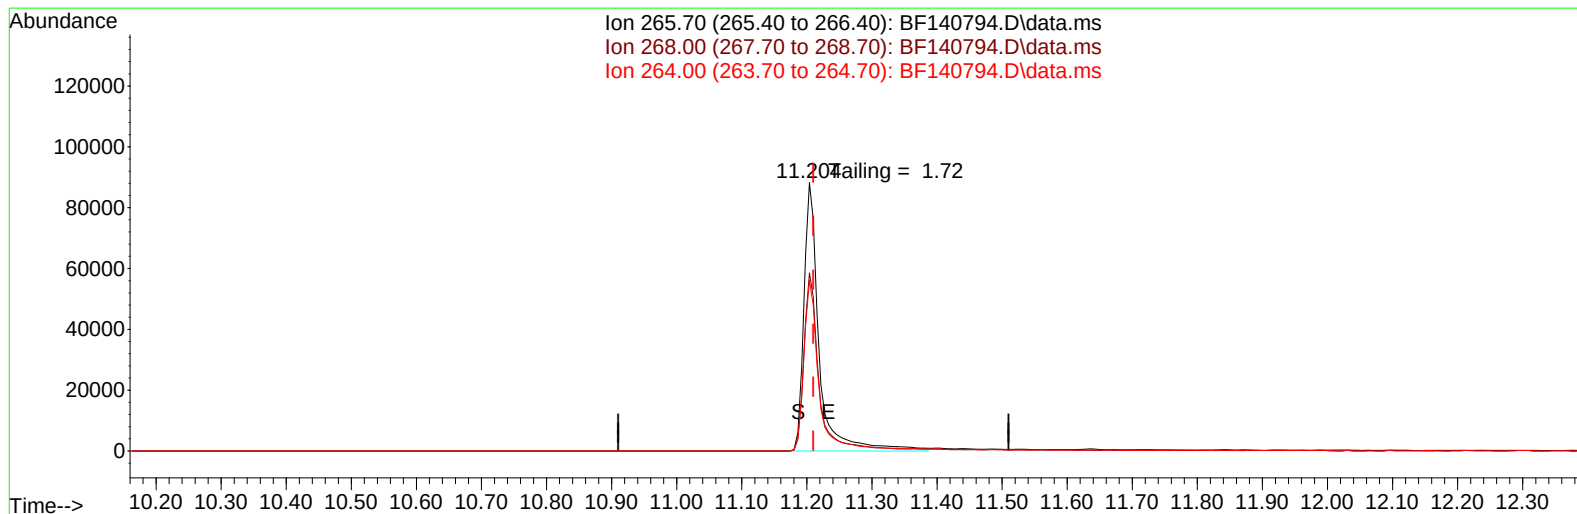

TIC: BF140794.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 18336.39 ng




response 144930

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.34
264.00	62.30	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121024\
Data File : BF140794.D
Acq On : 10 Dec 2024 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 10 13:02:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

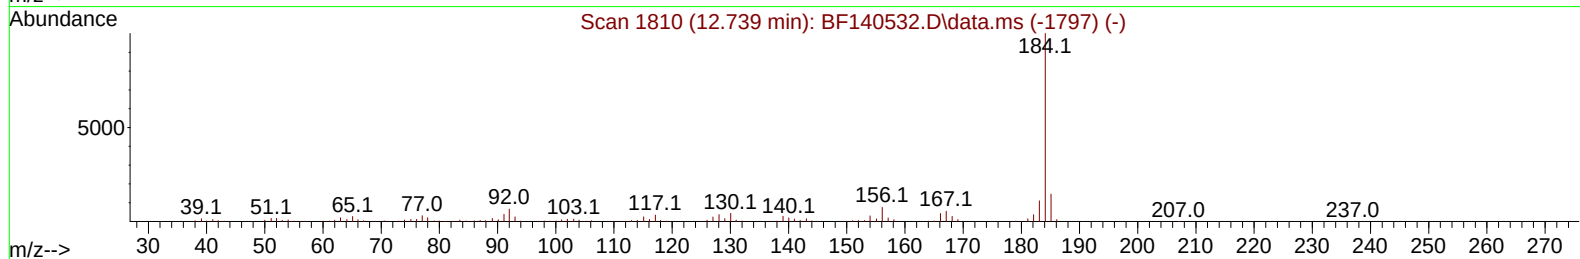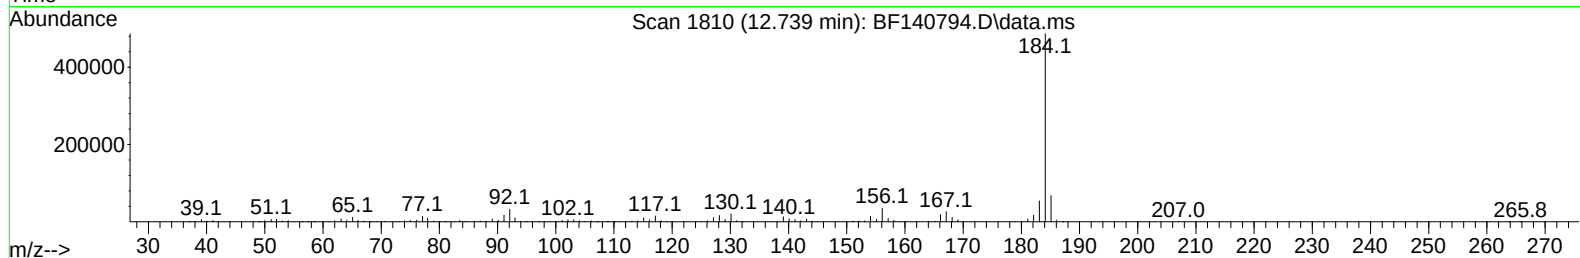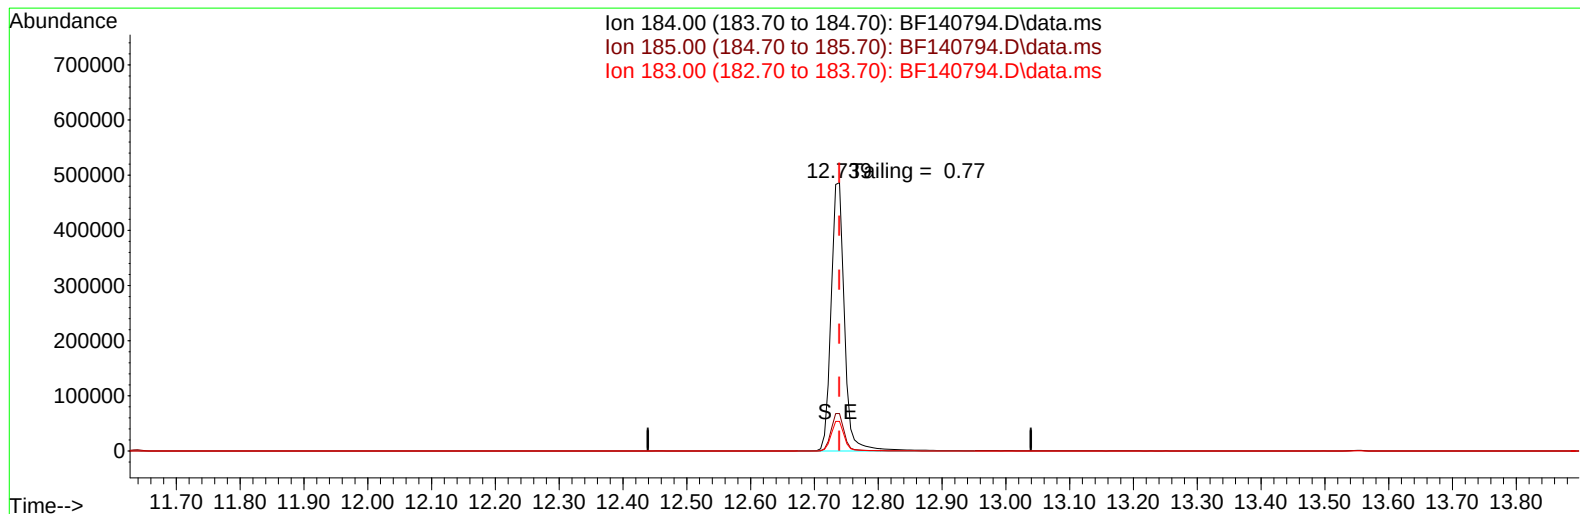

TIC: BF140794.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 18878.97 ng

response 709173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.95
183.00	11.00	11.08
0.00	0.00	0.00