
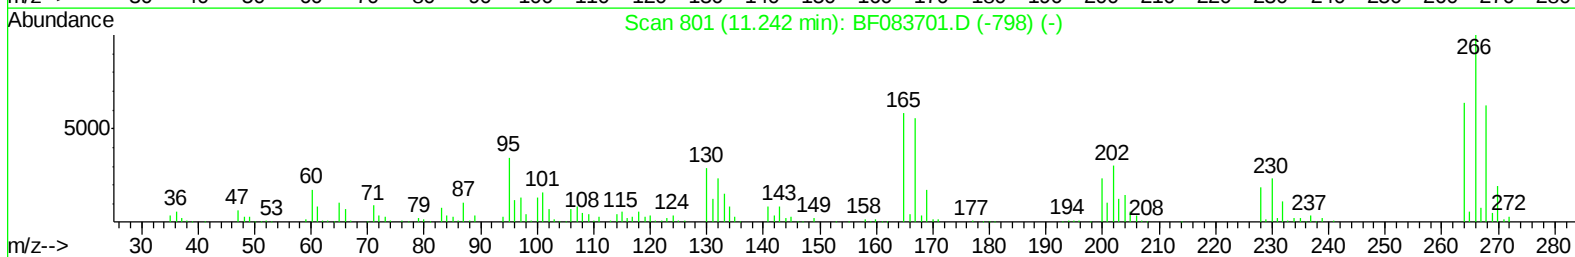
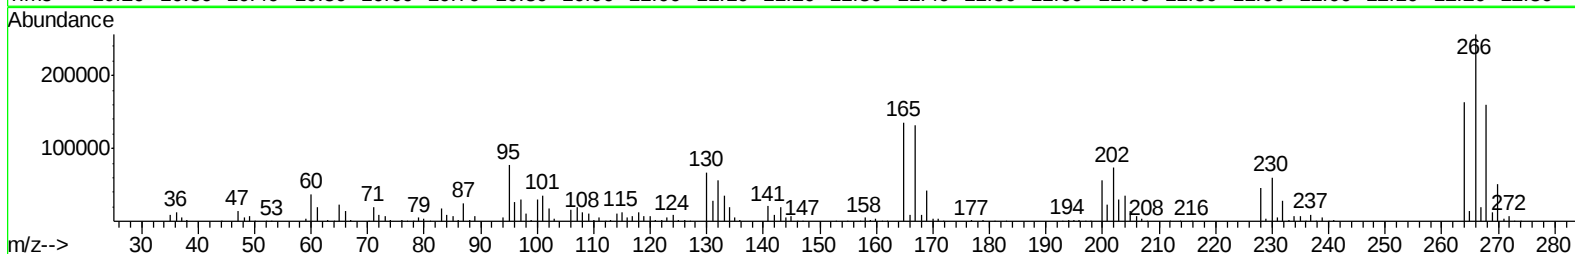


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121115\
Data File : BF083706.D
Acq On : 11 Dec 2015 20:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 04:41:29 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 11 19:24:37 2015
Response via : Initial Calibration

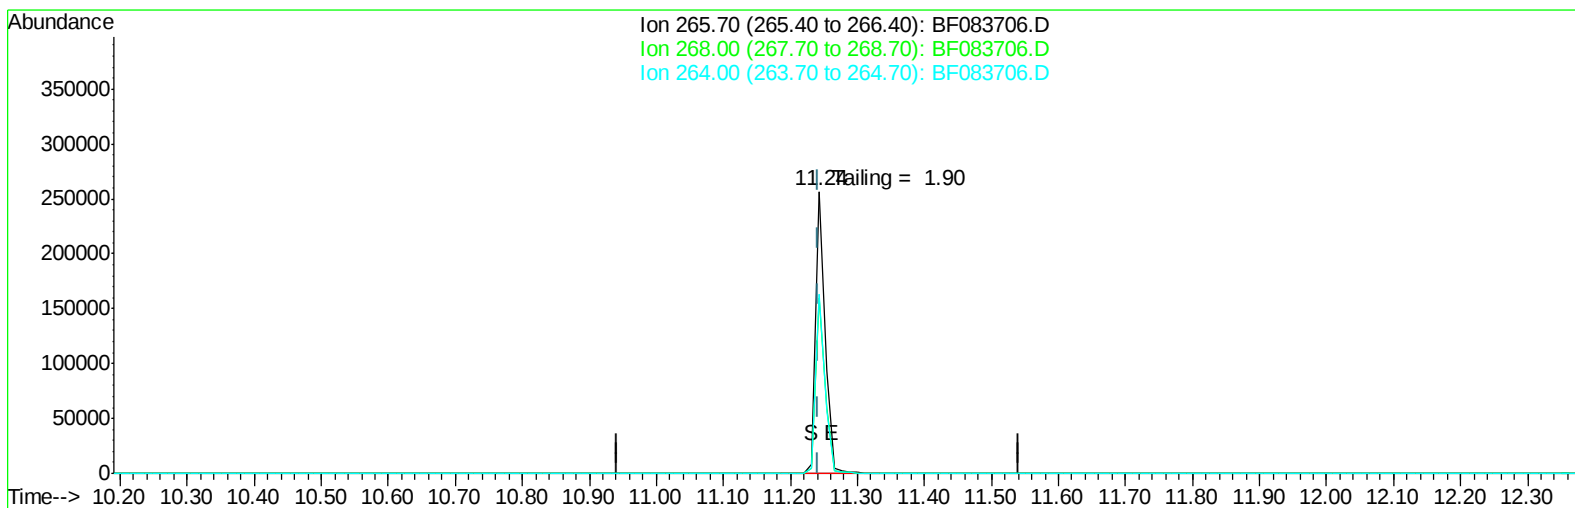

TIC: BF083706.D

(69) Pentachlorophenol (C)




11.242min (+0.000) 140164.14ng

response 252263

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	62.41
264.00	64.30	63.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121115\
Data File : BF083706.D
Acq On : 11 Dec 2015 20:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 04:41:29 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 11 19:24:37 2015
Response via : Initial Calibration

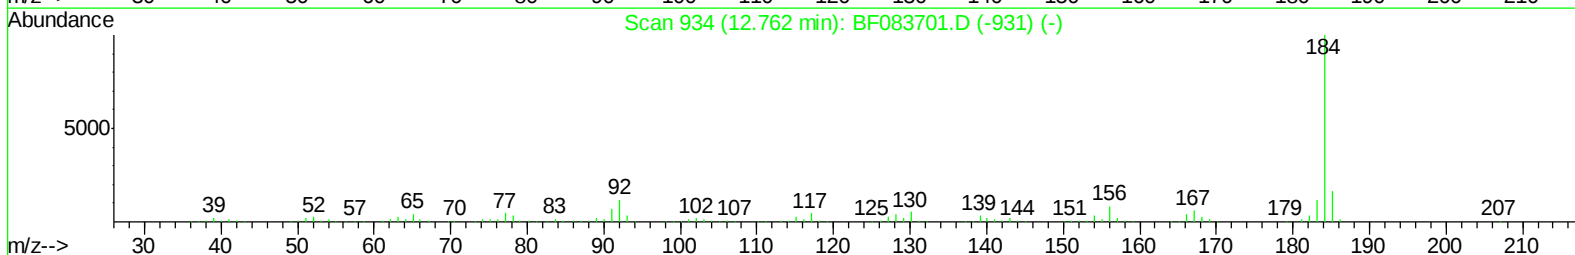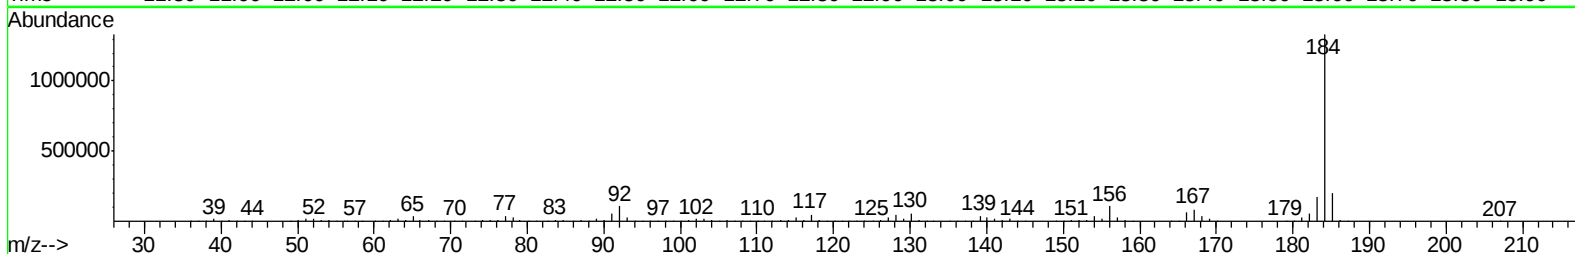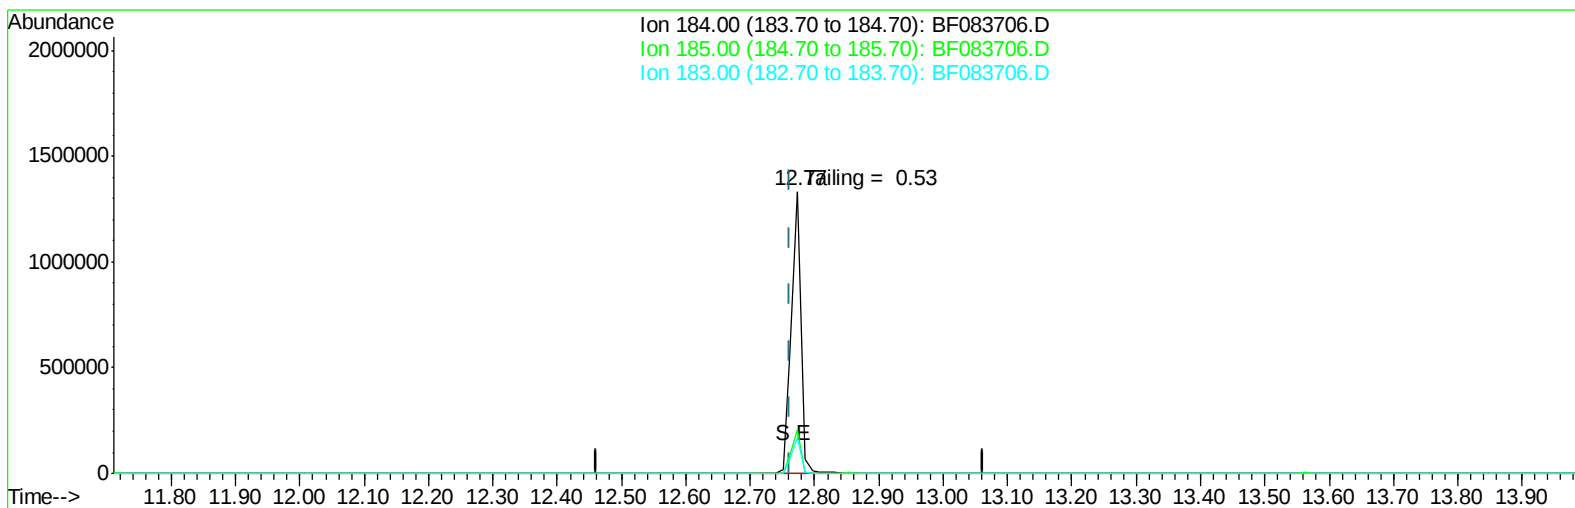

TIC: BF083706.D

(76) Benzidine

12.774min (+0.011) 96056.06ng

response 1381313

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.44
183.00	11.20	12.94
0.00	0.00	0.00