


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121115\
 Data File : BF083706.D
 Acq On : 11 Dec 2015 20:32
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 11 19:24:37 2015

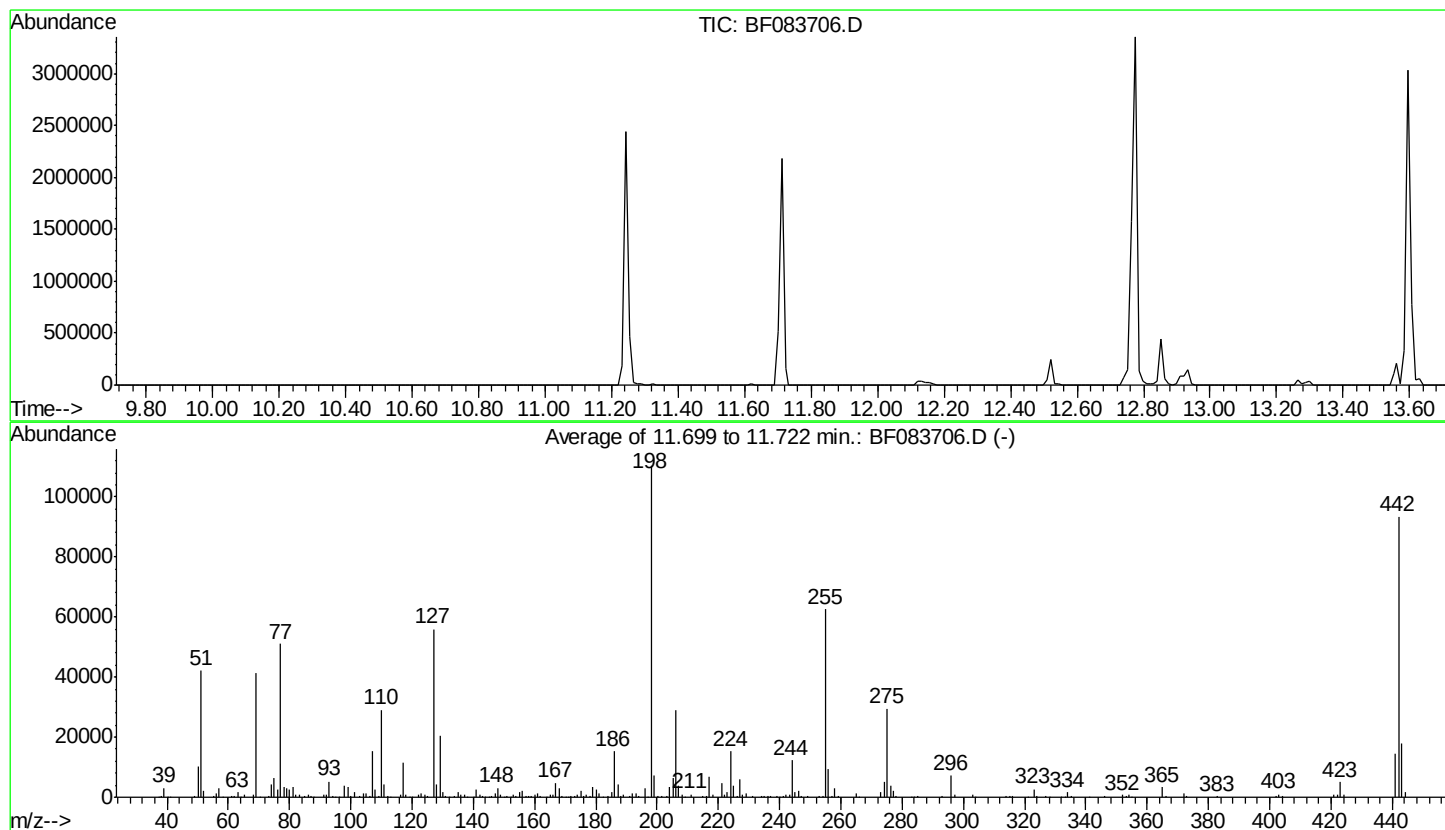

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	42104	PASS
68	69	0.00	2	1.9	796	PASS
69	198	0.00	100	37.4	41302	PASS
70	69	0.00	2	0.4	179	PASS
127	198	10	80	50.6	55883	PASS
197	198	0.00	2	0.1	136	PASS
198	198	100	100	100.0	110363	PASS
199	198	5	9	6.7	7357	PASS
275	198	10	60	26.8	29534	PASS
365	198	1	100	2.9	3238	PASS
441	442	0.01	24	15.6	14611	PASS
442	198	50	100	84.6	93405	PASS
443	442	15	24	19.4	18112	PASS