


Data Path : Z:\HPCHEM1\BNA F\Data\BF121117\
 Data File : BF101277.D
 Acq On : 11 Dec 2017 9:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 08 18:17:31 2017

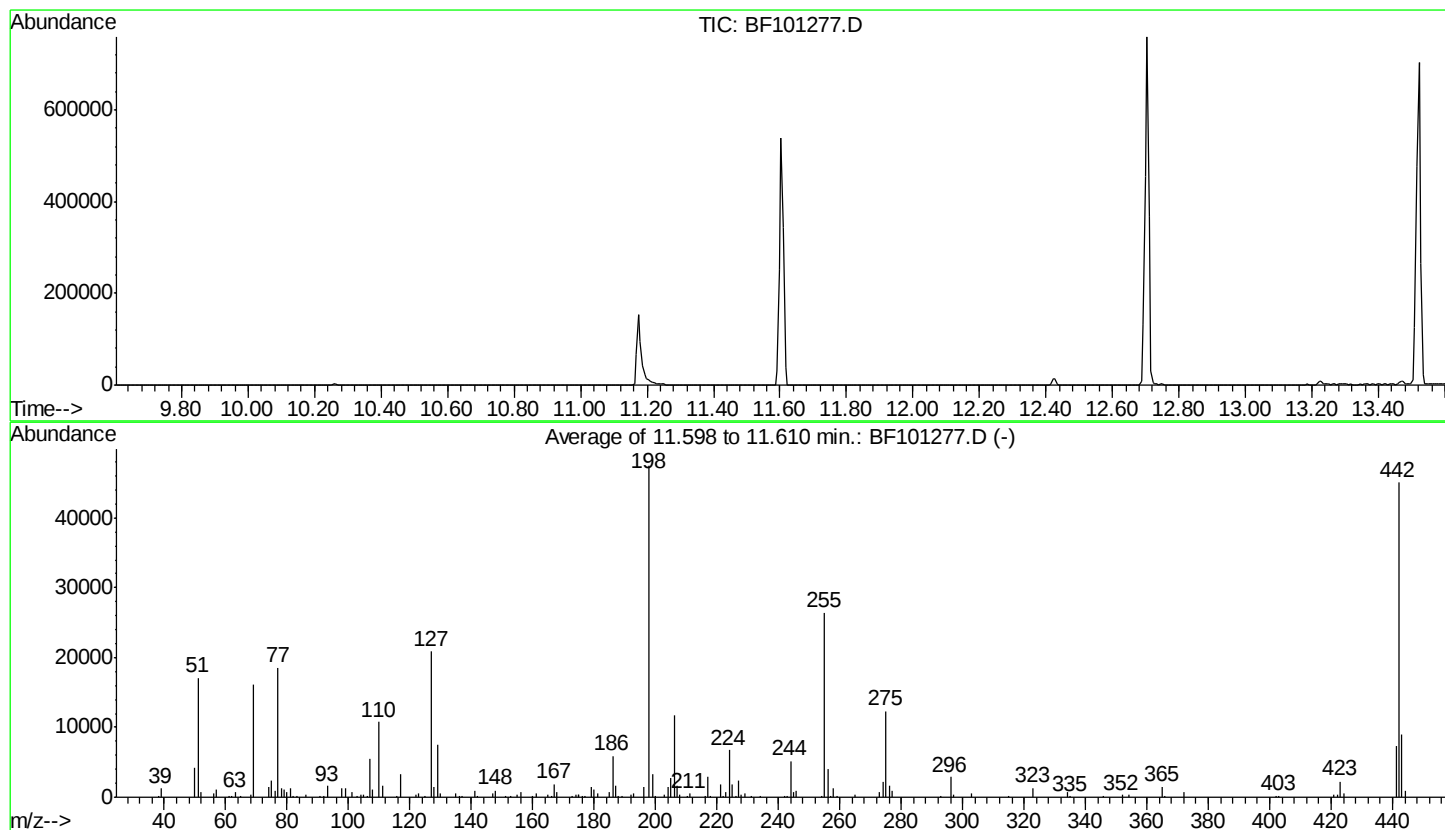

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	17100	PASS
68	69	0.00	2	1.8	295	PASS
69	198	0.00	100	33.8	16043	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	20850	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47474	PASS
199	198	5	9	6.9	3278	PASS
275	198	10	60	25.9	12281	PASS
365	198	1	100	3.1	1488	PASS
441	443	0.01	100	82.4	7400	PASS
442	198	50	100	94.9	45039	PASS
443	442	15	24	19.9	8979	PASS