
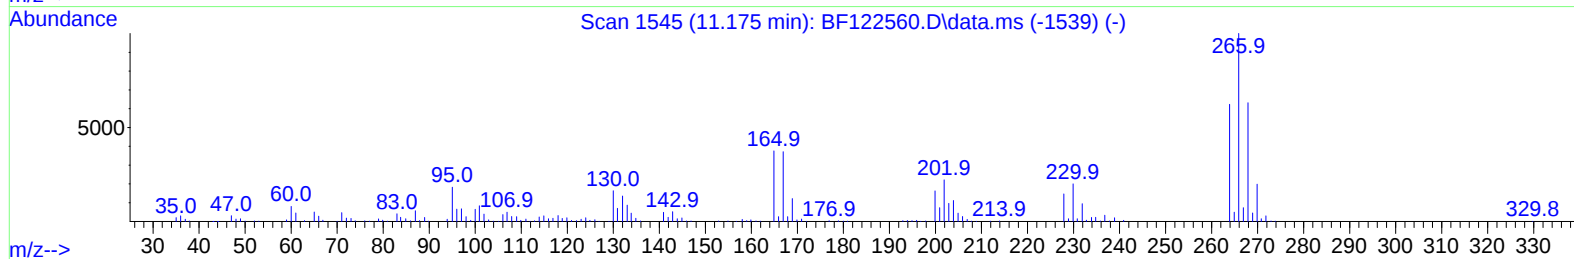
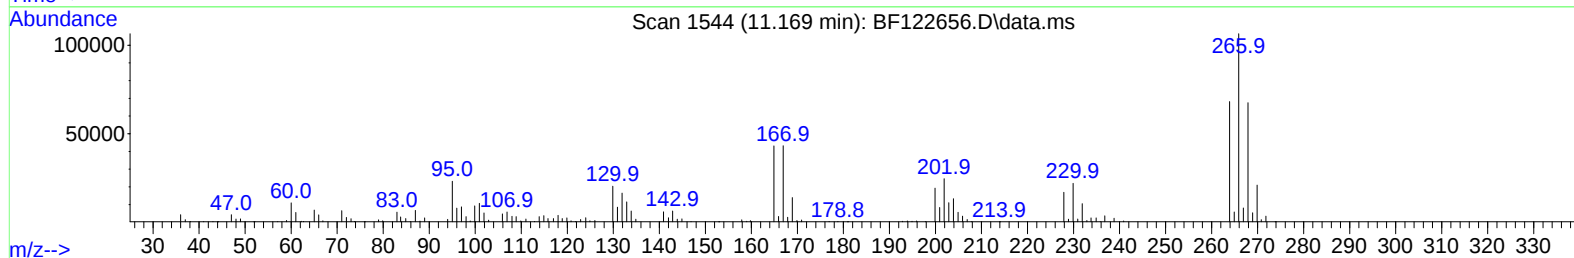


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121120\
Data File : BF122656.D
Acq On : 11 Dec 2020 10:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 06:46:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

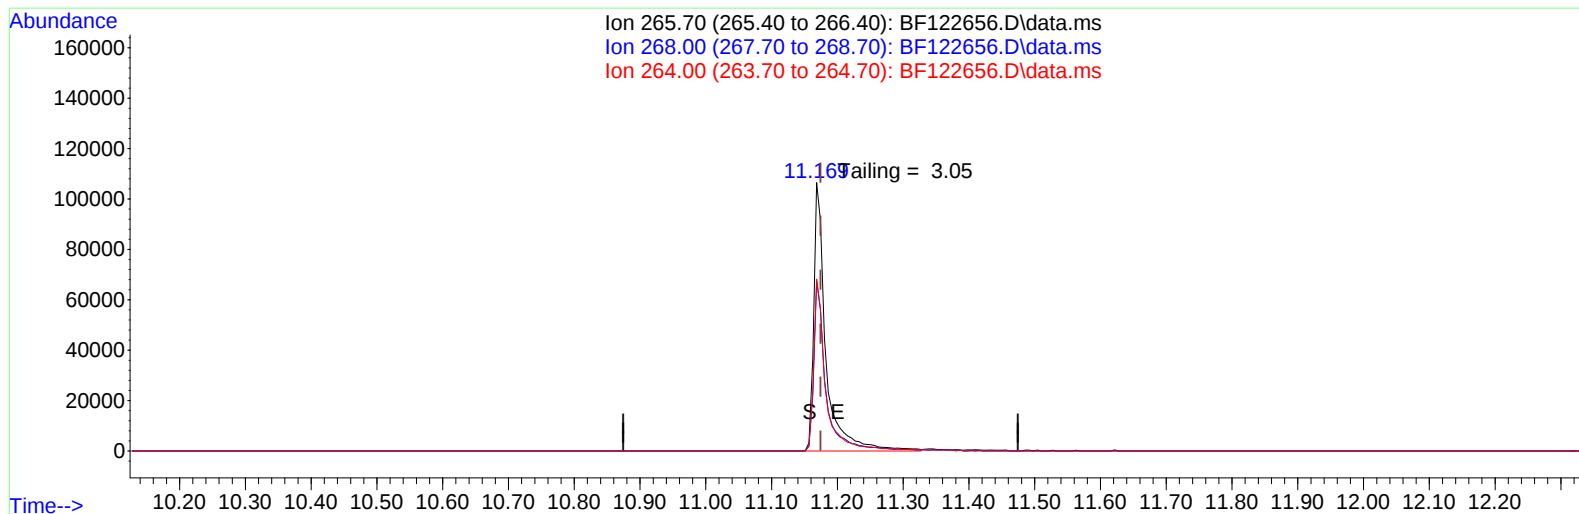

TIC: BF122656.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 47585.78 ng

response 138229

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.39
264.00	62.30	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121120\
Data File : BF122656.D
Acq On : 11 Dec 2020 10:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 06:46:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

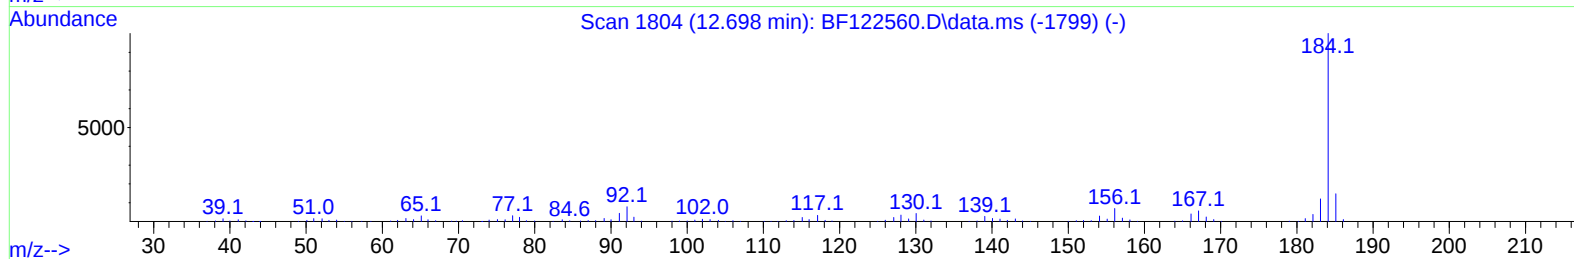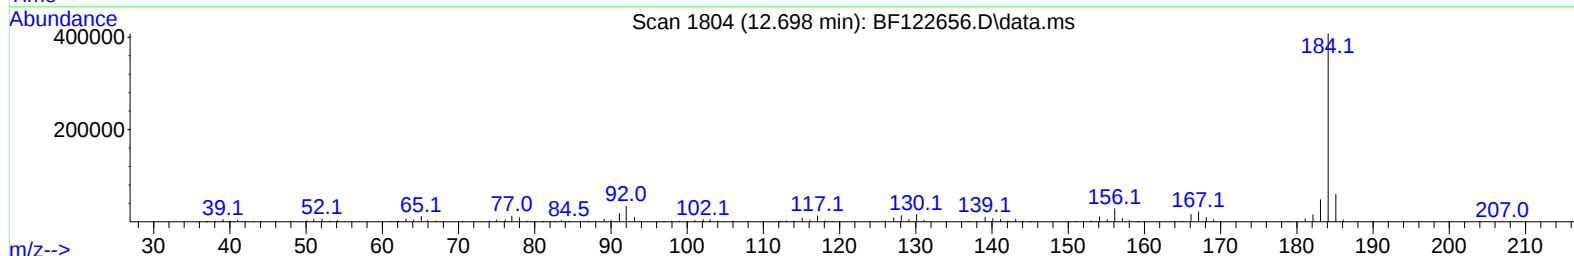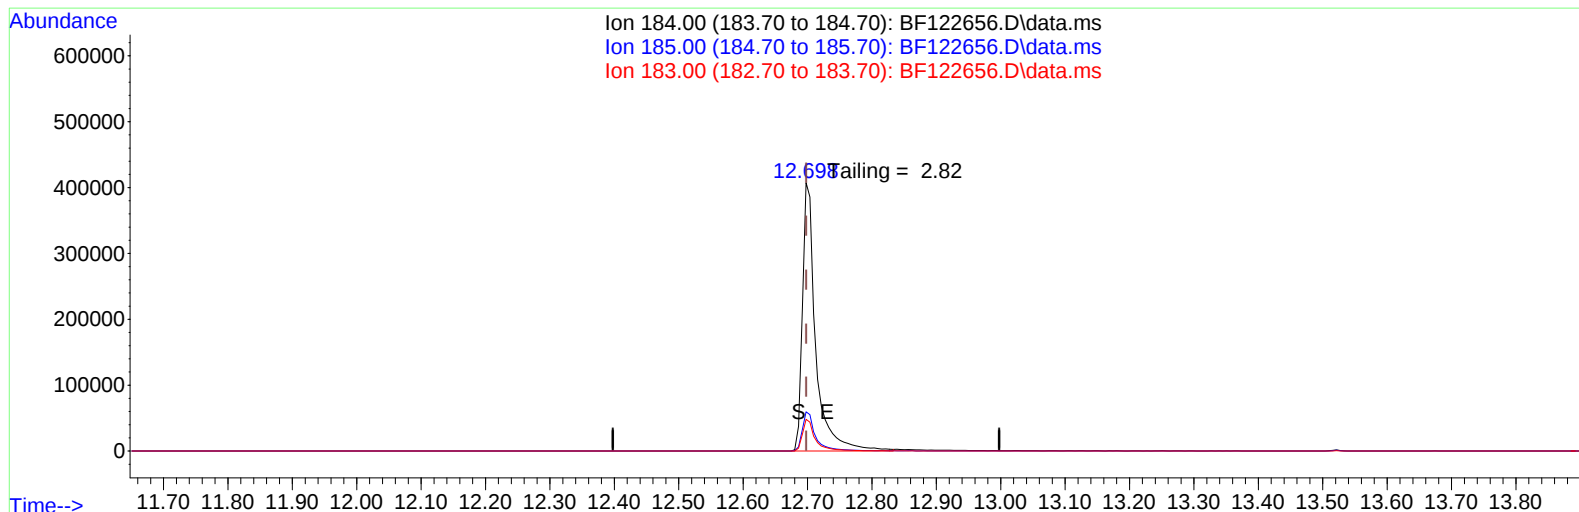

TIC: BF122656.D\data.ms

(77) Benzidine

12.698min (-0.000) 0.00 ng

response 595333

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.64
183.00	12.10	11.81
0.00	0.00	0.00