


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121120\
 Data File : BF122656.D
 Acq On : 11 Dec 2020 10:28
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 07 12:08:49 2020

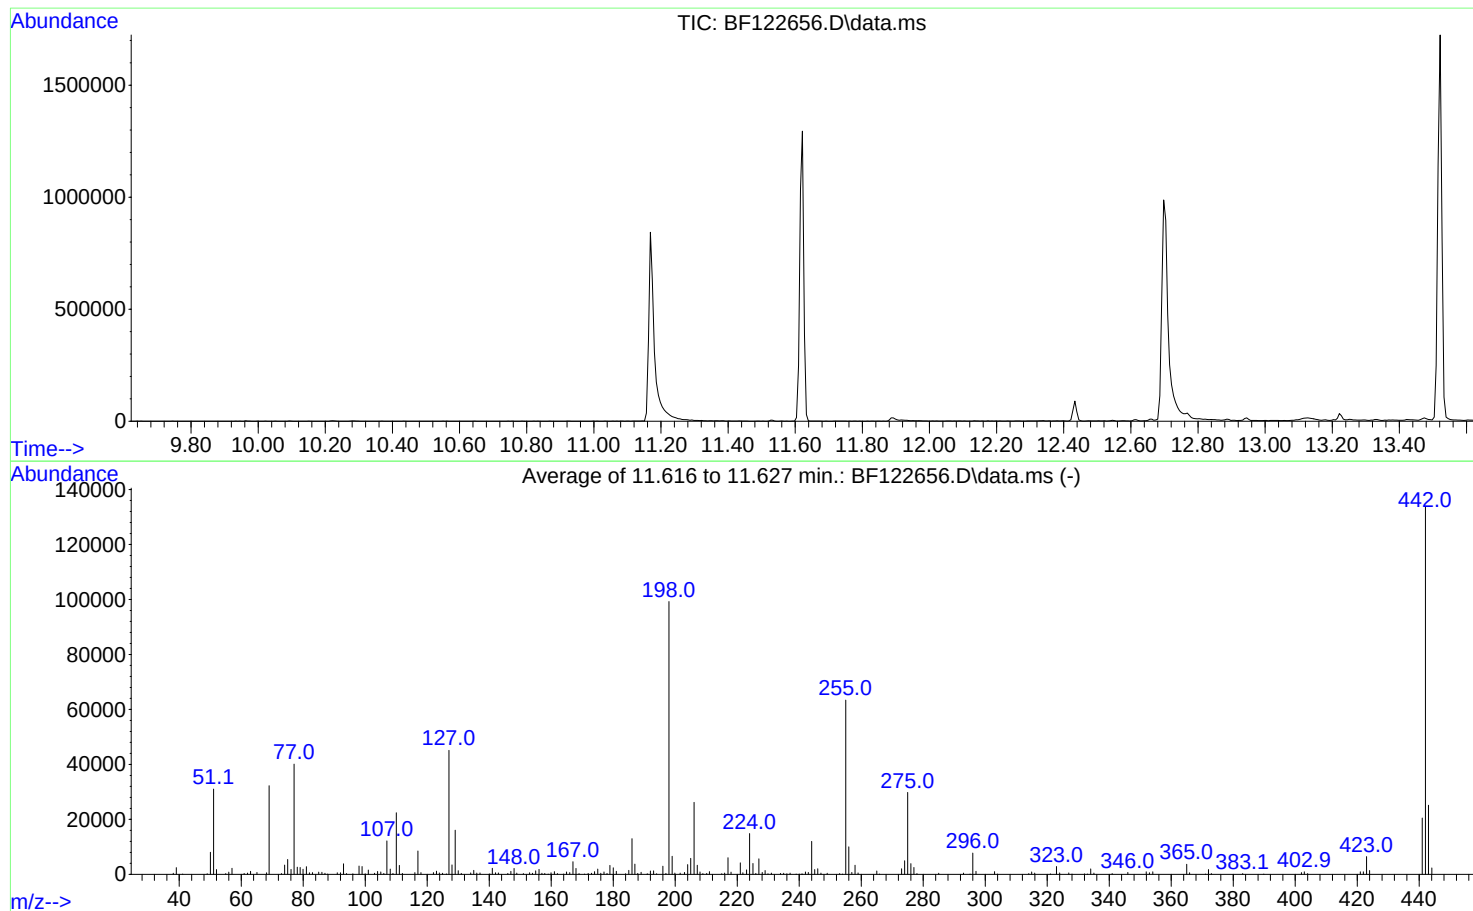

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	31053	PASS
68	69	0.00	2	1.8	586	PASS
69	198	0.00	100	32.5	32231	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.5	45122	PASS
197	198	0.00	2	0.3	346	PASS
198	198	100	100	100.0	99227	PASS
199	198	5	9	6.6	6584	PASS
275	198	10	60	30.0	29778	PASS
365	198	1	100	3.7	3675	PASS
441	198	0.01	100	20.6	20487	PASS
442	442	100	100	100.0	133819	PASS
443	442	15	24	18.8	25133	PASS