
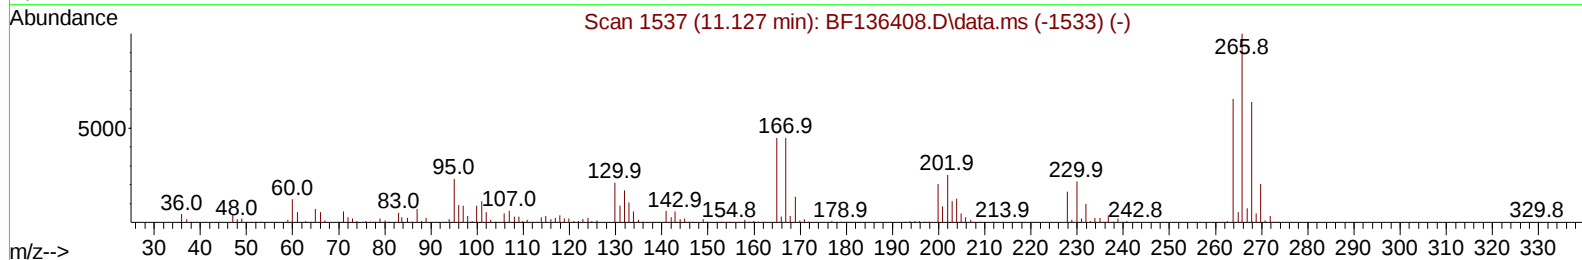
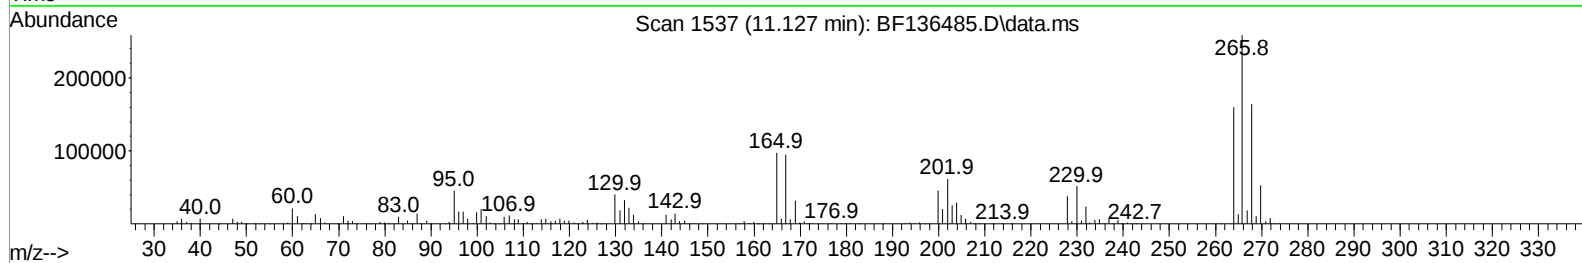


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121123\
Data File : BF136485.D
Acq On : 11 Dec 2023 12:19
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 00:34:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

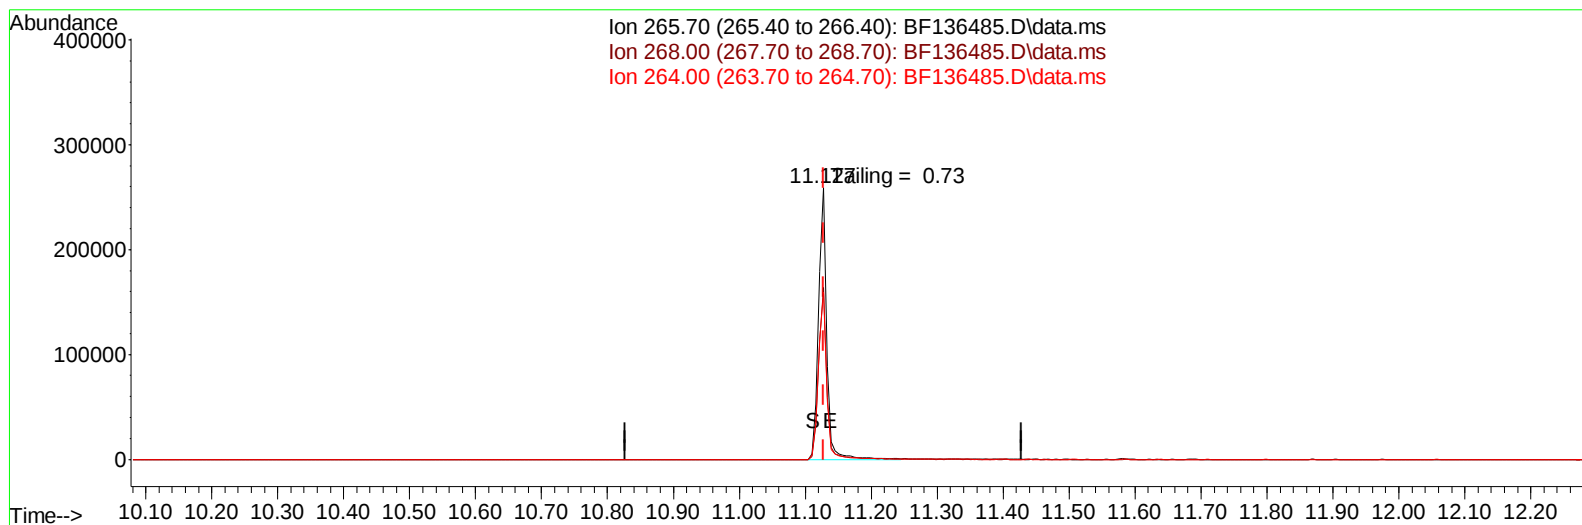

TIC: BF136485.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.000) 22410.94 ng

response 227073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.38
264.00	65.30	61.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121123\
Data File : BF136485.D
Acq On : 11 Dec 2023 12:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 00:34:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

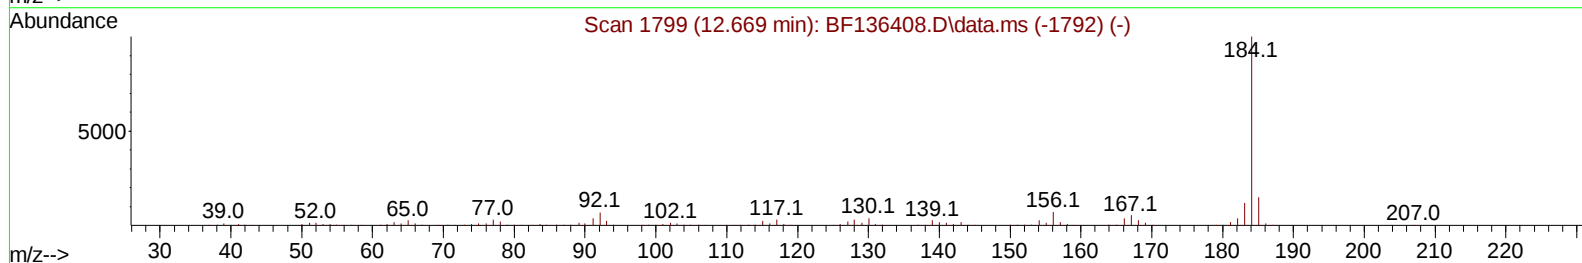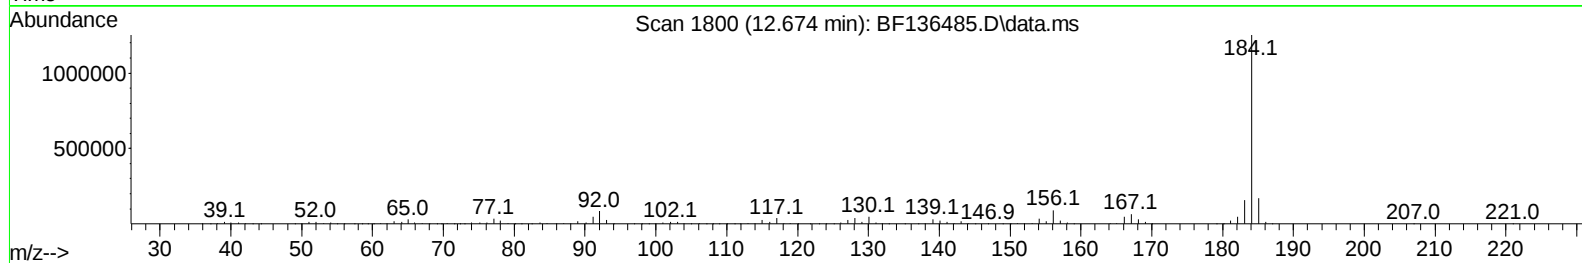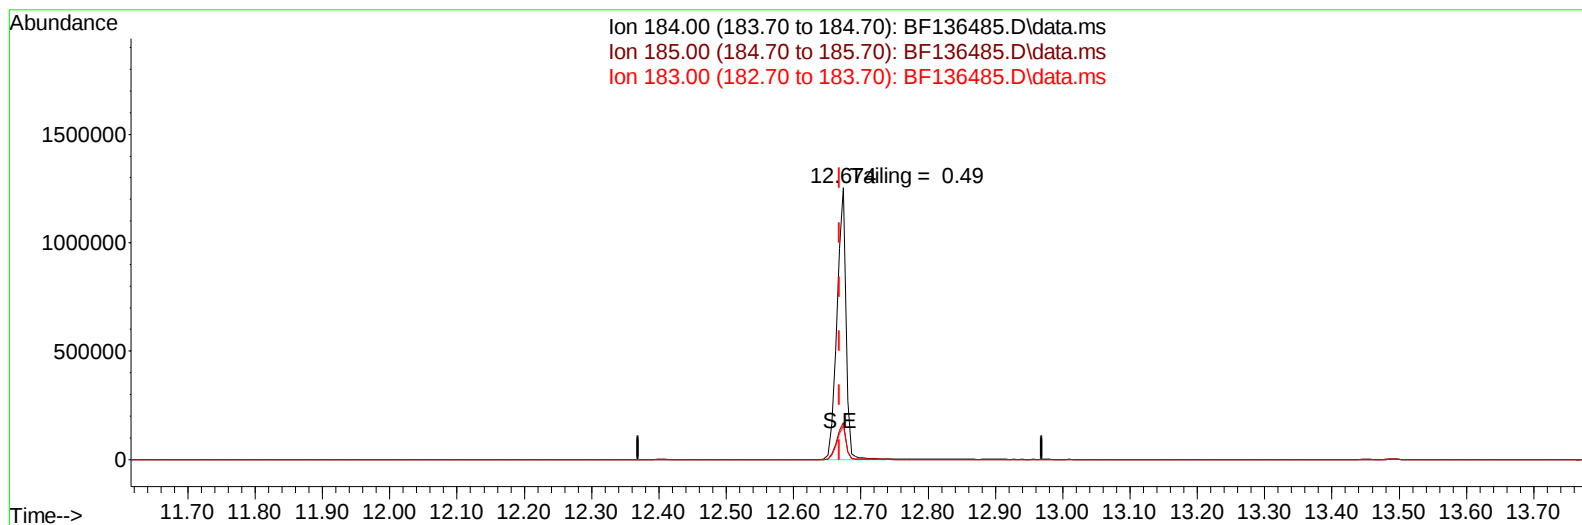

TIC: BF136485.D\data.ms

(77) Benzidine**12.674min (+ 0.005) 1694.10 ng****response 1154853**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.49
183.00	11.70	12.41
0.00	0.00	0.00