

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121123\
 Data File : BF136494.D
 Acq On : 11 Dec 2023 17:11
 Operator : CG\JU
 Sample : 05691-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-LINDEN

Quant Time: Dec 11 17:39:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 06 09:40:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.792	152	125680	20.000	ng	-0.01
21) Naphthalene-d8	8.069	136	511438	20.000	ng	-0.01
39) Acenaphthene-d10	9.828	164	264782	20.000	ng	-0.01
64) Phenanthrene-d10	11.316	188	490468	20.000	ng	-0.01
76) Chrysene-d12	13.968	240	253948	20.000	ng	-0.01
86) Perylene-d12	15.451	264	249195	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.440	112	690913	81.187	ng	0.00
7) Phenol-d6	6.439	99	864530	81.423	ng	0.00
23) Nitrobenzene-d5	7.351	82	527051	55.711	ng	-0.02
42) 2,4,6-Tribromophenol	10.622	330	268898	82.363	ng	-0.01
45) 2-Fluorobiphenyl	9.151	172	1054940	54.364	ng	-0.01
79) Terphenyl-d14	12.916	244	1041041	54.032	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121123\
Data File : BF136494.D
Acq On : 11 Dec 2023 17:11
Operator : CG\JU
Sample : 05691-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-LINDEN

Quant Time: Dec 11 17:39:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration




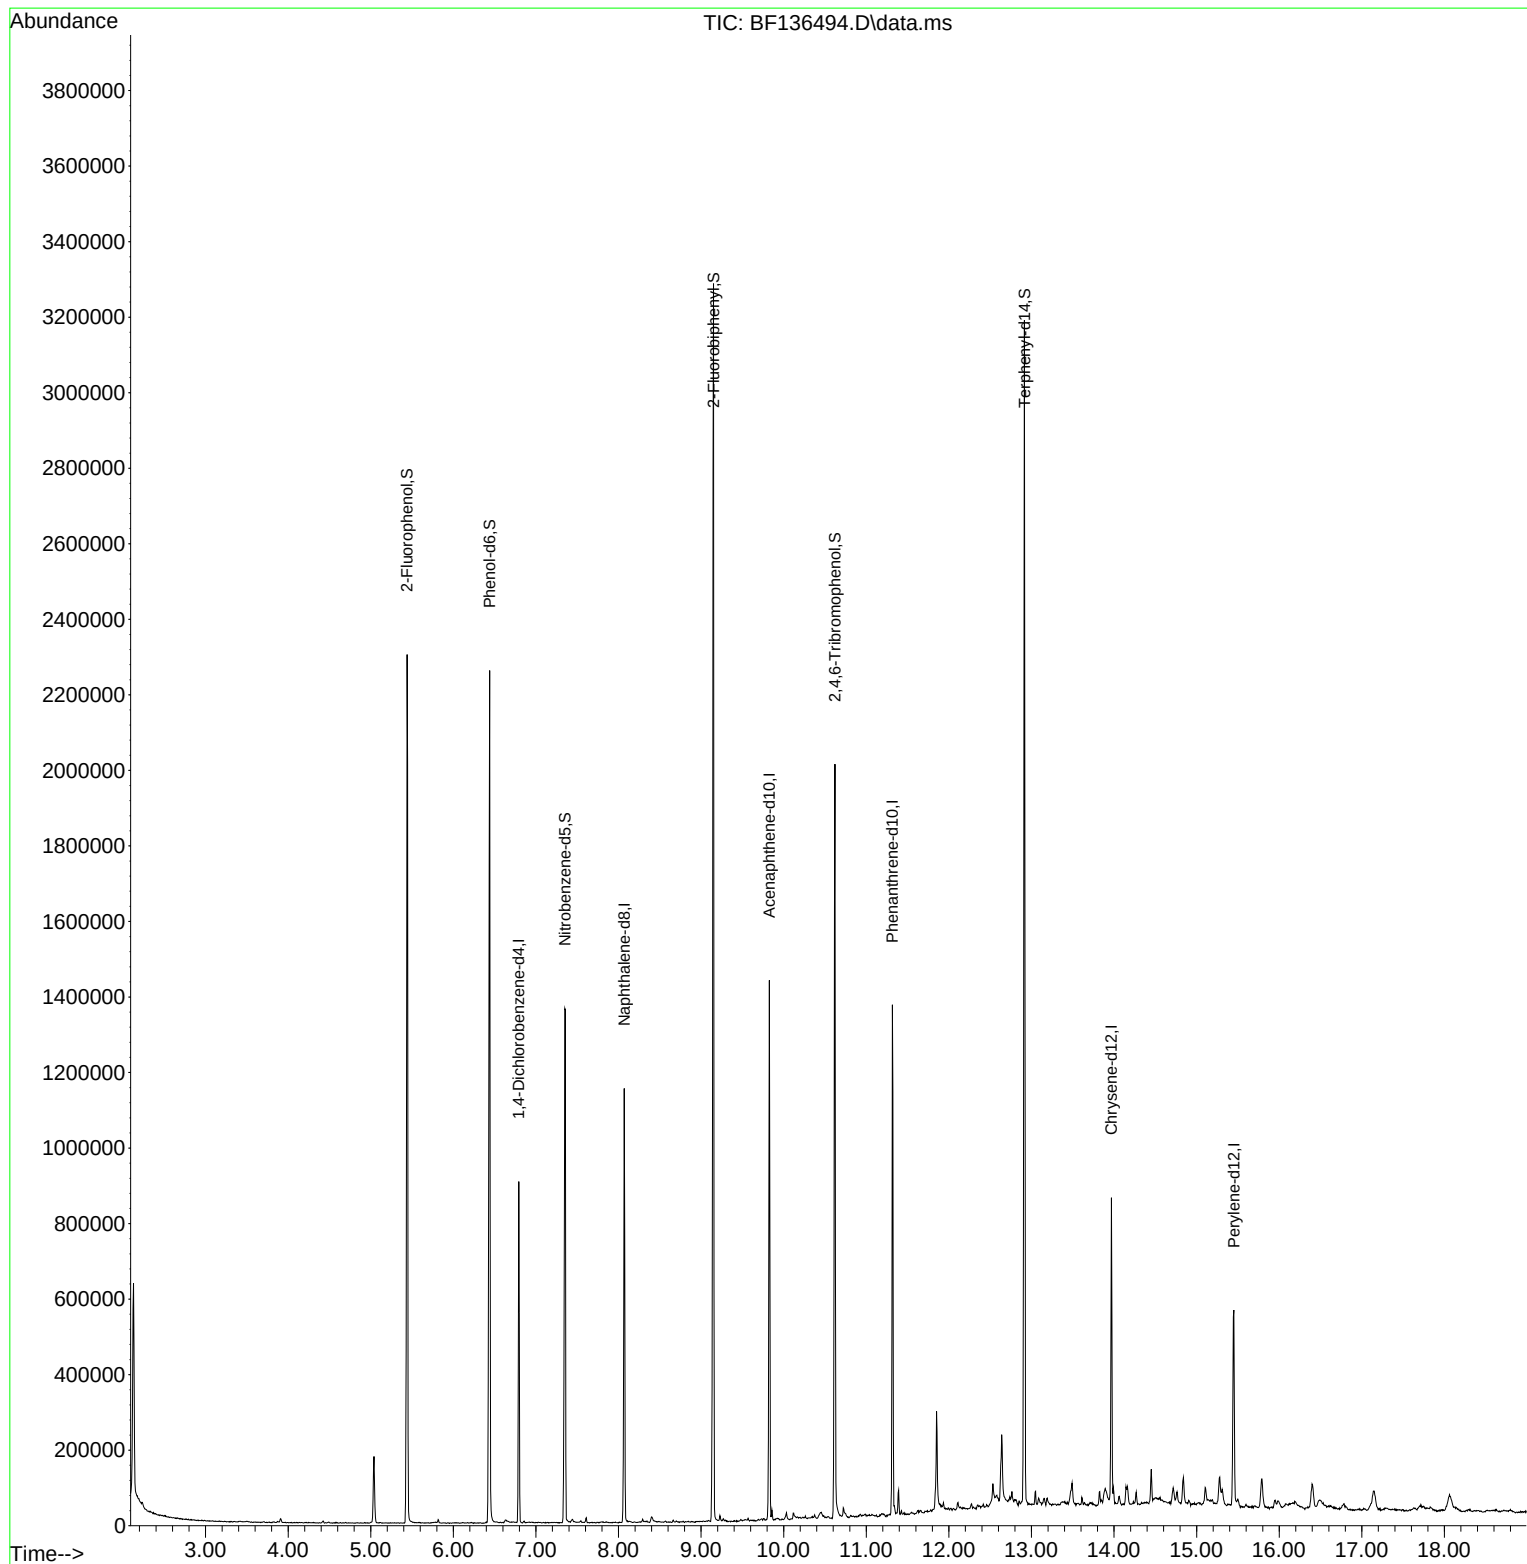


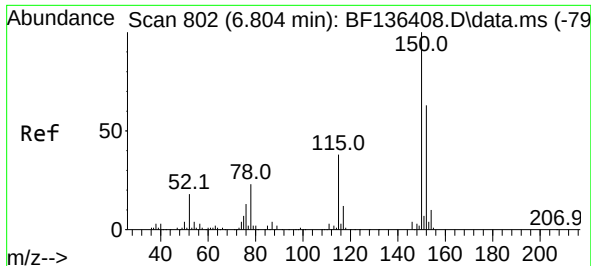

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.792 min Scan# 802
 Delta R.T. -0.012 min
 Lab File: BF136494.D
 Acq: 11 Dec 2023 17:11




Instrument :
 BNA_F
 ClientSampleId :
 SP-LINDEN


Tgt Ion:152 Resp: 125680
 Ion Ratio Lower Upper
 152 100
 150 158.9 126.4 189.6
 115 62.3 48.2 72.4

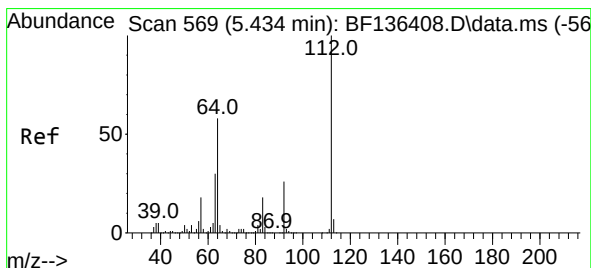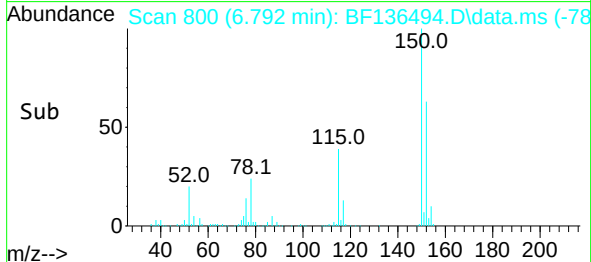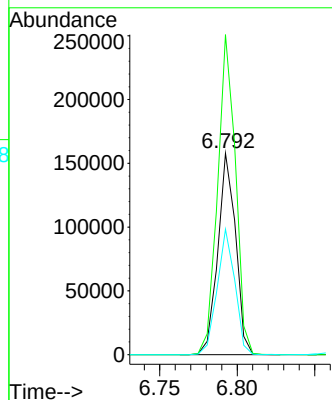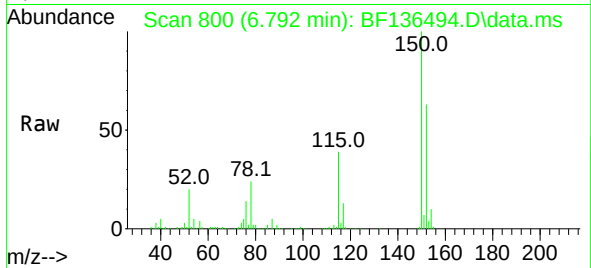

#5
 2-Fluorophenol
 Concen: 81.187 ng
 RT: 5.440 min Scan# 570
 Delta R.T. 0.006 min
 Lab File: BF136494.D
 Acq: 11 Dec 2023 17:11

Tgt Ion:112 Resp: 690913
 Ion Ratio Lower Upper
 112 100
 64 58.0 46.5 69.7
 63 30.1 23.9 35.9


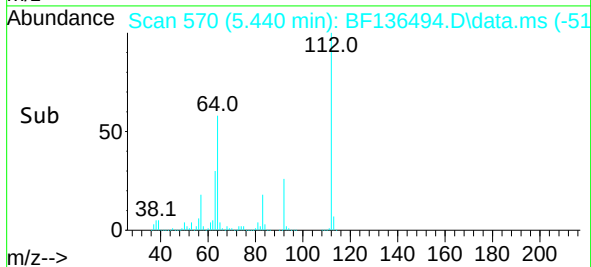
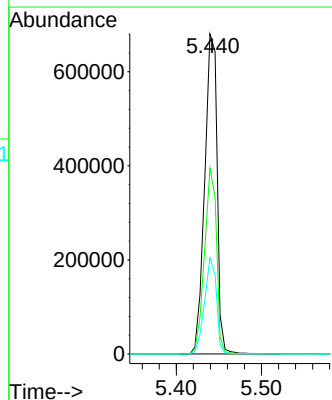
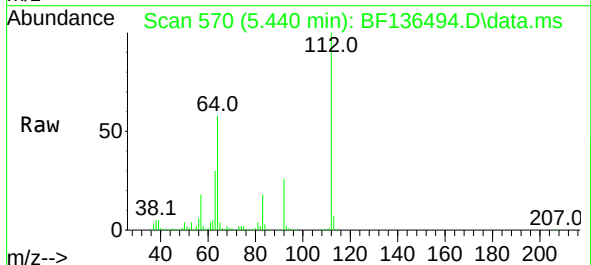


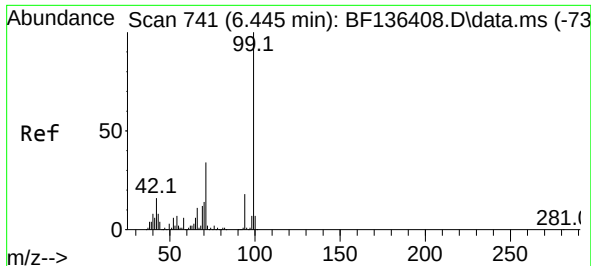

#7
Phenol-d6
Concen: 81.423 ng
RT: 6.439 min Scan# 741
Delta R.T. -0.006 min
Lab File: BF136494.D
Acq: 11 Dec 2023 17:11




Instrument :
BNA_F
ClientSampleId :
SP-LINDEN


Tgt Ion: 99 Resp: 864530
Ion Ratio Lower Upper
99 100
42 15.2 12.8 19.2
71 33.4 27.0 40.4

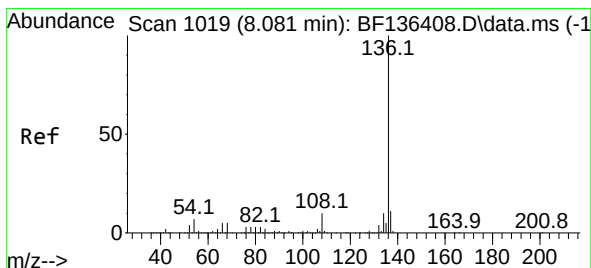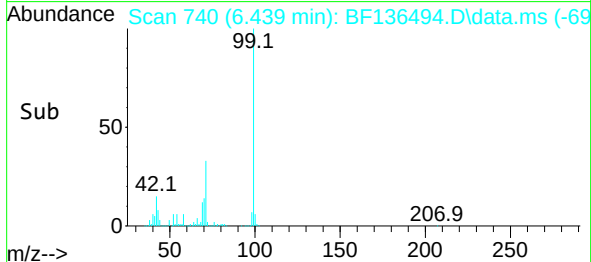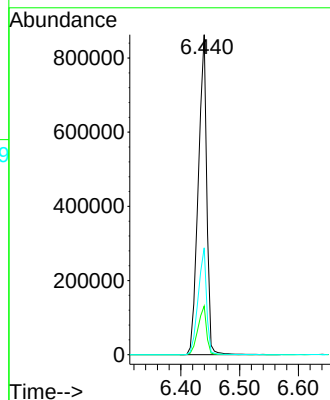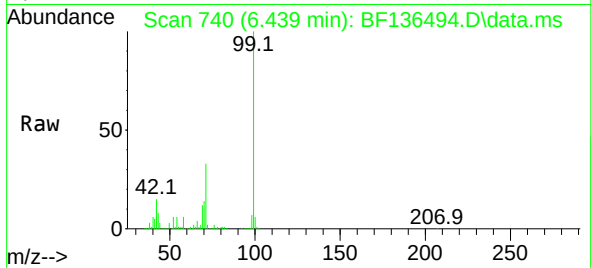

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.069 min Scan# 1017
Delta R.T. -0.012 min
Lab File: BF136494.D
Acq: 11 Dec 2023 17:11

Tgt Ion: 136 Resp: 511438
Ion Ratio Lower Upper
136 100
137 10.7 8.6 12.8
54 7.2 5.7 8.5
68 5.1 4.0 6.0

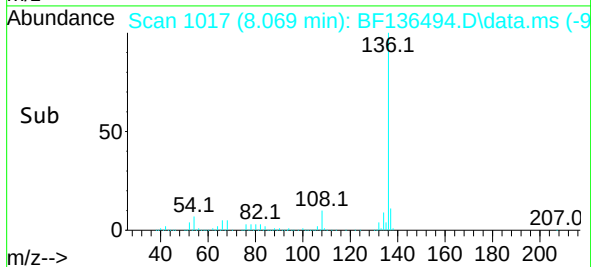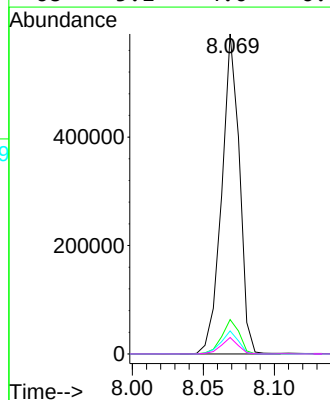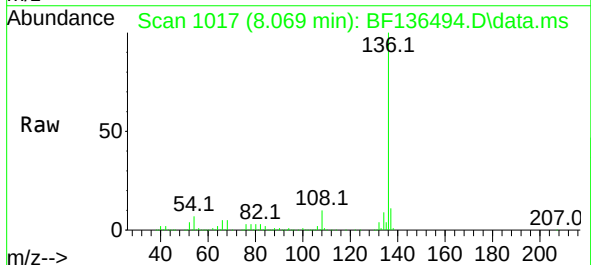

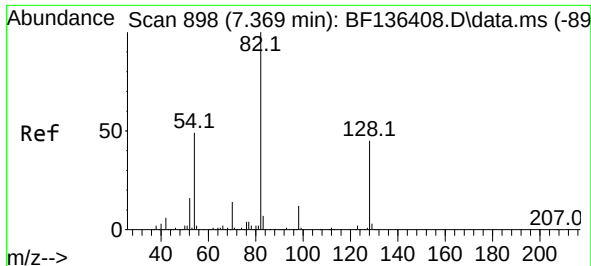

#23

Nitrobenzene-d5

Concen: 55.711 ng

RT: 7.351 min Scan# 89

Delta R.T. -0.018 min

Lab File: BF136494.D

Acq: 11 Dec 2023 17:11

Instrument :

BNA_F

ClientSampleId :

SP-LINDEN





Tgt Ion: 82 Resp: 527051

Ion Ratio Lower Upper

82 100

128 44.6 36.3 54.5

54 48.1 39.0 58.6

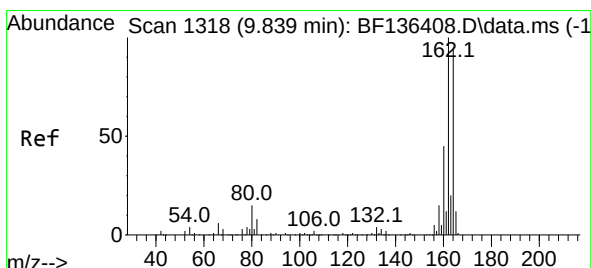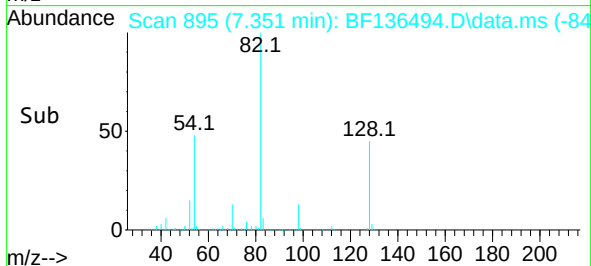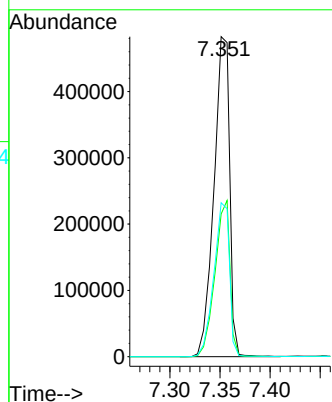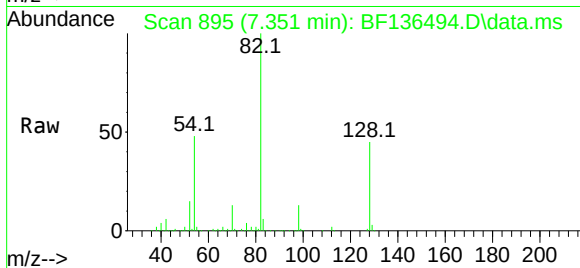

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.828 min Scan# 1316

Delta R.T. -0.012 min

Lab File: BF136494.D

Acq: 11 Dec 2023 17:11




Tgt Ion:164 Resp: 264782


Ion Ratio Lower Upper

164 100

162 103.1 84.4 126.6

160 45.5 37.6 56.4

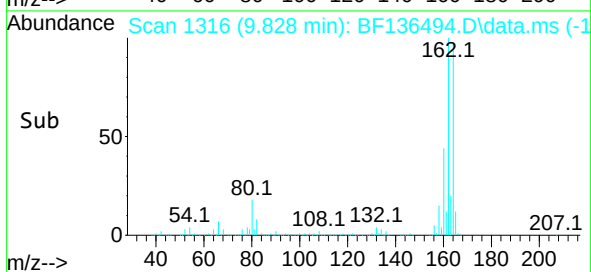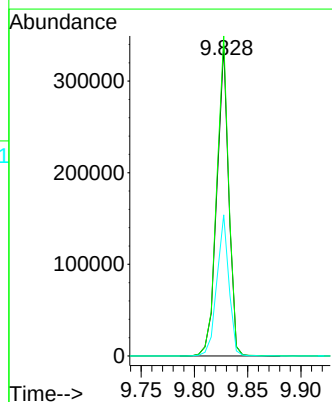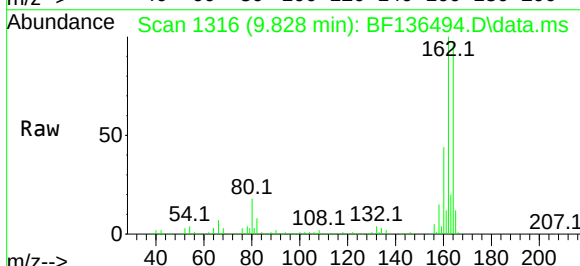

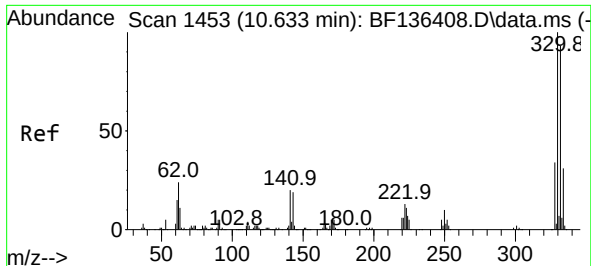

#42

2,4,6-Tribromophenol

Concen: 82.363 ng

RT: 10.622 min Scan# 1451

Delta R.T. -0.012 min

Lab File: BF136494.D


Acq: 11 Dec 2023 17:11

Instrument :

BNA_F

ClientSampleId :

SP-LINDEN

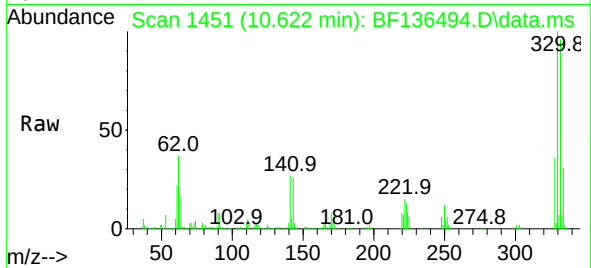




Tgt Ion:330 Resp: 268898

Ion Ratio Lower Upper

330 100

332 96.1 76.4 114.6

141 29.2 23.4 35.2

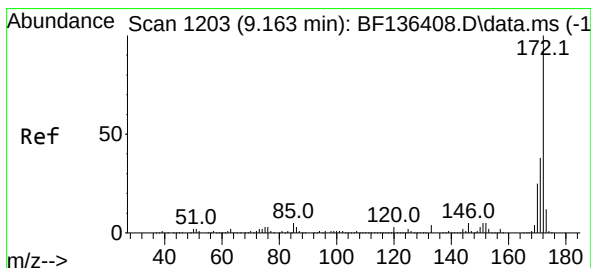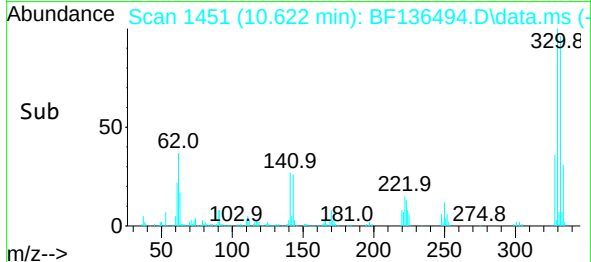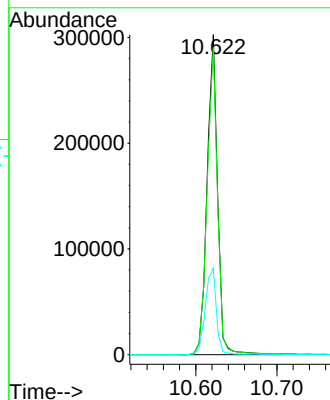

#45

2-Fluorobiphenyl

Concen: 54.364 ng

RT: 9.151 min Scan# 1201

Delta R.T. -0.012 min

Lab File: BF136494.D

Acq: 11 Dec 2023 17:11




Tgt Ion:172 Resp: 1054940


Ion Ratio Lower Upper

172 100

171 36.6 30.5 45.7

170 24.1 19.9 29.9


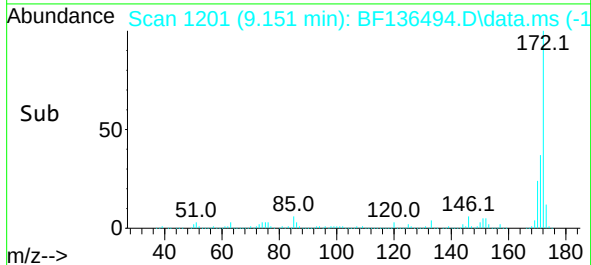
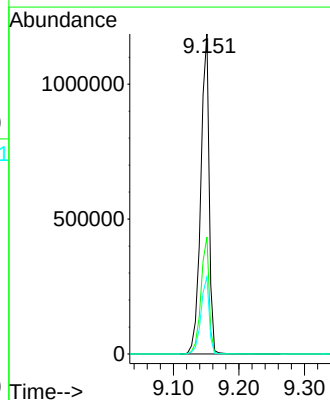
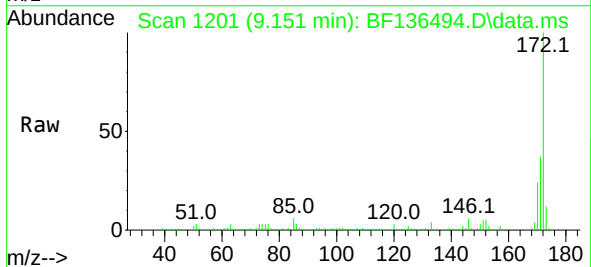


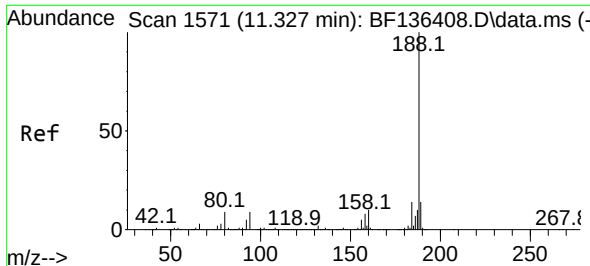

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.316 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF136494.D
Acq: 11 Dec 2023 17:11




Instrument :
BNA_F
ClientSampleId :
SP-LINDEN


Tgt Ion:188 Resp: 490468
Ion Ratio Lower Upper
188 100
94 9.1 7.2 10.8
80 10.2 7.2 10.8

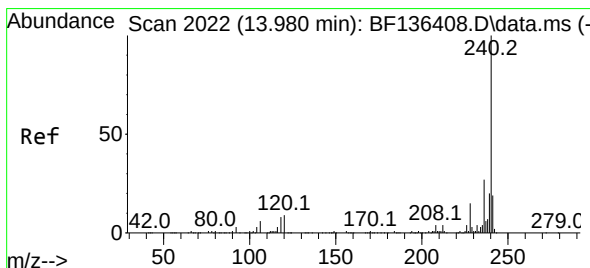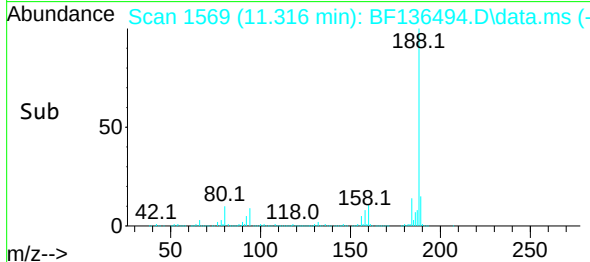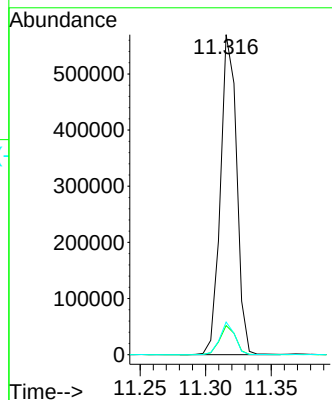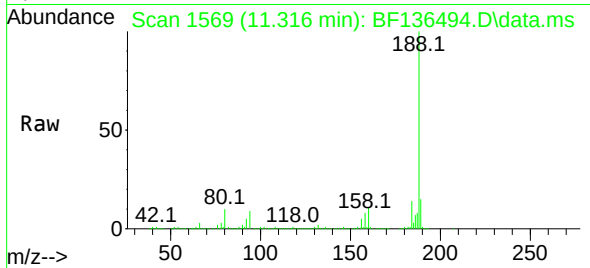

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.968 min Scan# 2020
Delta R.T. -0.012 min
Lab File: BF136494.D
Acq: 11 Dec 2023 17:11


Tgt Ion:240 Resp: 253948
Ion Ratio Lower Upper
240 100
120 10.3 7.3 10.9
236 25.2 21.3 31.9

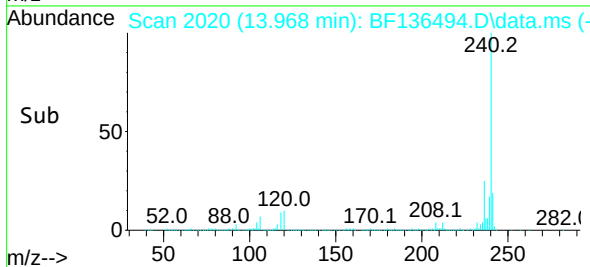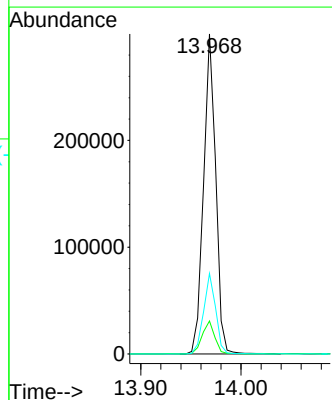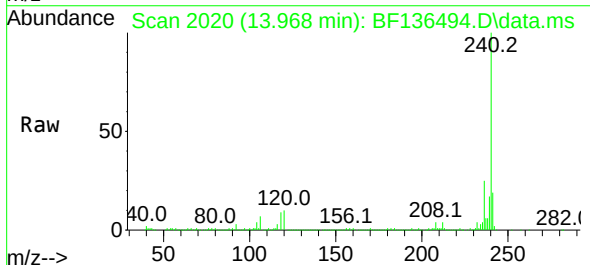

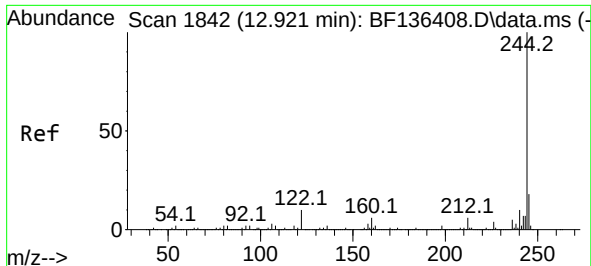




#79
 Terphenyl-d14
 Concen: 54.032 ng
 RT: 12.916 min Scan# 1841
 Delta R.T. -0.006 min
 Lab File: BF136494.D
 Acq: 11 Dec 2023 17:11

Instrument :
 BNA_F
 ClientSampleId :
 SP-LINDEN

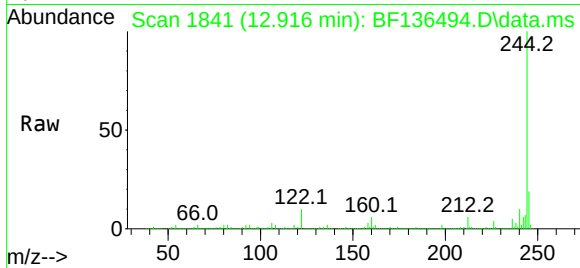

Tgt Ion:244 Resp: 1041041

Ion	Ratio	Lower	Upper
244	100		
212	6.4	5.0	7.4
122	9.9	8.3	12.5

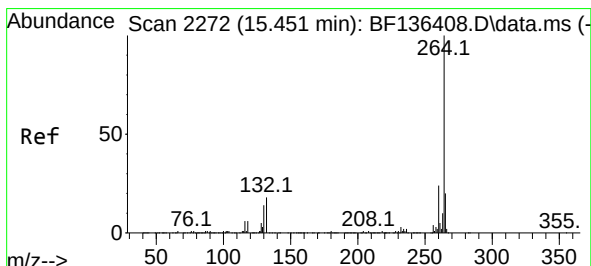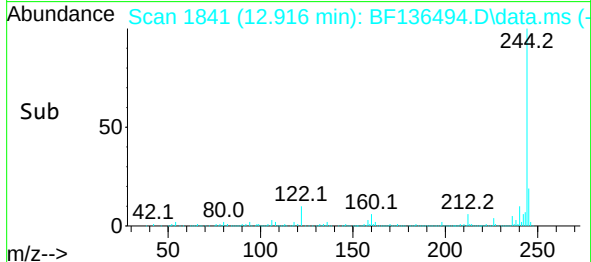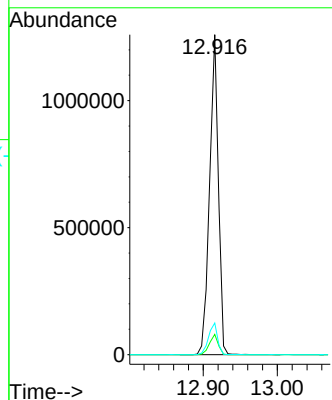

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.451 min Scan# 2272
 Delta R.T. -0.000 min
 Lab File: BF136494.D
 Acq: 11 Dec 2023 17:11

Tgt Ion:264 Resp: 249195

Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.2	28.8
265	21.1	15.9	23.9

